

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048600.D
 Acq On : 12 Nov 2024 00:57
 Operator : RC/JU
 Sample : PB164732BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK732

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	31	rVB	58558	81168	1.87%	0.187%
2	3.540	90	94	114	rBV	656861	1093168	25.14%	2.518%
3	3.857	145	148	153	rVB2	9105	13761	0.32%	0.032%
4	6.840	648	655	672	rBV	708042	1217228	27.99%	2.804%
5	6.993	675	681	694	rVV	602345	973605	22.39%	2.243%
6	7.193	708	715	734	rBV	785304	1284991	29.55%	2.960%
7	7.657	786	794	804	rBV	545100	879091	20.21%	2.025%
8	8.375	909	916	935	rBV	868233	1517377	34.89%	3.495%
9	8.816	984	991	1005	rBV	678745	1165454	26.80%	2.685%
10	9.534	1106	1113	1124	rBV	553800	946644	21.77%	2.181%
11	10.075	1198	1205	1216	rBV	773932	1445581	33.24%	3.330%
12	10.445	1260	1268	1276	rBV	745675	1253965	28.83%	2.889%
13	10.592	1285	1293	1315	rBV	692266	1535049	35.30%	3.536%
14	10.769	1321	1323	1329	rVB5	3525	5091	0.12%	0.012%
15	12.063	1539	1543	1548	rBV	10289	16922	0.39%	0.039%
16	13.722	1819	1825	1840	rBV	1392384	2030872	46.70%	4.678%
17	13.998	1865	1872	1888	rBV	1714934	2622468	60.30%	6.041%
18	14.304	1918	1924	1933	rBV	1060684	1629466	37.47%	3.754%
19	14.539	1957	1964	1987	rBV	343832	903130	20.77%	2.080%
20	15.304	2087	2094	2105	rBV	2183591	3191816	73.39%	7.353%
21	15.433	2110	2116	2132	rVV	492539	810400	18.63%	1.867%
22	15.539	2132	2134	2141	rVB5	13220	21441	0.49%	0.049%
23	15.863	2185	2189	2196	rBV7	7456	12920	0.30%	0.030%
24	16.404	2279	2281	2286	rVB4	4642	5502	0.13%	0.013%
25	16.545	2300	2305	2309	rBV6	6689	11637	0.27%	0.027%
26	16.574	2309	2310	2319	rVB7	3224	5969	0.14%	0.014%
27	17.051	2384	2391	2401	rBV	1350721	1927813	44.33%	4.441%
28	17.151	2401	2408	2428	rVV2	2318504	3547215	81.57%	8.171%
29	19.015	2721	2725	2730	rBV2	28730	37588	0.86%	0.087%
30	19.086	2733	2737	2742	rBV	29185	39828	0.92%	0.092%
31	19.451	2793	2799	2814	rBV	3020012	4208437	96.77%	9.695%
32	20.945	3050	3053	3057	rBV	84770	112046	2.58%	0.258%
33	21.280	3104	3110	3121	rBV2	1313235	2171548	49.93%	5.002%
34	23.991	3562	3571	3589	rVB	1795563	4348885	100.00%	10.018%
35	24.186	3596	3604	3618	rVB	902376	2341678	53.85%	5.394%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048600.D
Acq On : 12 Nov 2024 00:57
Operator : RC/JU
Sample : PB164732BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK732

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 43409754

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048600.D
Acq On : 12 Nov 2024 00:57
Operator : RC/JU
Sample : PB164732BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK732

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

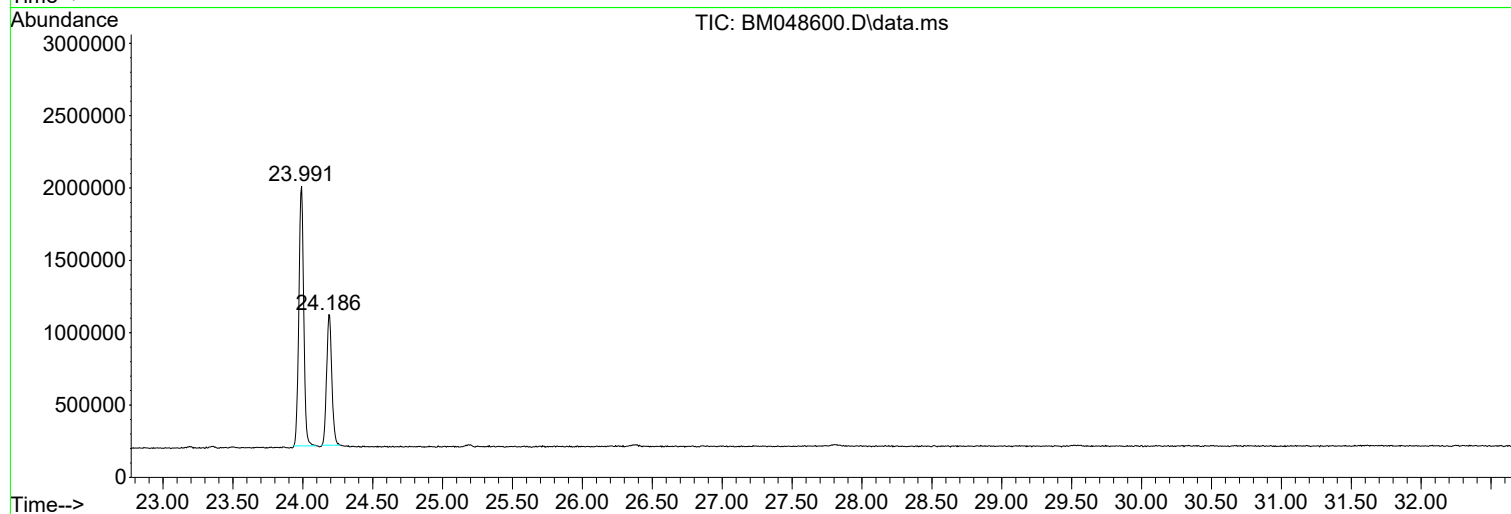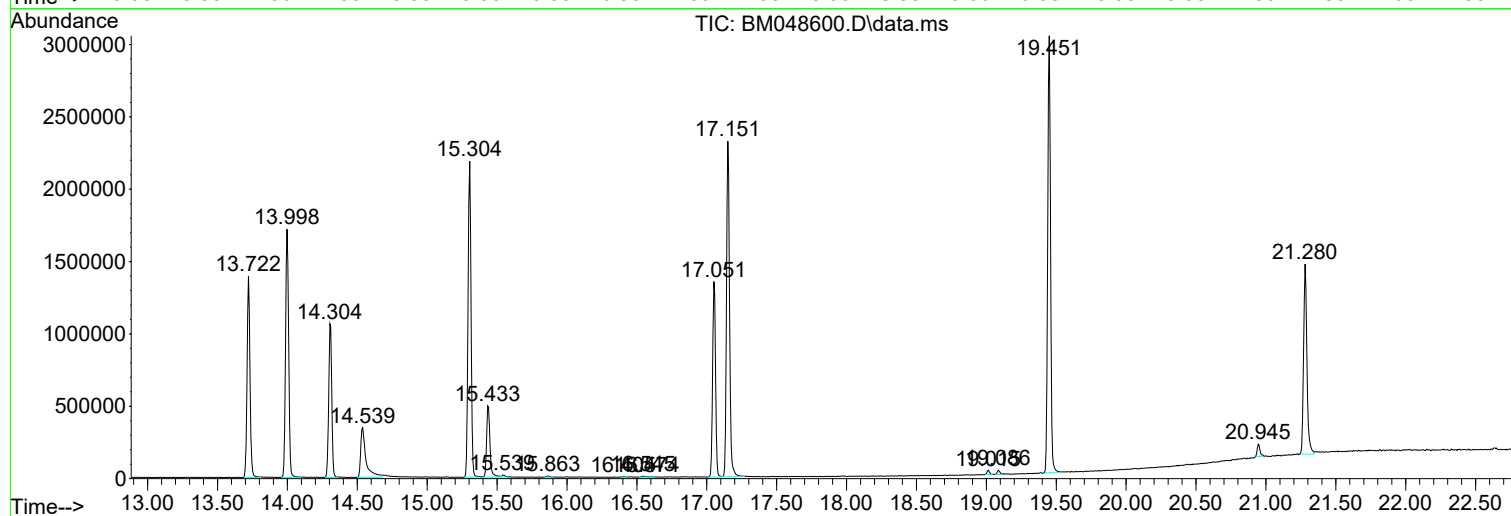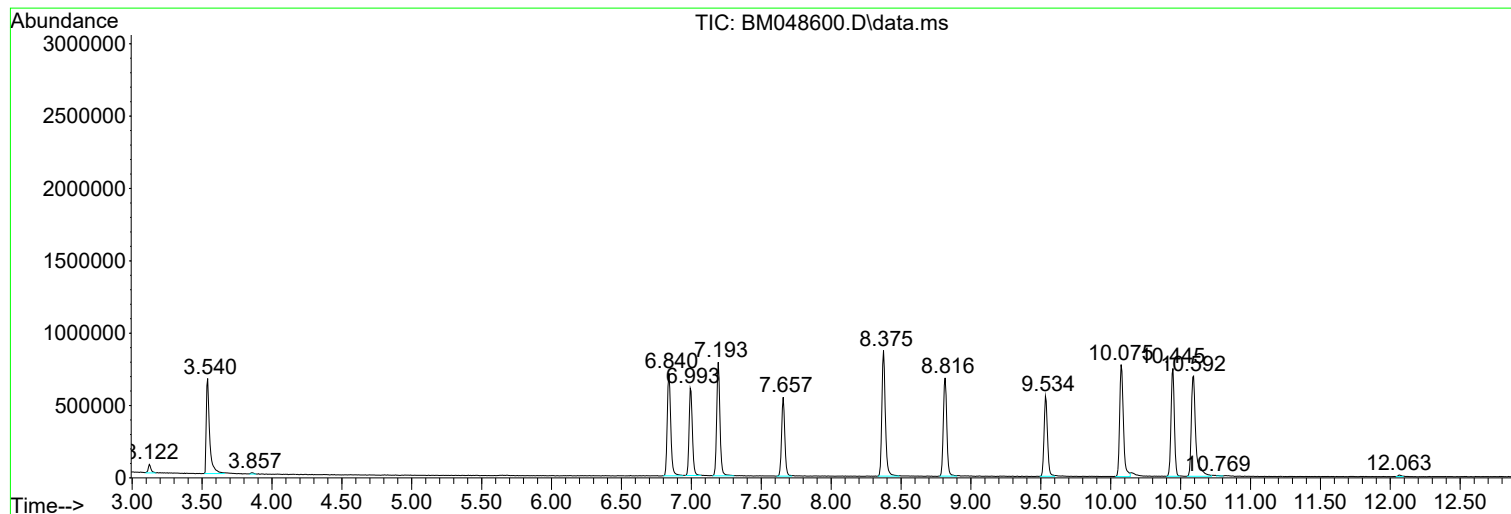

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048600.D
Acq On : 12 Nov 2024 00:57
Operator : RC/JU
Sample : PB164732BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK732

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048600.D
Acq On : 12 Nov 2024 00:57
Operator : RC/JU
Sample : PB164732BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK732

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------