

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048604.D
 Acq On : 12 Nov 2024 04:14
 Operator : RC/JU
 Sample : PB164730BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK730

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	31	rVB	51254	68721	1.74%	0.163%
2	3.540	90	94	114	rBV	582527	977406	24.73%	2.314%
3	3.857	145	148	155	rVB3	9325	13775	0.35%	0.033%
4	6.840	649	655	670	rBV	624077	1088625	27.55%	2.577%
5	6.992	675	681	696	rVV	537147	879336	22.25%	2.082%
6	7.192	708	715	729	rBV	691031	1141513	28.88%	2.702%
7	7.657	787	794	806	rBV	633304	1041921	26.36%	2.467%
8	8.375	906	916	929	rBV	785875	1363981	34.51%	3.229%
9	8.816	983	991	1006	rBV	620793	1067827	27.02%	2.528%
10	9.533	1107	1113	1129	rBV	493355	851319	21.54%	2.015%
11	10.075	1198	1205	1227	rBV	711721	1356956	34.34%	3.212%
12	10.445	1261	1268	1277	rBV	876270	1496647	37.87%	3.543%
13	10.592	1285	1293	1314	rBV	602898	1370837	34.69%	3.245%
14	12.069	1536	1544	1548	rBV3	10536	20286	0.51%	0.048%
15	13.721	1818	1825	1840	rBV	1263326	1855001	46.94%	4.391%
16	13.998	1865	1872	1883	rBV	1580375	2374396	60.08%	5.621%
17	14.304	1917	1924	1935	rBV	1272551	1930683	48.85%	4.571%
18	14.539	1956	1964	2002	rBV	292466	823939	20.85%	1.951%
19	15.304	2087	2094	2110	rBV	1975310	2877766	72.82%	6.813%
20	15.439	2110	2117	2130	rVV	412069	692533	17.52%	1.639%
21	15.545	2132	2135	2143	rVB3	12889	21109	0.53%	0.050%
22	15.862	2185	2189	2195	rVV6	7282	13207	0.33%	0.031%
23	15.998	2206	2212	2215	rBV6	1883	4315	0.11%	0.010%
24	16.409	2279	2282	2292	rVB9	3750	8064	0.20%	0.019%
25	16.539	2301	2304	2309	rBV5	7330	13184	0.33%	0.031%
26	16.739	2334	2338	2341	rBV6	2266	4298	0.11%	0.010%
27	16.845	2352	2356	2358	rBV3	3571	4273	0.11%	0.010%
28	17.051	2385	2391	2402	rBV	1588464	2246047	56.83%	5.317%
29	17.151	2402	2408	2427	rVB	2087656	3143887	79.55%	7.443%
30	19.015	2720	2725	2732	rBV2	25638	39543	1.00%	0.094%
31	19.086	2733	2737	2743	rBV3	25529	38225	0.97%	0.090%
32	19.450	2792	2799	2812	rBV	2514633	3758785	95.11%	8.898%
33	20.944	3050	3053	3061	rVB	90364	128074	3.24%	0.303%
34	21.280	3104	3110	3125	rBV	1631848	2607466	65.98%	6.173%
35	23.985	3562	3570	3587	rVB	1657095	3952089	100.00%	9.356%
36	24.185	3596	3604	3621	rVB	1121761	2966209	75.05%	7.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048604.D
Acq On : 12 Nov 2024 04:14
Operator : RC/JU
Sample : PB164730BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK730

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42242243

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048604.D
Acq On : 12 Nov 2024 04:14
Operator : RC/JU
Sample : PB164730BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK730

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

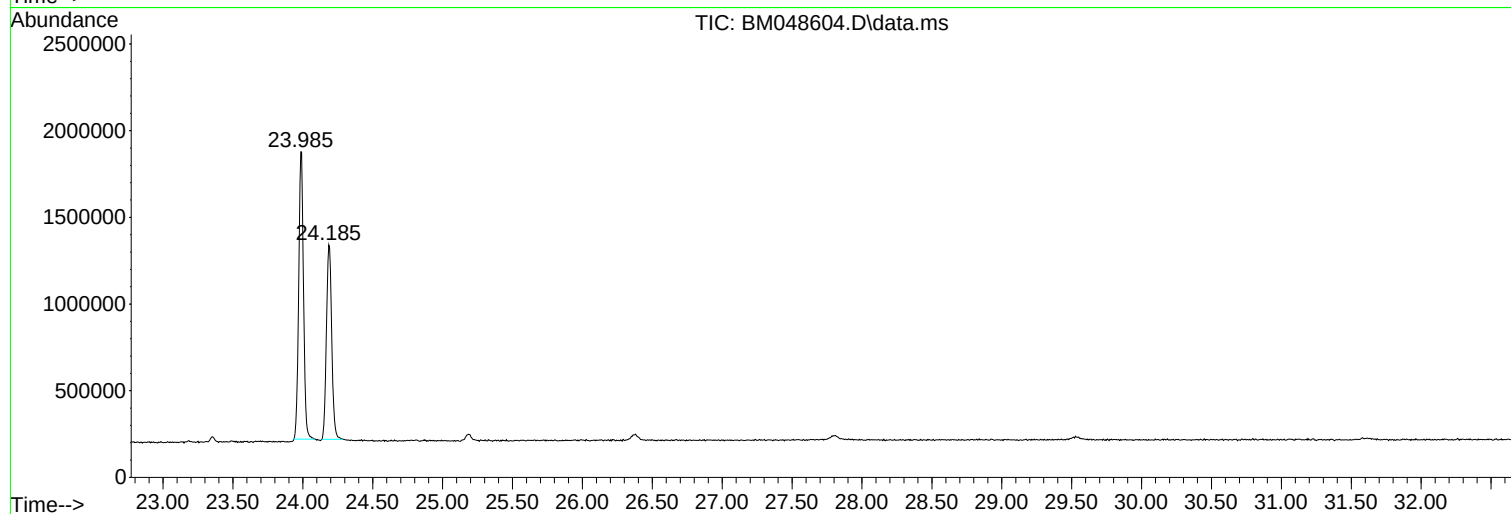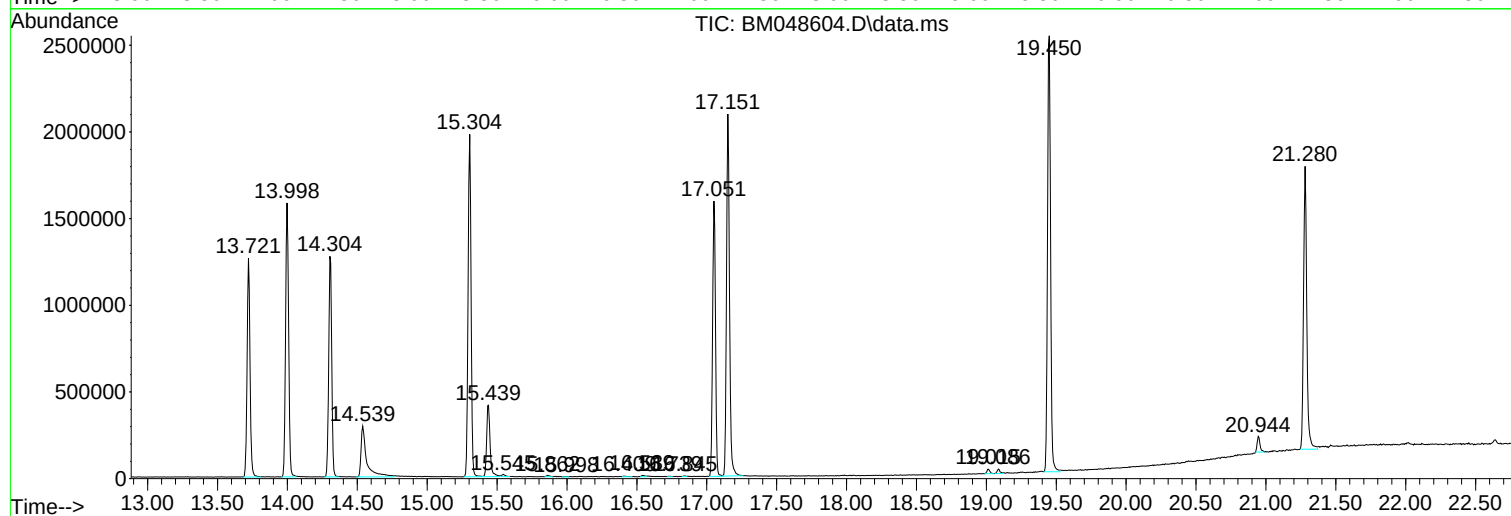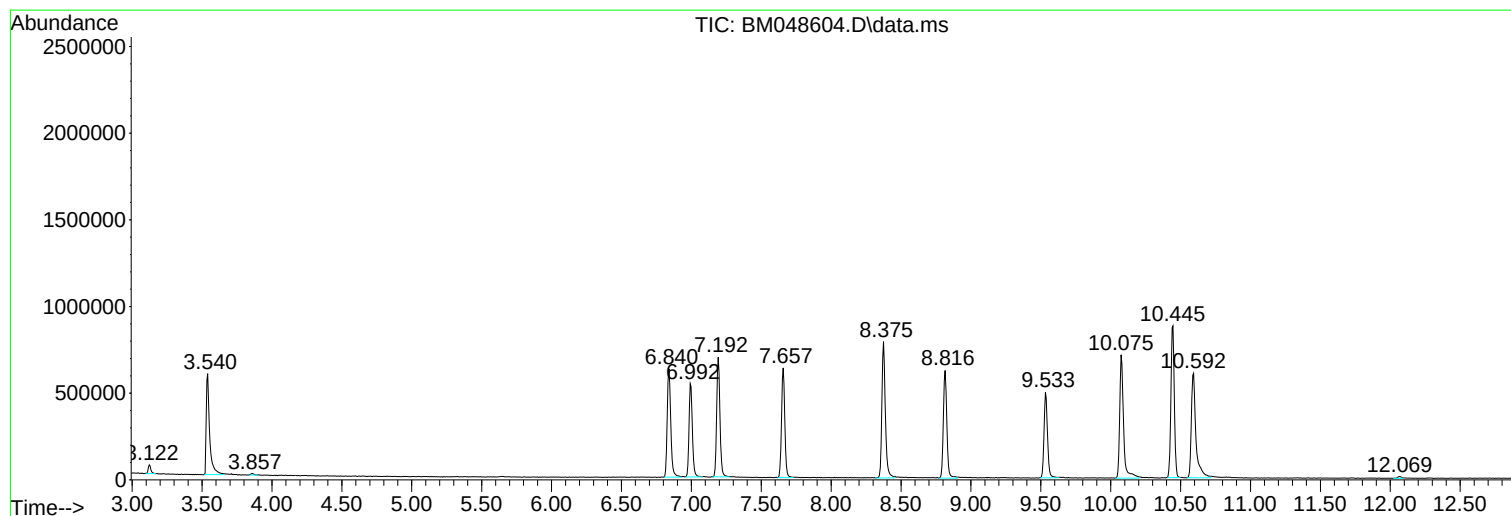

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048604.D
Acq On : 12 Nov 2024 04:14
Operator : RC/JU
Sample : PB164730BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK730

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048604.D
Acq On : 12 Nov 2024 04:14
Operator : RC/JU
Sample : PB164730BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK730

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc