

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048607.D
 Acq On : 12 Nov 2024 06:12
 Operator : RC/JU
 Sample : P4714-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	29	rBV	37627	48179	0.87%	0.105%
2	3.546	91	95	111	rBV	182384	332276	6.02%	0.722%
3	3.857	145	148	152	rBV2	9836	12590	0.23%	0.027%
4	4.369	230	235	239	rBV	30301	41736	0.76%	0.091%
5	4.804	305	309	313	rVB6	5749	8886	0.16%	0.019%
6	5.092	355	358	364	rBV4	4804	6056	0.11%	0.013%
7	5.304	390	394	402	rBV3	10386	21022	0.38%	0.046%
8	5.516	426	430	436	rBV2	11900	18856	0.34%	0.041%
9	5.675	453	457	462	rVB5	10665	18971	0.34%	0.041%
10	6.216	544	549	557	rBV6	5377	11522	0.21%	0.025%
11	6.292	559	562	565	rBV4	4308	6330	0.11%	0.014%
12	6.839	649	655	670	rVB	161335	319192	5.79%	0.694%
13	6.992	675	681	694	rBV	585661	969136	17.57%	2.107%
14	7.192	708	715	725	rBV	664080	1108033	20.09%	2.409%
15	7.281	726	730	738	rVB4	24553	42595	0.77%	0.093%
16	7.657	787	794	804	rBV	611857	1004905	18.22%	2.184%
17	7.939	837	842	847	rBV7	3990	9114	0.17%	0.020%
18	8.375	909	916	932	rBV	530133	934097	16.94%	2.031%
19	8.481	932	934	938	rVB5	3587	5669	0.10%	0.012%
20	8.816	984	991	1000	rBV	665984	1150856	20.87%	2.502%
21	8.951	1009	1014	1018	rBV6	7414	12003	0.22%	0.026%
22	8.986	1018	1020	1026	rVB6	4428	6363	0.12%	0.014%
23	9.533	1104	1113	1125	rBV	565292	961732	17.44%	2.091%
24	10.075	1198	1205	1229	rBV	781528	1508010	27.34%	3.278%
25	10.445	1256	1268	1277	rBV	852340	1450042	26.29%	3.152%
26	10.592	1285	1293	1315	rBV	615670	1379292	25.01%	2.998%
27	12.069	1536	1544	1548	rBV4	9356	16791	0.30%	0.037%
28	13.721	1817	1825	1843	rBV	1619719	2285835	41.45%	4.969%
29	13.998	1865	1872	1885	rBV	1740288	2634235	47.77%	5.726%
30	14.304	1918	1924	1933	rBV	1253478	1861234	33.75%	4.046%
31	14.557	1962	1967	1984	rBV3	52324	181874	3.30%	0.395%
32	15.304	2086	2094	2103	rBV	2470372	3557008	64.50%	7.732%
33	15.433	2110	2116	2132	rBV	649464	1025739	18.60%	2.230%
34	15.551	2132	2136	2144	rVV5	15233	27645	0.50%	0.060%
35	15.674	2148	2157	2162	rBV	29347	43373	0.79%	0.094%
36	15.862	2184	2189	2195	rBV7	9481	20250	0.37%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048607.D
 Acq On : 12 Nov 2024 06:12
 Operator : RC/JU
 Sample : P4714-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	16.404	2275	2281	2285	rBV7	4391	8027	0.15%	0.017%
38	16.545	2301	2305	2309	rBV5	7664	11611	0.21%	0.025%
39	16.839	2351	2355	2362	rVB8	4044	8599	0.16%	0.019%
40	17.051	2384	2391	2401	rBV	1566434	2206914	40.02%	4.797%
41	17.151	2402	2408	2425	rVV	2820562	4244335	76.96%	9.226%
42	17.268	2425	2428	2433	rVB6	9249	14588	0.26%	0.032%
43	17.462	2455	2461	2465	rBV8	2895	6335	0.11%	0.014%
44	17.956	2540	2545	2552	rBV5	26317	46408	0.84%	0.101%
45	19.015	2720	2725	2732	rBV	36312	52295	0.95%	0.114%
46	19.086	2732	2737	2740	rBV	38400	52371	0.95%	0.114%
47	19.239	2759	2763	2770	rBV8	15512	31615	0.57%	0.069%
48	19.386	2786	2788	2792	rBV5	6382	6688	0.12%	0.015%
49	19.445	2792	2798	2811	rBV	3565269	5166773	93.69%	11.232%
50	20.944	3049	3053	3062	rBV2	96965	179861	3.26%	0.391%
51	21.280	3104	3110	3120	rBV	1604664	2527584	45.83%	5.495%
52	23.985	3561	3570	3590	rVB	2260334	5514982	100.00%	11.989%
53	24.185	3596	3604	3620	rVB	1154958	2881532	52.25%	6.264%




Sum of corrected areas: 46001965

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048607.D
Acq On : 12 Nov 2024 06:12
Operator : RC/JU
Sample : P4714-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

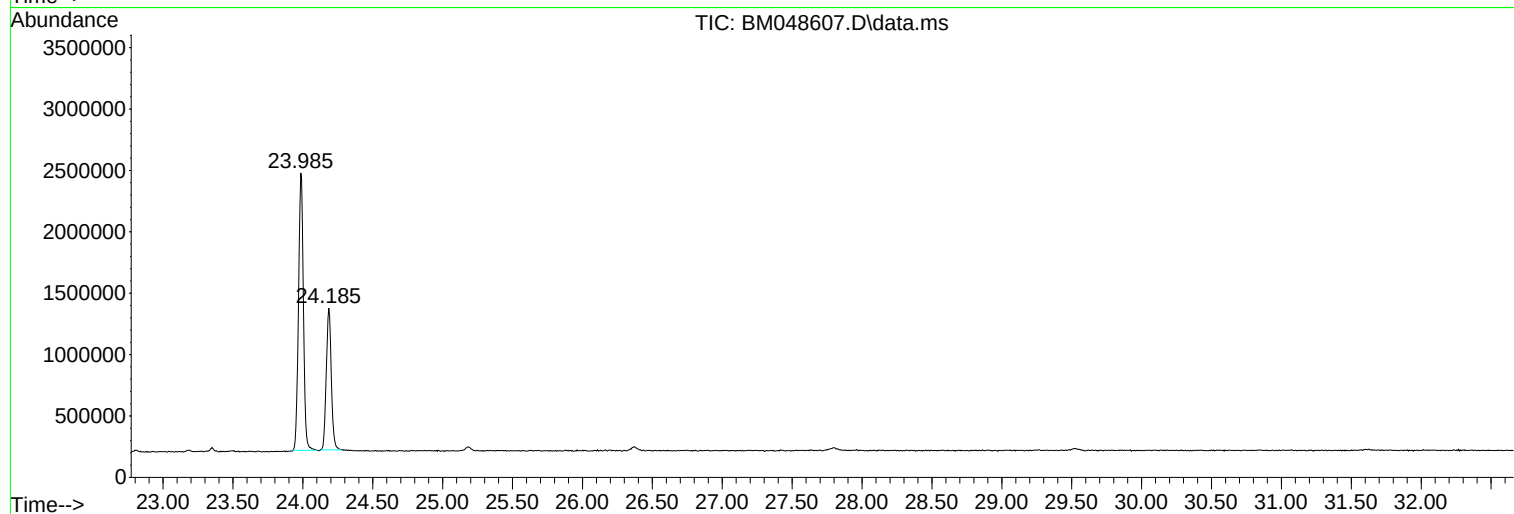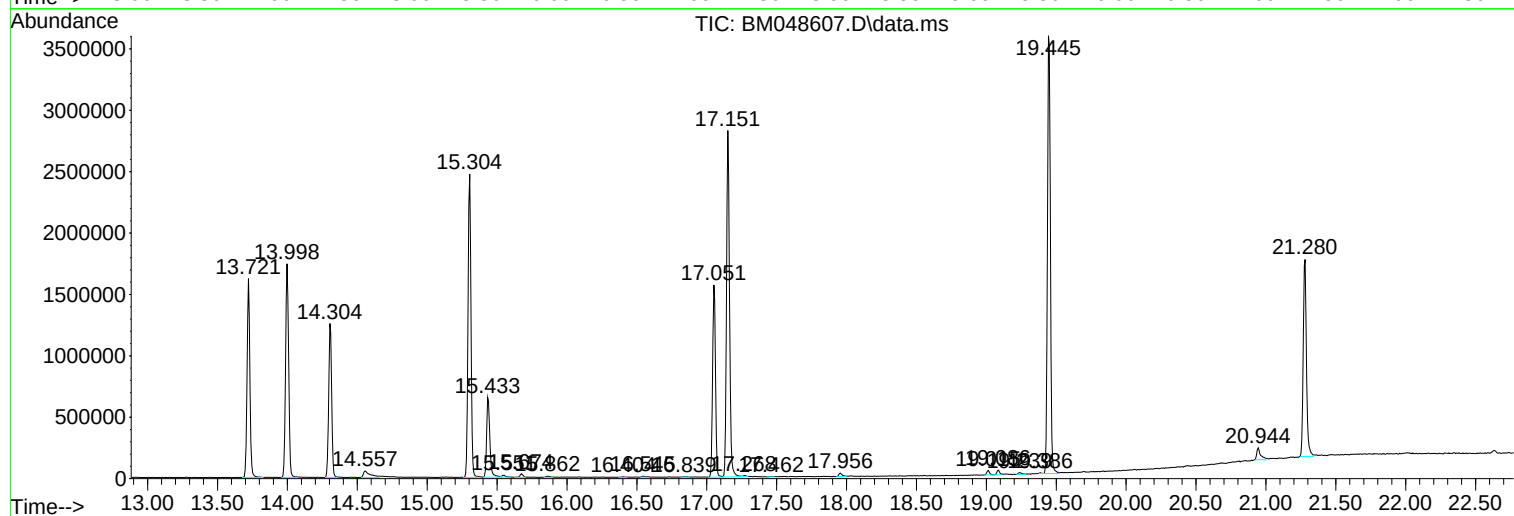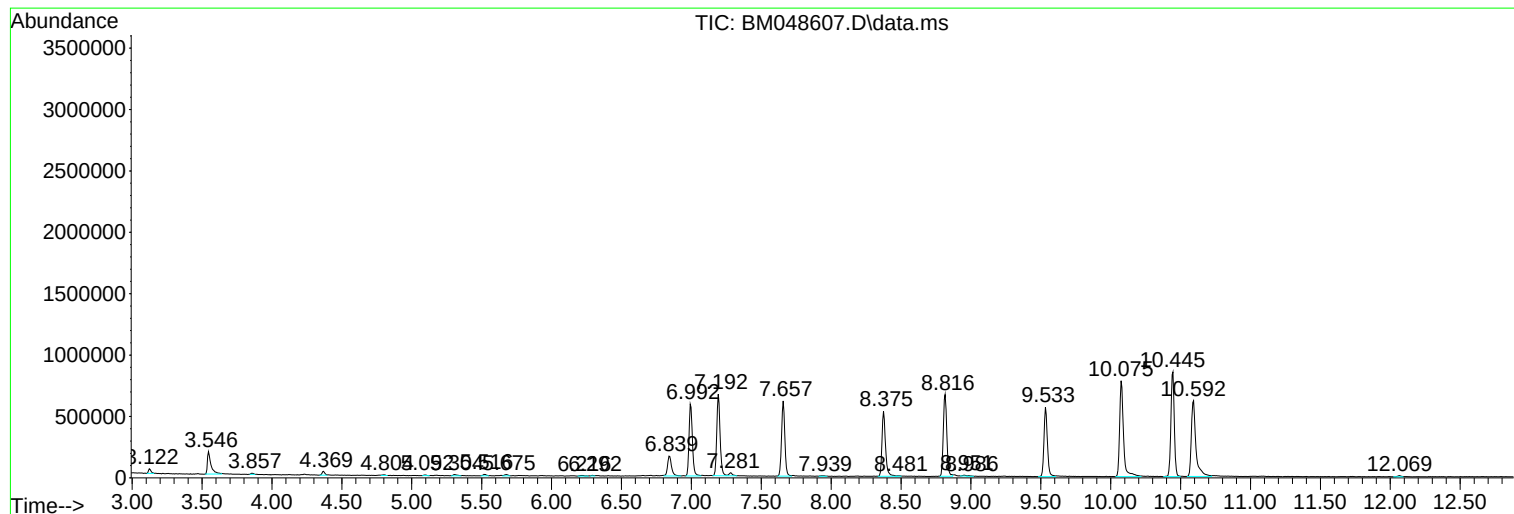

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048607.D
Acq On : 12 Nov 2024 06:12
Operator : RC/JU
Sample : P4714-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048607.D
Acq On : 12 Nov 2024 06:12
Operator : RC/JU
Sample : P4714-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc