

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048609.D
 Acq On : 12 Nov 2024 07:31
 Operator : RC/JU
 Sample : P4714-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	31	rVB	38612	50988	1.01%	0.120%
2	3.546	91	95	108	rBV	174597	313067	6.21%	0.735%
3	3.863	145	149	152	rVB2	8882	12399	0.25%	0.029%
4	4.369	231	235	241	rBV	26013	34455	0.68%	0.081%
5	5.093	354	358	361	rBV5	5134	7677	0.15%	0.018%
6	5.257	381	386	388	rBV5	3262	5611	0.11%	0.013%
7	5.310	391	395	397	rVV4	4079	5681	0.11%	0.013%
8	5.522	428	431	435	rVB4	5042	6104	0.12%	0.014%
9	5.675	454	457	461	rVB4	8871	13593	0.27%	0.032%
10	5.934	499	501	507	rVB7	3538	5570	0.11%	0.013%
11	6.216	546	549	554	rVB4	5096	8277	0.16%	0.019%
12	6.651	621	623	626	rVB4	5501	5229	0.10%	0.012%
13	6.840	650	655	668	rVB	146472	280462	5.57%	0.659%
14	6.992	675	681	693	rBV	543213	895861	17.78%	2.104%
15	7.192	709	715	725	rBV	605366	1011390	20.08%	2.375%
16	7.281	726	730	737	rVB3	22346	38287	0.76%	0.090%
17	7.481	760	764	769	rBV8	3216	6057	0.12%	0.014%
18	7.657	785	794	804	rBV	590501	971878	19.29%	2.282%
19	8.375	910	916	929	rBV	484293	862250	17.12%	2.025%
20	8.816	983	991	999	rBV	631678	1069007	21.22%	2.510%
21	9.233	1059	1062	1067	rVB6	4169	5878	0.12%	0.014%
22	9.533	1106	1113	1126	rBV	523120	894375	17.75%	2.100%
23	10.075	1197	1205	1225	rBV	715819	1387027	27.53%	3.257%
24	10.439	1260	1267	1275	rBV	805813	1389795	27.59%	3.263%
25	10.586	1284	1292	1315	rBV	552674	1274029	25.29%	2.992%
26	12.063	1539	1543	1549	rBV4	9578	17638	0.35%	0.041%
27	13.721	1818	1825	1841	rBV	1447667	2076889	41.23%	4.877%
28	13.998	1865	1872	1884	rBV	1676417	2474408	49.12%	5.810%
29	14.304	1917	1924	1933	rBV	1224493	1790614	35.55%	4.205%
30	14.557	1962	1967	1988	rBV3	41746	169704	3.37%	0.398%
31	15.115	2057	2062	2065	rBV4	3673	6543	0.13%	0.015%
32	15.304	2087	2094	2110	rBV	2169199	3242776	64.37%	7.615%
33	15.433	2110	2116	2129	rVV	578388	911349	18.09%	2.140%
34	15.545	2132	2135	2139	rVB3	11512	15115	0.30%	0.035%
35	15.674	2152	2157	2163	rVV	34498	51625	1.02%	0.121%
36	15.862	2183	2189	2193	rBV5	7401	14693	0.29%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048609.D
 Acq On : 12 Nov 2024 07:31
 Operator : RC/JU
 Sample : P4714-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	16.551	2300	2306	2312	rBV9	8171	18038	0.36%	0.042%
38	16.833	2352	2354	2362	rVB5	4075	7818	0.16%	0.018%
39	17.051	2385	2391	2401	rBV	1485532	2107959	41.85%	4.950%
40	17.151	2402	2408	2424	rVV	2600329	3821821	75.87%	8.974%
41	17.468	2458	2462	2464	rBV5	3924	5177	0.10%	0.012%
42	17.615	2484	2487	2491	rVB6	4127	6190	0.12%	0.015%
43	17.951	2538	2544	2553	rBV4	36481	70576	1.40%	0.166%
44	18.027	2553	2557	2561	rVV5	6145	9670	0.19%	0.023%
45	19.015	2720	2725	2730	rBV	34396	52550	1.04%	0.123%
46	19.086	2733	2737	2744	rBV	32641	52296	1.04%	0.123%
47	19.239	2759	2763	2770	rBV5	21313	33594	0.67%	0.079%
48	19.445	2792	2798	2814	rBV	3267833	4695536	93.21%	11.026%
49	20.944	3049	3053	3064	rBV	98430	183604	3.64%	0.431%
50	21.280	3104	3110	3123	rBV	1532064	2421875	48.08%	5.687%
51	23.985	3561	3570	3589	rBV	2039747	5037427	100.00%	11.829%
52	24.185	3596	3604	3617	rVB	1053348	2735960	54.31%	6.424%




Sum of corrected areas: 42586392

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048609.D
Acq On : 12 Nov 2024 07:31
Operator : RC/JU
Sample : P4714-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

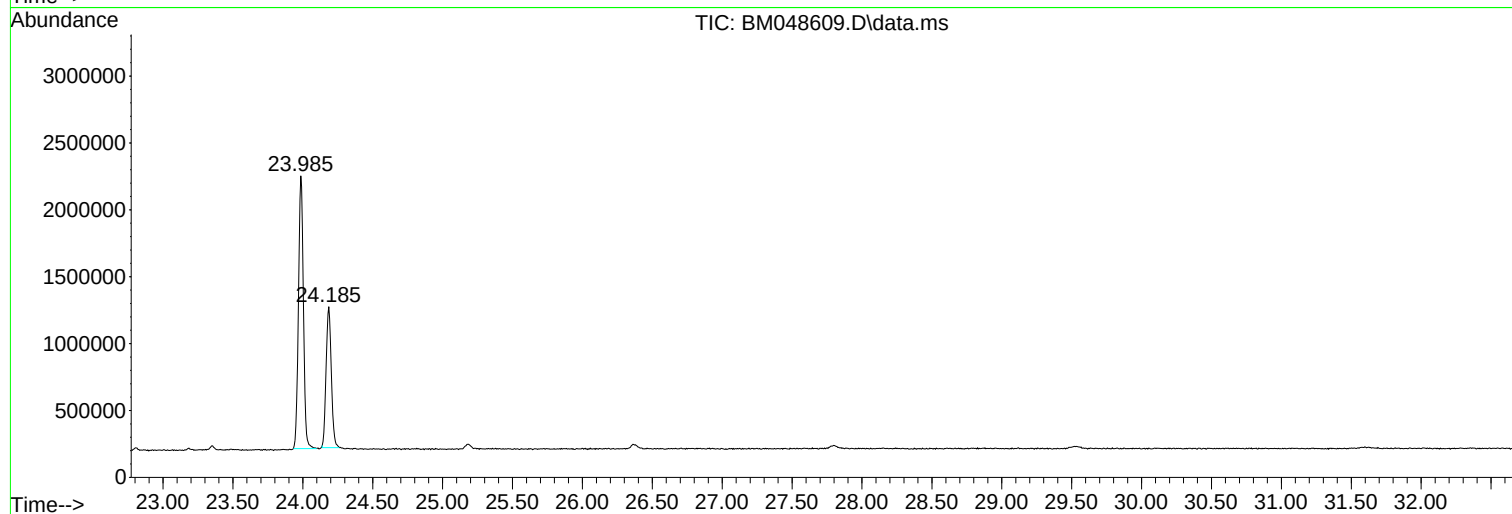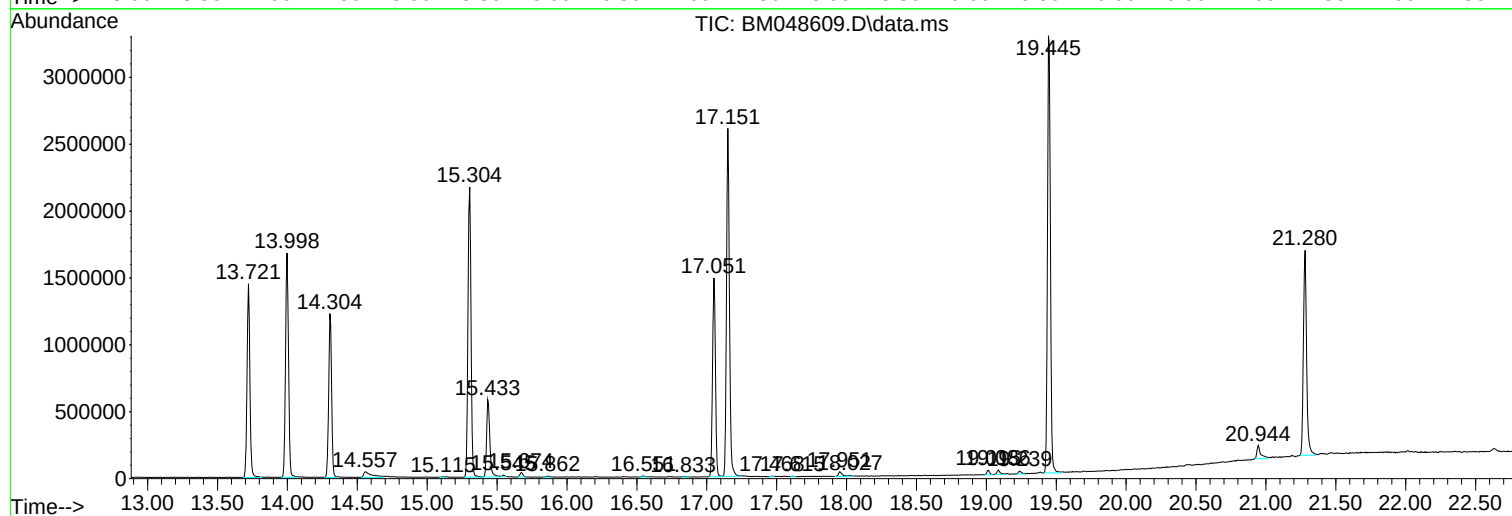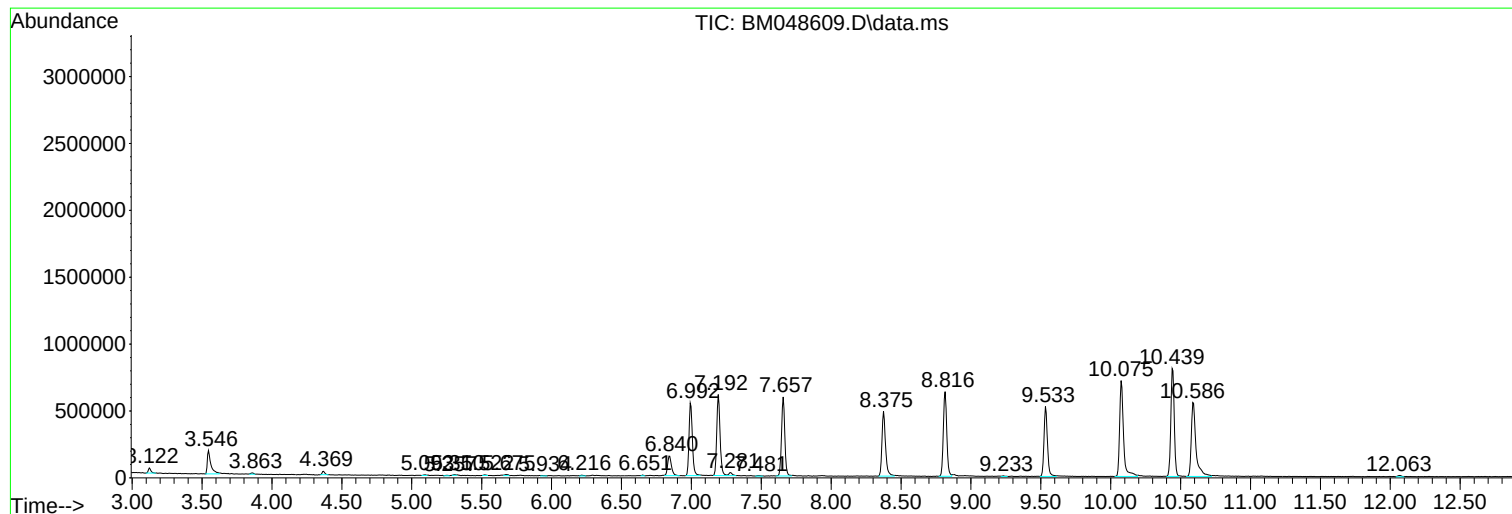

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048609.D
Acq On : 12 Nov 2024 07:31
Operator : RC/JU
Sample : P4714-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048609.D
Acq On : 12 Nov 2024 07:31
Operator : RC/JU
Sample : P4714-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc