

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048610.D
 Acq On : 12 Nov 2024 08:10
 Operator : RC/JU
 Sample : P4714-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	28	rVB	36873	47076	1.15%	0.122%
2	3.546	92	95	110	rBV	172785	322718	7.85%	0.834%
3	3.857	145	148	153	rBV3	7647	13713	0.33%	0.035%
4	4.369	231	235	243	rBV	25115	34491	0.84%	0.089%
5	4.951	329	334	335	rBV4	4317	5910	0.14%	0.015%
6	5.098	356	359	363	rVB5	4734	6123	0.15%	0.016%
7	5.304	391	394	400	rBV4	4787	8724	0.21%	0.023%
8	5.675	455	457	464	rVB8	8725	13892	0.34%	0.036%
9	5.934	496	501	504	rBV5	4414	7547	0.18%	0.019%
10	6.222	545	550	553	rVB5	4242	6762	0.16%	0.017%
11	6.293	558	562	565	rBV4	4469	6941	0.17%	0.018%
12	6.698	629	631	636	rVB6	3033	4548	0.11%	0.012%
13	6.845	649	656	669	rVB	131653	259402	6.31%	0.670%
14	6.992	675	681	692	rBV	471803	791968	19.26%	2.046%
15	7.192	709	715	726	rBV	537449	901939	21.94%	2.330%
16	7.281	726	730	739	rVB3	22316	38590	0.94%	0.100%
17	7.657	785	794	802	rBV	609014	1001251	24.36%	2.586%
18	7.716	802	804	807	rVB4	3604	4115	0.10%	0.011%
19	8.322	902	907	909	rBV5	3341	6156	0.15%	0.016%
20	8.375	909	916	931	rVV	435605	785008	19.10%	2.028%
21	8.816	984	991	1001	rBV	528071	926477	22.54%	2.393%
22	9.533	1105	1113	1127	rBV	443790	768733	18.70%	1.986%
23	9.863	1163	1169	1173	rBV8	2809	6136	0.15%	0.016%
24	10.075	1199	1205	1231	rBV	610453	1227075	29.85%	3.169%
25	10.439	1260	1267	1276	rBV	846617	1445884	35.17%	3.735%
26	10.592	1285	1293	1310	rBV	505362	1154888	28.09%	2.983%
27	11.157	1385	1389	1398	rVB8	8626	19920	0.48%	0.051%
28	12.069	1538	1544	1548	rBV4	7710	13943	0.34%	0.036%
29	13.721	1818	1825	1838	rBV	1242465	1803470	43.87%	4.658%
30	13.998	1865	1872	1885	rBV	1420423	2114129	51.43%	5.461%
31	14.304	1917	1924	1935	rVV	1256614	1871110	45.51%	4.833%
32	14.557	1959	1967	1985	rBV7	30712	136233	3.31%	0.352%
33	15.163	2068	2070	2074	rVB4	4304	5104	0.12%	0.013%
34	15.304	2087	2094	2110	rBV	1792735	2811595	68.39%	7.262%
35	15.439	2110	2117	2130	rBV	429827	715575	17.41%	1.848%
36	15.539	2132	2134	2139	rVB6	9765	16094	0.39%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048610.D
 Acq On : 12 Nov 2024 08:10
 Operator : RC/JU
 Sample : P4714-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	15.674	2151	2157	2165	rBV	56280	82805	2.01%	0.214%
38	15.862	2184	2189	2195	rBV6	7838	14210	0.35%	0.037%
39	16.027	2213	2217	2221	rBV5	6956	10571	0.26%	0.027%
40	16.409	2278	2282	2286	rVV5	4404	6819	0.17%	0.018%
41	16.551	2300	2306	2308	rBV6	7175	12187	0.30%	0.031%
42	16.821	2346	2352	2355	rBV6	9860	17206	0.42%	0.044%
43	16.874	2357	2361	2365	rVB7	3491	6711	0.16%	0.017%
44	17.051	2385	2391	2401	rBV	1631790	2202265	53.57%	5.688%
45	17.151	2401	2408	2421	rVV	2246691	3290715	80.05%	8.500%
46	17.274	2425	2429	2435	rVV9	10335	22444	0.55%	0.058%
47	17.345	2438	2441	2446	rVB5	5716	9486	0.23%	0.025%
48	17.468	2460	2462	2468	rVB7	3582	5956	0.14%	0.015%
49	17.556	2472	2477	2483	rBV6	10074	18548	0.45%	0.048%
50	17.951	2540	2544	2550	rBV6	28570	46093	1.12%	0.119%
51	18.251	2590	2595	2598	rBV2	12166	17000	0.41%	0.044%
52	18.315	2602	2606	2608	rBV5	3004	4599	0.11%	0.012%
53	18.886	2700	2703	2710	rVB7	7609	10945	0.27%	0.028%
54	19.015	2720	2725	2730	rBV3	27687	43819	1.07%	0.113%
55	19.086	2733	2737	2742	rVV	24834	36062	0.88%	0.093%
56	19.245	2760	2764	2768	rBV7	14445	19180	0.47%	0.050%
57	19.386	2785	2788	2791	rVB3	9328	11966	0.29%	0.031%
58	19.445	2792	2798	2812	rVV	2750871	3978937	96.79%	10.277%
59	20.944	3049	3053	3065	rBV2	98125	190127	4.62%	0.491%
60	21.280	3104	3110	3122	rBV	1526929	2456181	59.75%	6.344%
61	23.985	3561	3570	3588	rBV	1708207	4111064	100.00%	10.619%
62	24.185	3596	3604	3619	rVB	1073506	2786912	67.79%	7.198%




Sum of corrected areas: 38716048

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048610.D
Acq On : 12 Nov 2024 08:10
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

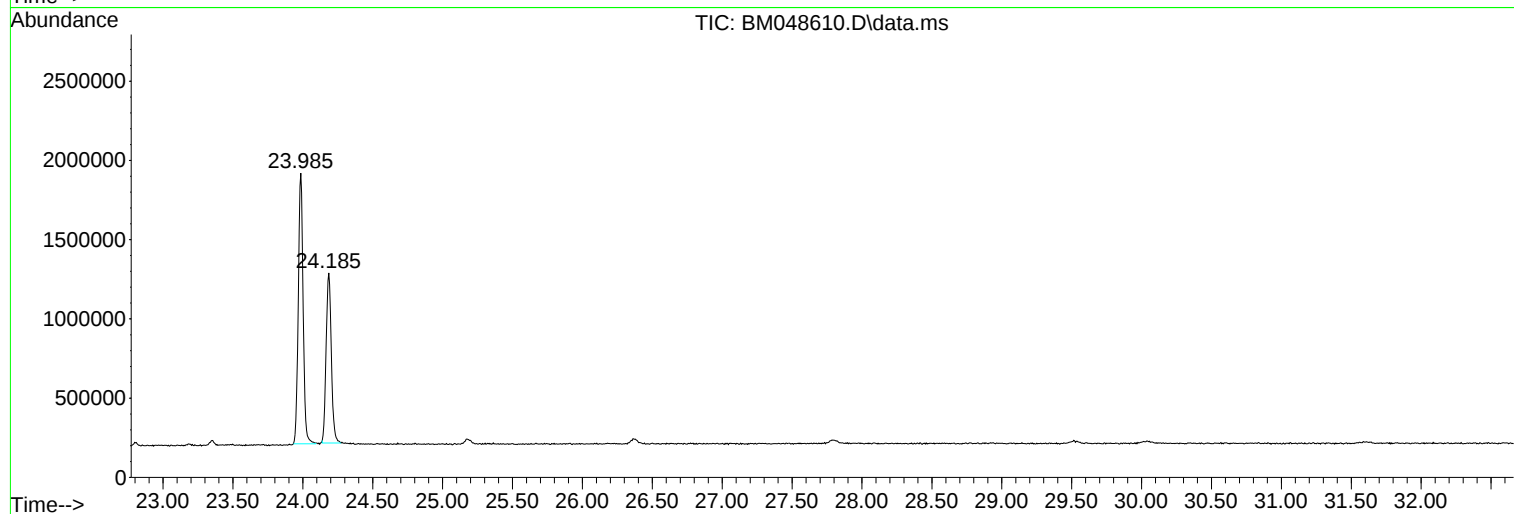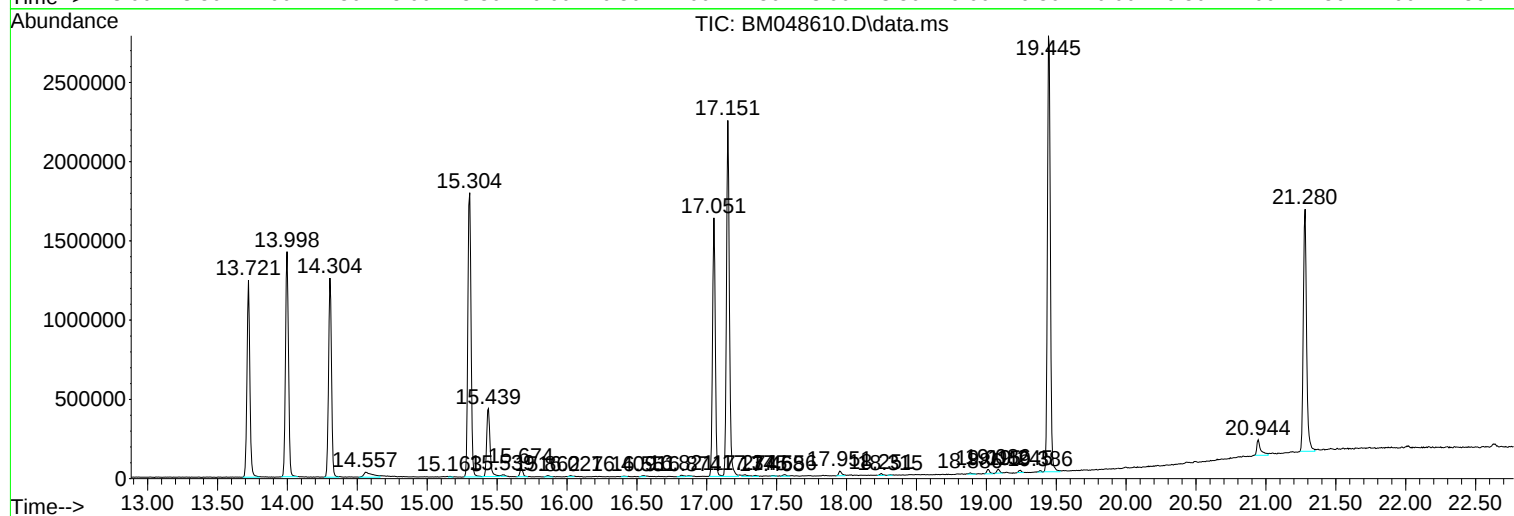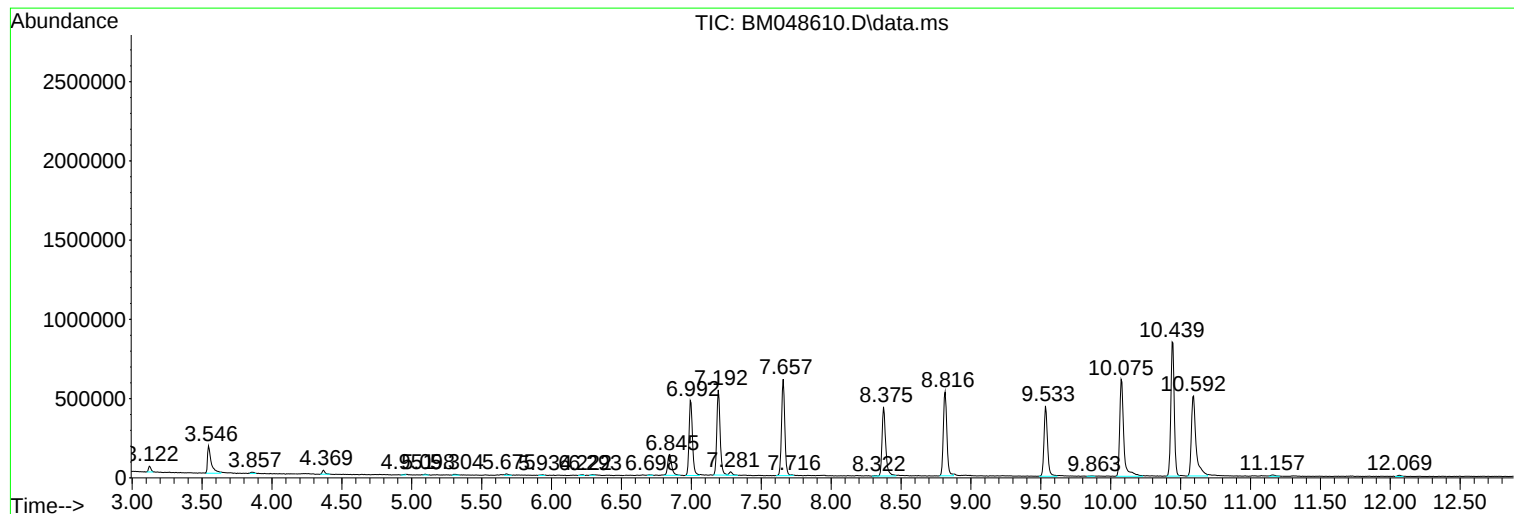

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048610.D
Acq On : 12 Nov 2024 08:10
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048610.D
Acq On : 12 Nov 2024 08:10
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc