

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048617.D
 Acq On : 12 Nov 2024 12:45
 Operator : RC/JU
 Sample : PB164897BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK897

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	33	rVB	43082	65474	1.91%	0.183%
2	3.540	91	94	110	rBV	458104	803992	23.40%	2.246%
3	3.863	145	149	154	rVB2	10063	14083	0.41%	0.039%
4	4.287	219	221	225	rVB5	3567	3696	0.11%	0.010%
5	6.840	649	655	669	rBV	516924	905364	26.35%	2.530%
6	6.993	676	681	694	rVB	453494	754401	21.96%	2.108%
7	7.193	708	715	729	rBV	594396	999371	29.09%	2.792%
8	7.657	787	794	806	rVV	493673	823163	23.96%	2.300%
9	8.375	909	916	935	rBV	658302	1173479	34.15%	3.279%
10	8.816	982	991	1001	rBV	519372	906538	26.39%	2.533%
11	8.951	1008	1014	1021	rBV	37163	66261	1.93%	0.185%
12	9.228	1059	1061	1066	rVB6	2877	3530	0.10%	0.010%
13	9.534	1107	1113	1127	rBV	425968	745700	21.70%	2.084%
14	10.075	1197	1205	1216	rBV	581600	1130041	32.89%	3.157%
15	10.439	1260	1267	1278	rBV	701208	1192586	34.71%	3.332%
16	10.592	1286	1293	1314	rBV	471763	1127007	32.80%	3.149%
17	10.828	1330	1333	1336	rBV5	3138	3441	0.10%	0.010%
18	12.063	1539	1543	1551	rBV5	6616	14081	0.41%	0.039%
19	13.274	1747	1749	1754	rBV5	2324	3628	0.11%	0.010%
20	13.721	1818	1825	1838	rBV	1147878	1682032	48.96%	4.700%
21	13.998	1865	1872	1882	rBV	1402658	2101167	61.16%	5.871%
22	14.304	1917	1924	1935	rBV	1064607	1563046	45.49%	4.367%
23	14.539	1958	1964	1984	rBV	221654	619338	18.03%	1.730%
24	15.304	2087	2094	2106	rBV	1751547	2600184	75.68%	7.265%
25	15.439	2111	2117	2130	rVV	378161	621992	18.10%	1.738%
26	15.545	2132	2135	2140	rVV6	9446	16721	0.49%	0.047%
27	15.674	2154	2157	2161	rVB6	3760	6193	0.18%	0.017%
28	15.863	2182	2189	2194	rBV6	7819	14688	0.43%	0.041%
29	16.092	2223	2228	2233	rBV7	4211	6431	0.19%	0.018%
30	16.410	2279	2282	2285	rVB5	2550	3828	0.11%	0.011%
31	16.539	2300	2304	2308	rBV5	6035	9612	0.28%	0.027%
32	17.051	2385	2391	2402	rBV	1271407	1797109	52.31%	5.021%
33	17.151	2402	2408	2423	rVV2	1856053	2809055	81.76%	7.849%
34	17.357	2439	2443	2445	rVB5	2944	4291	0.12%	0.012%
35	17.727	2502	2506	2510	rBV6	4742	8441	0.25%	0.024%
36	17.962	2542	2546	2550	rBV5	7521	11074	0.32%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048617.D
Acq On : 12 Nov 2024 12:45
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK897

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	19.009	2720	2724	2728	rBV2	24228	35530	1.03%	0.099%
38	19.086	2733	2737	2741	rBV2	20826	29834	0.87%	0.083%
39	19.239	2759	2763	2769	rBV8	14811	25988	0.76%	0.073%
40	19.445	2792	2798	2811	rBV	2291931	3333049	97.01%	9.313%
41	20.945	3049	3053	3062	rBV	100290	161332	4.70%	0.451%
42	21.280	3104	3110	3122	rBV	1226486	1984697	57.77%	5.545%
43	23.986	3561	3570	3585	rBV	1399849	3435756	100.00%	9.600%
44	24.186	3596	3604	3617	rVB	811660	2172853	63.24%	6.071%




Sum of corrected areas: 35790077

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048617.D
Acq On : 12 Nov 2024 12:45
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

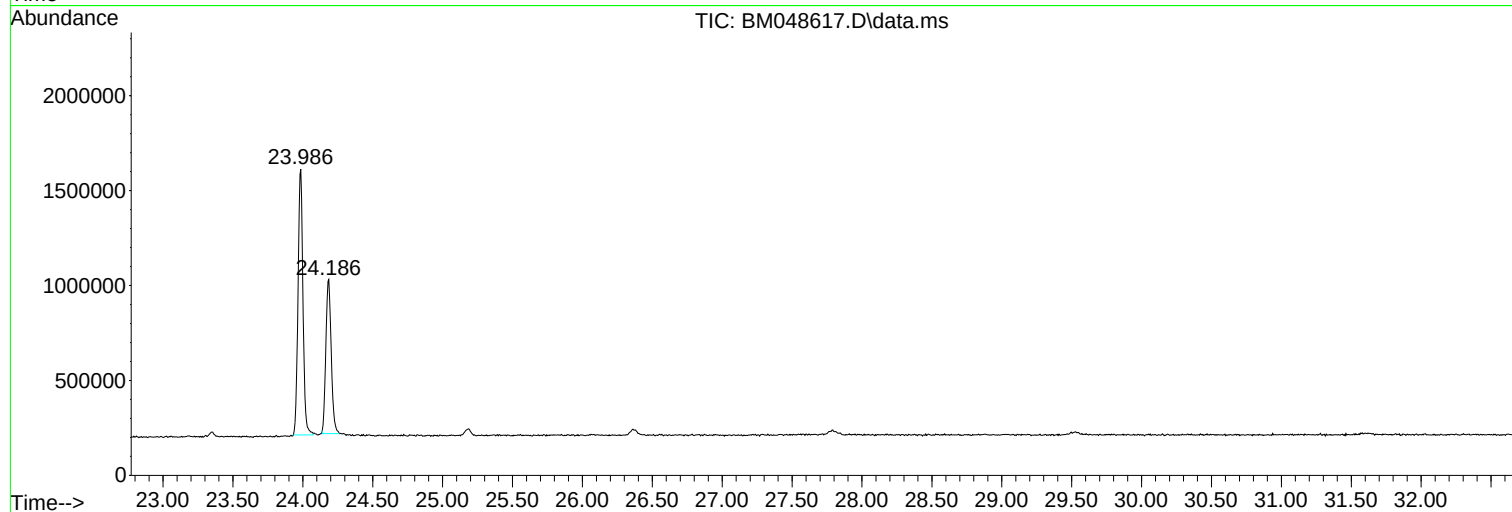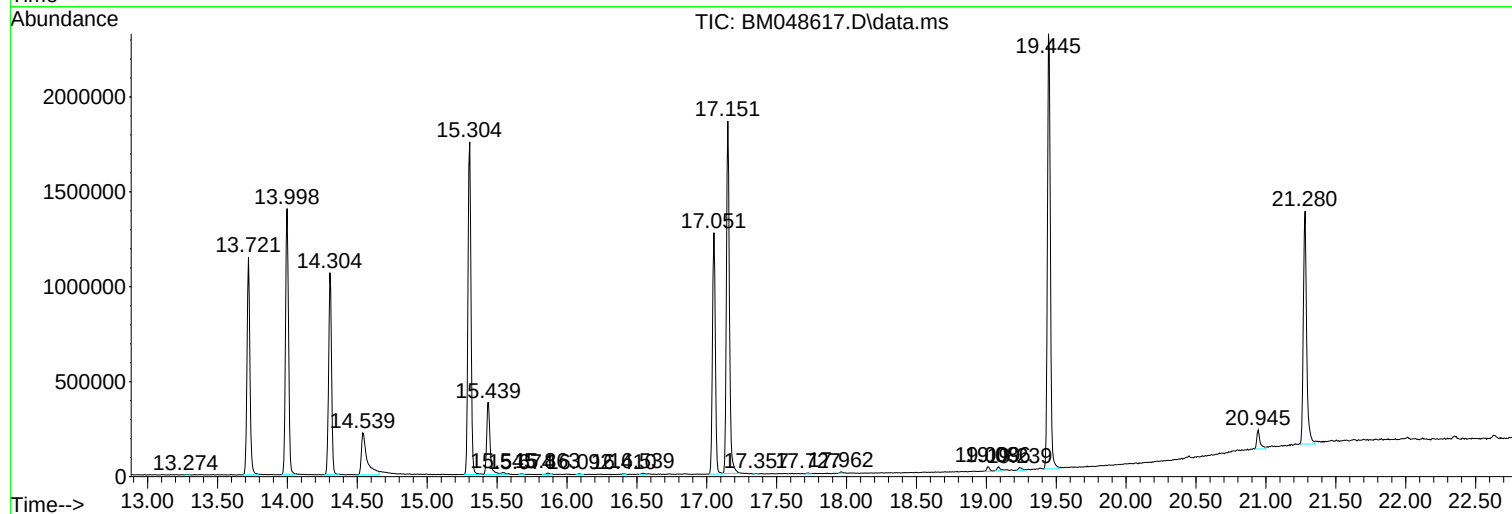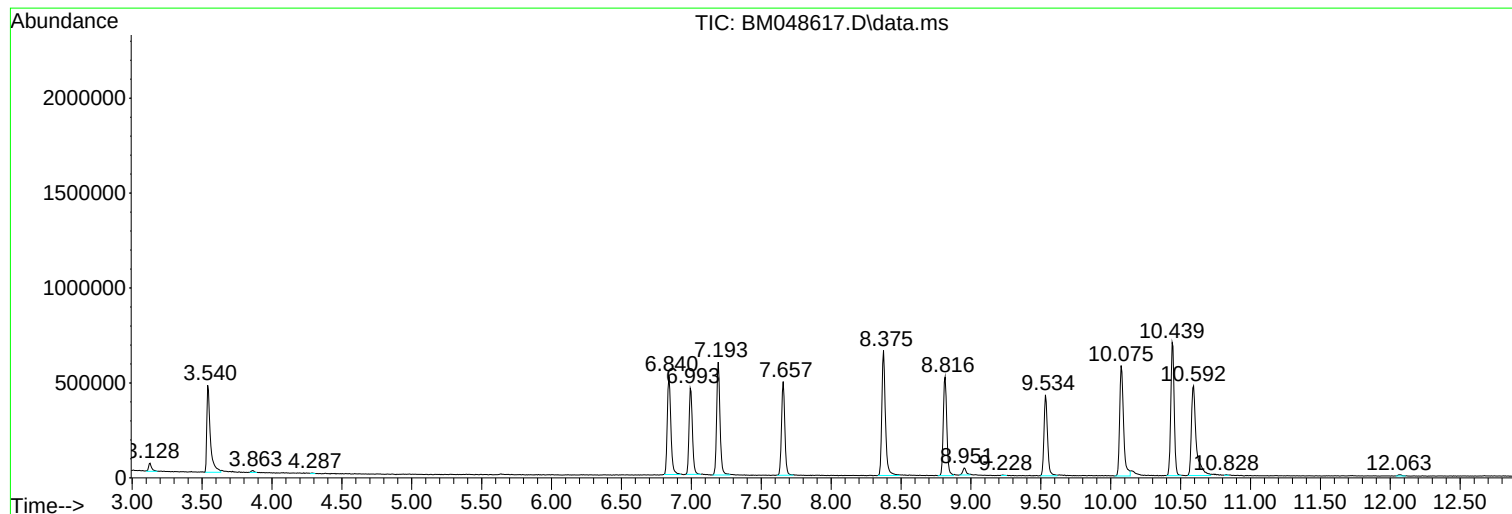

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048617.D
Acq On : 12 Nov 2024 12:45
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048617.D
Acq On : 12 Nov 2024 12:45
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc