

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048618.D
 Acq On : 12 Nov 2024 13:25
 Operator : RC/JU
 Sample : PB164899BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK899

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	29	rVB	39212	50783	1.52%	0.150%
2	3.534	90	93	111	rBV	422067	725598	21.75%	2.146%
3	3.857	146	148	152	rVB3	9137	9288	0.28%	0.027%
4	6.840	648	655	672	rBV	465269	829994	24.88%	2.455%
5	6.993	675	681	696	rVV	423761	681882	20.44%	2.017%
6	7.193	708	715	729	rBV	527634	874646	26.22%	2.587%
7	7.657	787	794	805	rBV	462330	783022	23.47%	2.316%
8	8.375	910	916	929	rBV	583325	1042317	31.25%	3.083%
9	8.816	983	991	1005	rBV	463099	817935	24.52%	2.419%
10	8.951	1009	1014	1020	rBV	31224	57973	1.74%	0.171%
11	9.534	1105	1113	1125	rBV	376111	667431	20.01%	1.974%
12	9.657	1132	1134	1142	rVB6	2872	4770	0.14%	0.014%
13	10.075	1197	1205	1216	rBV	520360	995845	29.85%	2.945%
14	10.439	1261	1267	1278	rBV	669382	1136198	34.06%	3.360%
15	10.592	1284	1293	1315	rBV	417729	1020058	30.58%	3.017%
16	11.645	1470	1472	1477	rVB4	2287	3593	0.11%	0.011%
17	11.716	1482	1484	1489	rVB6	2295	3614	0.11%	0.011%
18	12.069	1540	1544	1554	rVB3	6856	16390	0.49%	0.048%
19	13.722	1818	1825	1836	rBV	1031974	1529553	45.85%	4.524%
20	13.998	1865	1872	1882	rBV2	1255970	1918559	57.52%	5.674%
21	14.304	1917	1924	1933	rBV	1038630	1509501	45.25%	4.464%
22	14.539	1957	1964	1987	rBV	195065	569432	17.07%	1.684%
23	15.304	2087	2094	2110	rBV	1620122	2386006	71.53%	7.057%
24	15.439	2110	2117	2129	rVV	341654	585047	17.54%	1.730%
25	15.545	2132	2135	2145	rVB7	11843	22380	0.67%	0.066%
26	15.680	2153	2158	2159	rBV4	3398	4543	0.14%	0.013%
27	15.863	2182	2189	2196	rBV8	6399	13956	0.42%	0.041%
28	16.086	2223	2227	2232	rBV5	2701	4373	0.13%	0.013%
29	16.545	2301	2305	2308	rBV5	6316	8379	0.25%	0.025%
30	16.586	2310	2312	2316	rVB5	3577	3850	0.12%	0.011%
31	16.733	2333	2337	2339	rBV5	2835	3552	0.11%	0.011%
32	16.845	2351	2356	2358	rBV5	3037	4808	0.14%	0.014%
33	17.051	2385	2391	2402	rBV	1301663	1789802	53.66%	5.294%
34	17.151	2402	2408	2422	rVV	1707961	2635435	79.01%	7.795%
35	17.715	2502	2504	2510	rBV7	3462	6758	0.20%	0.020%
36	19.009	2720	2724	2729	rBV4	22280	34742	1.04%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048618.D
Acq On : 12 Nov 2024 13:25
Operator : RC/JU
Sample : PB164899BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK899

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	19.086	2734	2737	2742	rVB	15721	21543	0.65%	0.064%
38	19.445	2792	2798	2814	rBV	2122190	3187601	95.56%	9.428%
39	20.945	3049	3053	3062	rBV	94144	148832	4.46%	0.440%
40	21.280	3104	3110	3122	rBV	1219485	2032942	60.95%	6.013%
41	23.980	3561	3569	3583	rBV	1430141	3335640	100.00%	9.865%
42	24.180	3596	3603	3621	rVB	884570	2332707	69.93%	6.899%




Sum of corrected areas: 33811278

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048618.D
Acq On : 12 Nov 2024 13:25
Operator : RC/JU
Sample : PB164899BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

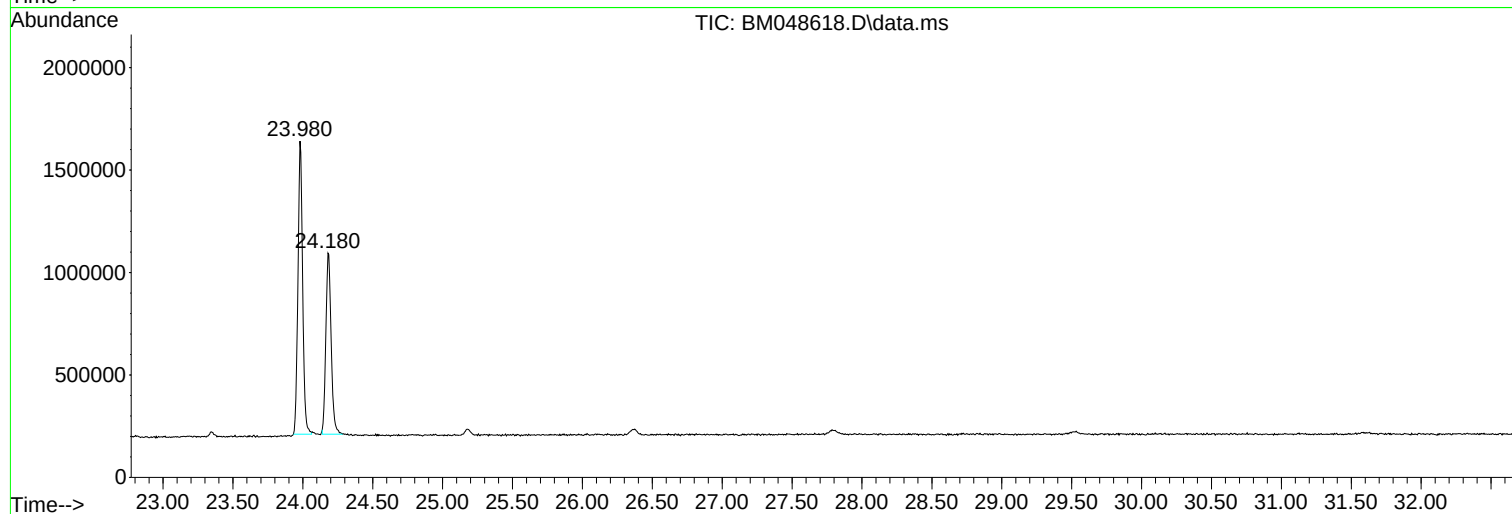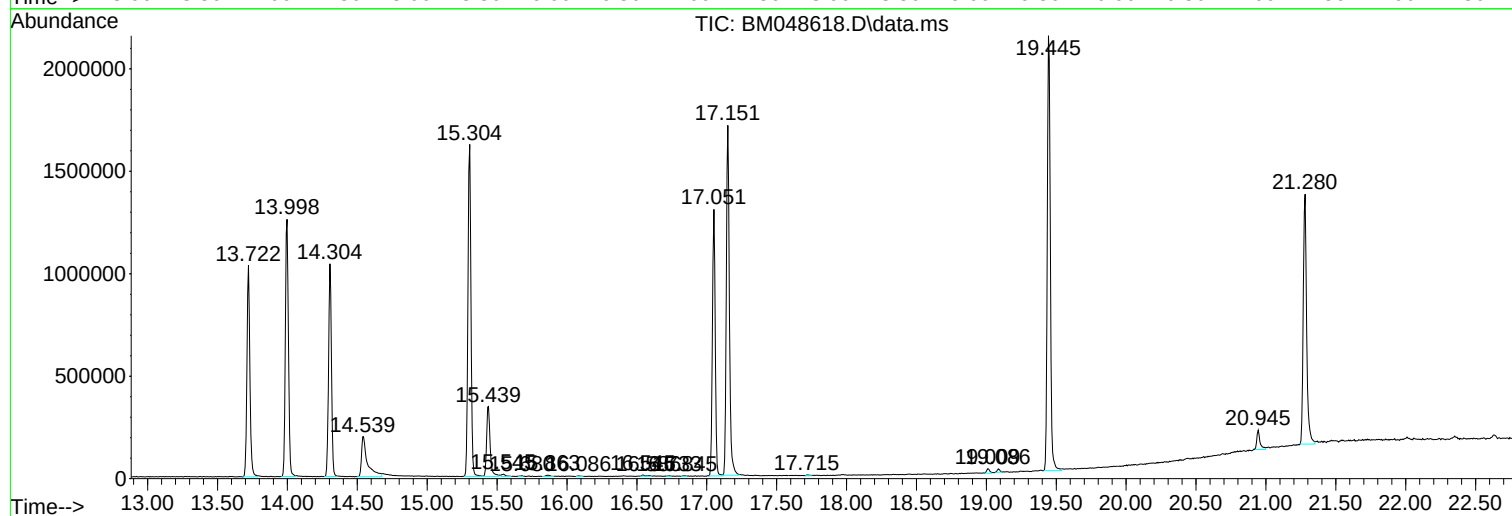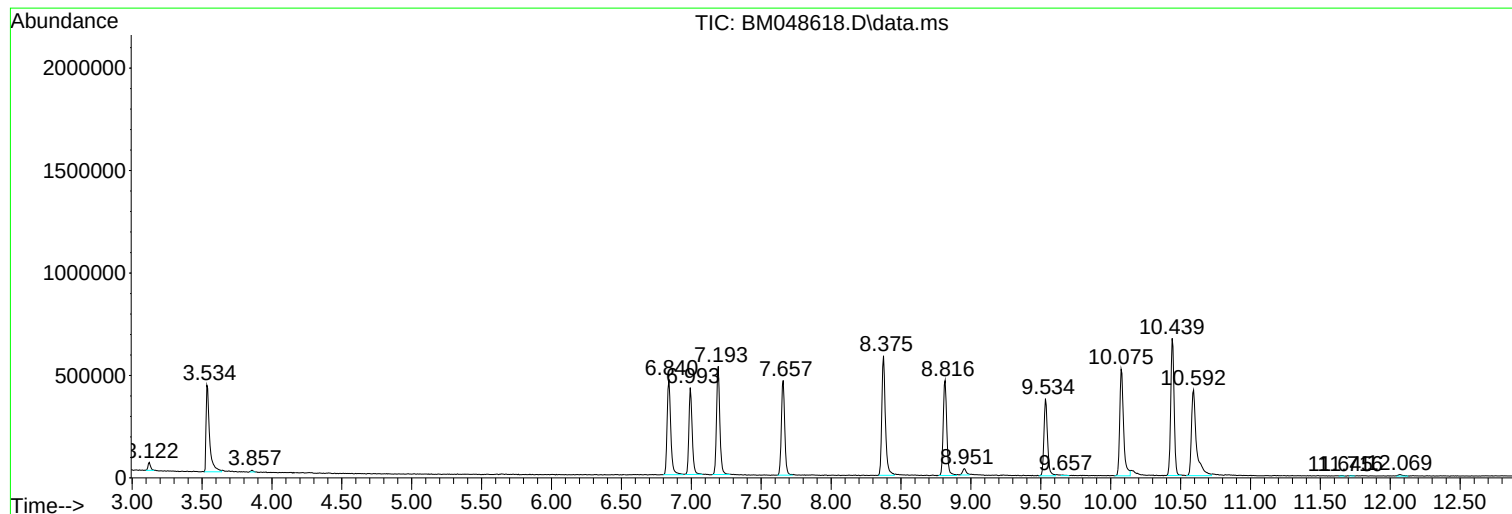

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048618.D
Acq On : 12 Nov 2024 13:25
Operator : RC/JU
Sample : PB164899BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048618.D
Acq On : 12 Nov 2024 13:25
Operator : RC/JU
Sample : PB164899BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc