
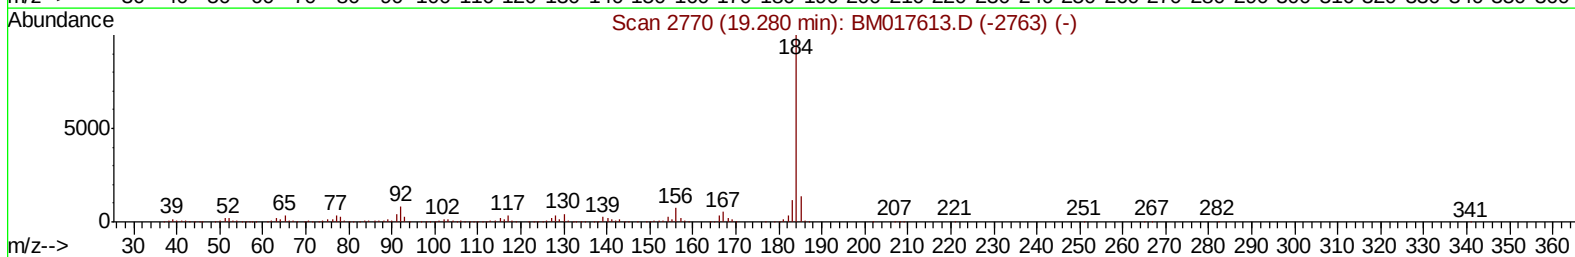
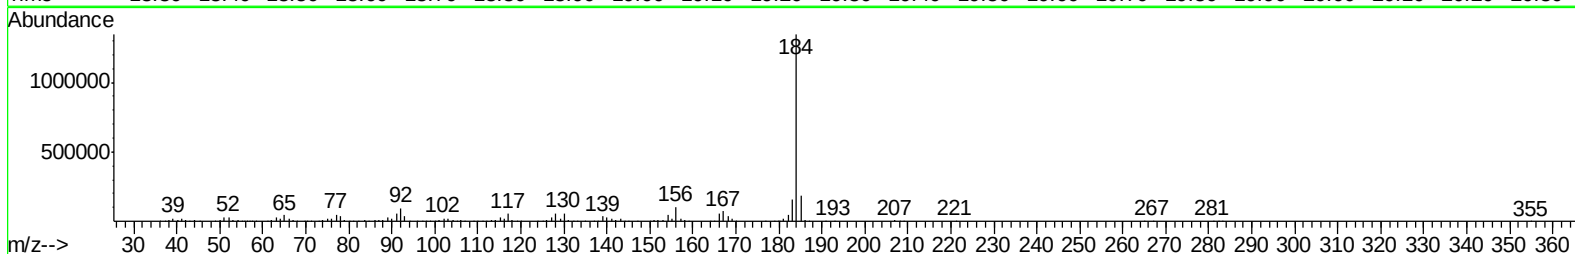


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111218\
 Data File : BM017608.D
 Acq On : 12 Nov 2018 11:38
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 08:23:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 12 18:37:25 2018
 Response via : Initial Calibration

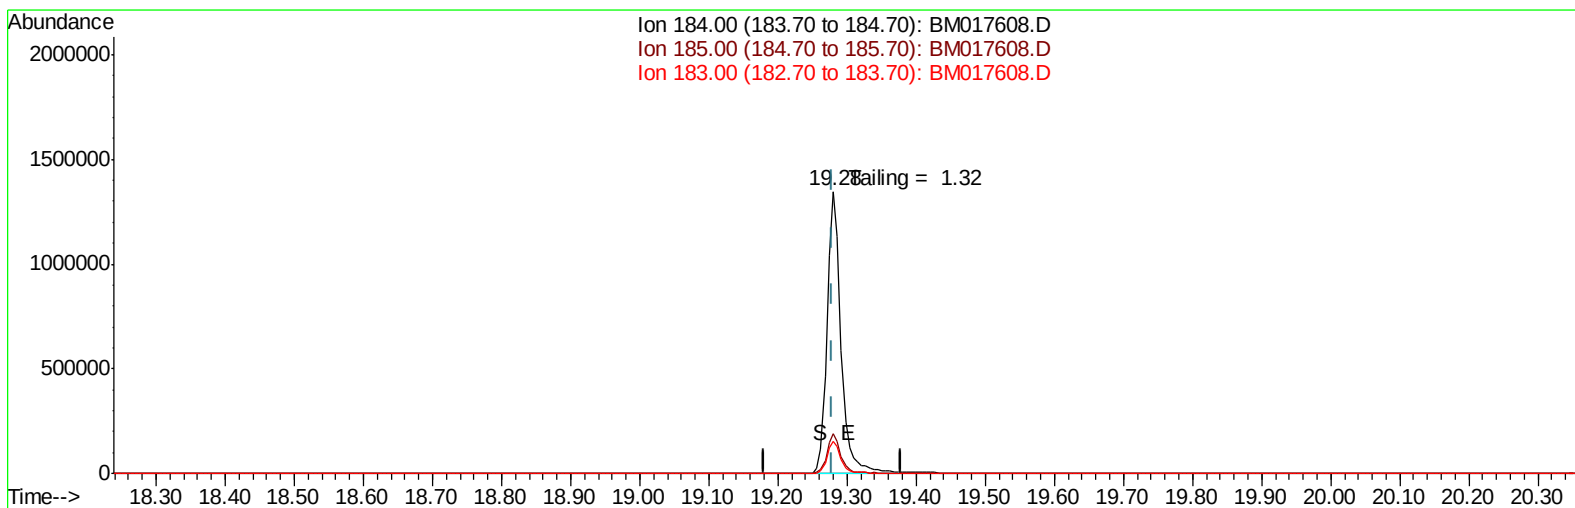

TIC: BM017608.D

(77) Benzidine




19.280min (-0.000) 0.00ng

response 1895834

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.00
183.00	11.90	11.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111218\
Data File : BM017608.D
Acq On : 12 Nov 2018 11:38
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 08:23:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

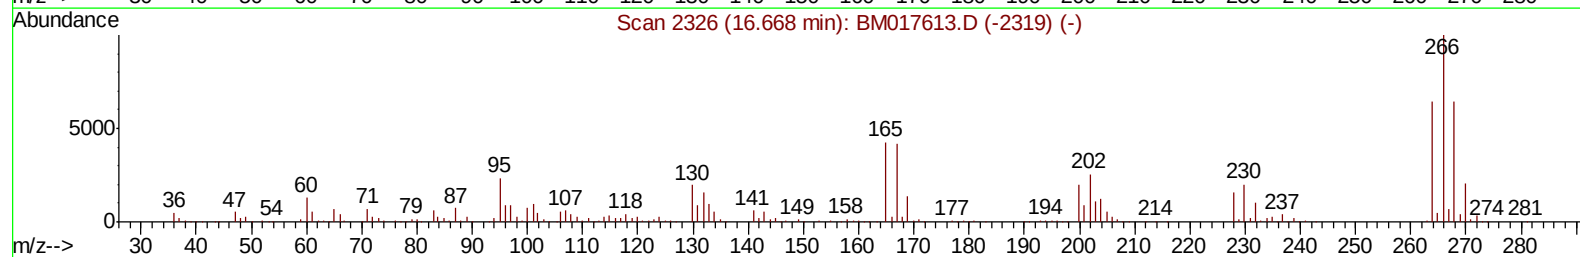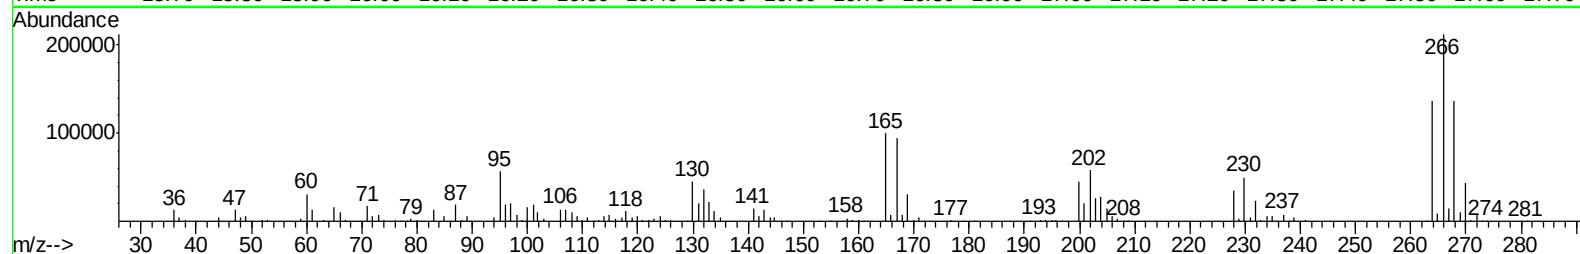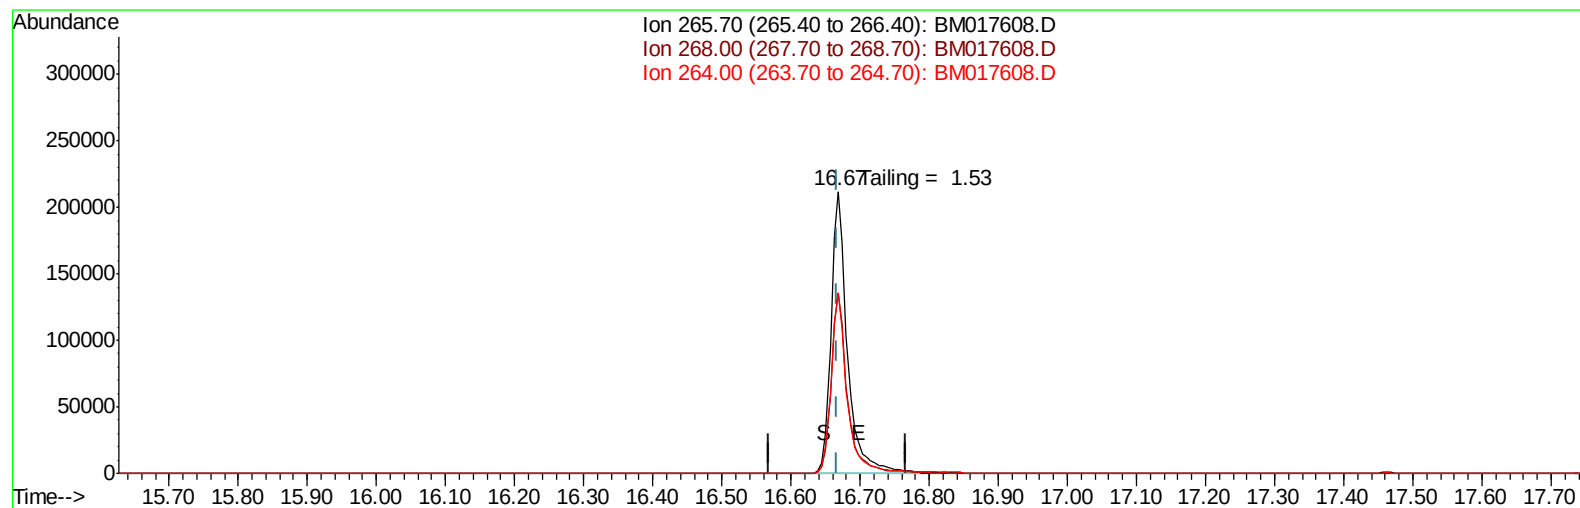

TIC: BM017608.D

(70) Pentachlorophenol (C)

16.668min (-0.000) 0.00ng

response 344501

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	64.32
264.00	64.10	64.23
0.00	0.00	0.00