


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111218\
 Data File : BM017608.D
 Acq On : 12 Nov 2018 11:38
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

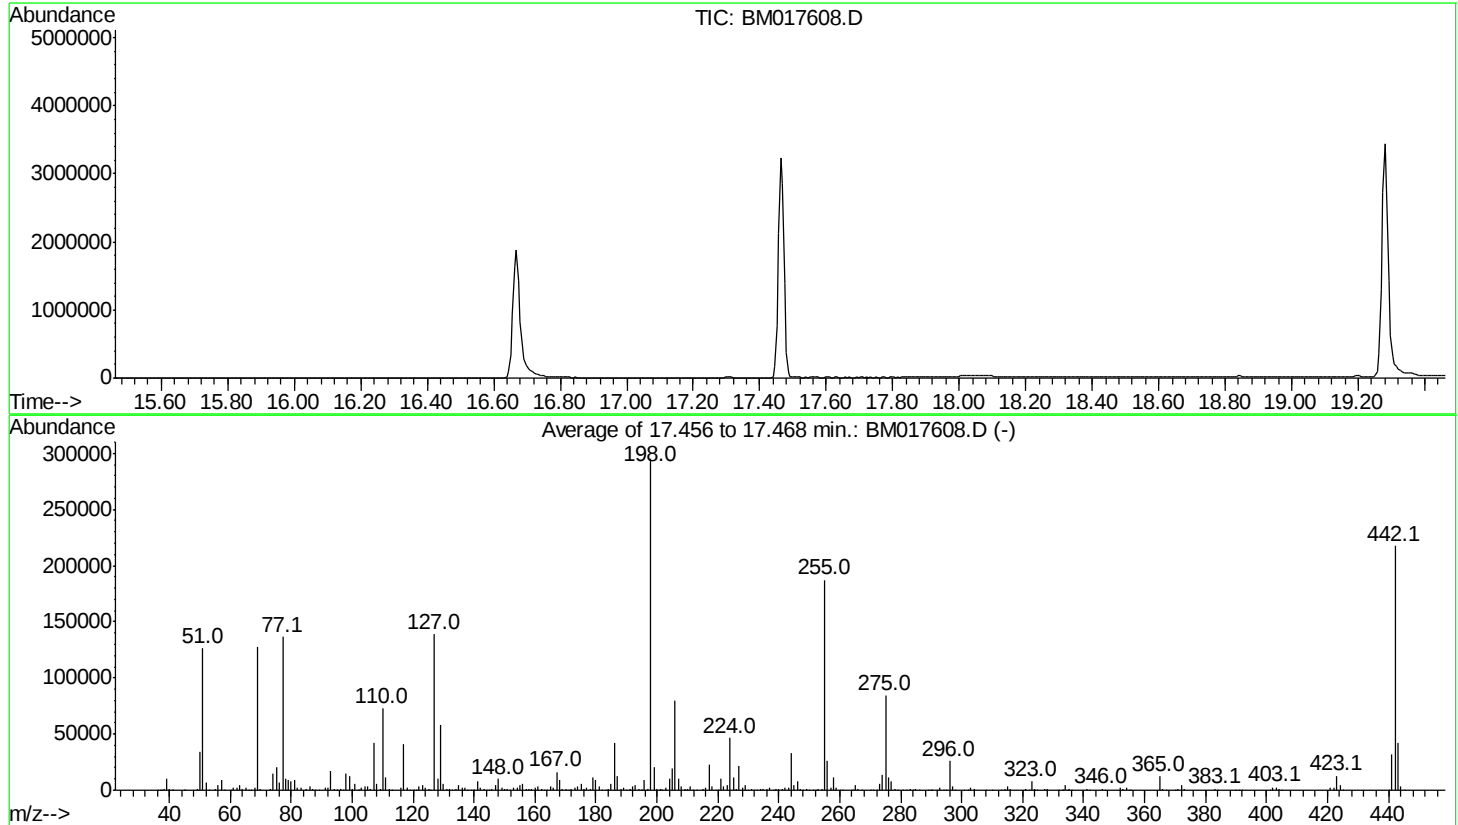

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	126309	PASS
68	69	0.00	2	1.9	2423	PASS
69	198	0.00	100	43.4	128218	PASS
70	69	0.00	2	0.6	811	PASS
127	198	10	80	47.0	138837	PASS
197	198	0.00	2	0.5	1370	PASS
198	198	100	100	100.0	295296	PASS
199	198	5	9	6.8	20033	PASS
275	198	10	60	28.5	84029	PASS
365	198	1	100	4.1	12108	PASS
441	198	0.01	100	10.9	32157	PASS
442	198	50	100	73.7	217584	PASS
443	442	15	24	19.2	41682	PASS