

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
 Data File : BM023686.D
 Acq On : 13 Nov 2019 04:37
 Operator : JU
 Sample : K5579-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 13 06:52:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 05:56:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	572402	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	2732529	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1985201	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	4509282	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	4076879	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	3691645	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.07	96	67570	4.87	ng/uL	0.00
5) Phenol-d5	6.73	99	395977	7.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	896932	29.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	1002087	26.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	715402	17.19	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	655537	33.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	778683	37.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	1403730	29.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	99694	1.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	4925787	31.82	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	5692070	32.22	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	178914	6.77	ng/ul	0.00
58) Fluorene-d10	15.20	176	4300277	31.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	758630	29.08	ng/ul	0.00
71) Anthracene-d10	17.04	188	6701027	31.33	ng/ul	0.00
79) Pyrene-d10	19.35	212	7717139	36.30	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	6528886	33.61	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.66	163	370645	2.443	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
Data File : BM023686.D
Acq On : 13 Nov 2019 04:37
Operator : JU
Sample : K5579-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 13 06:52:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 05:56:01 2019
Response via : Initial Calibration

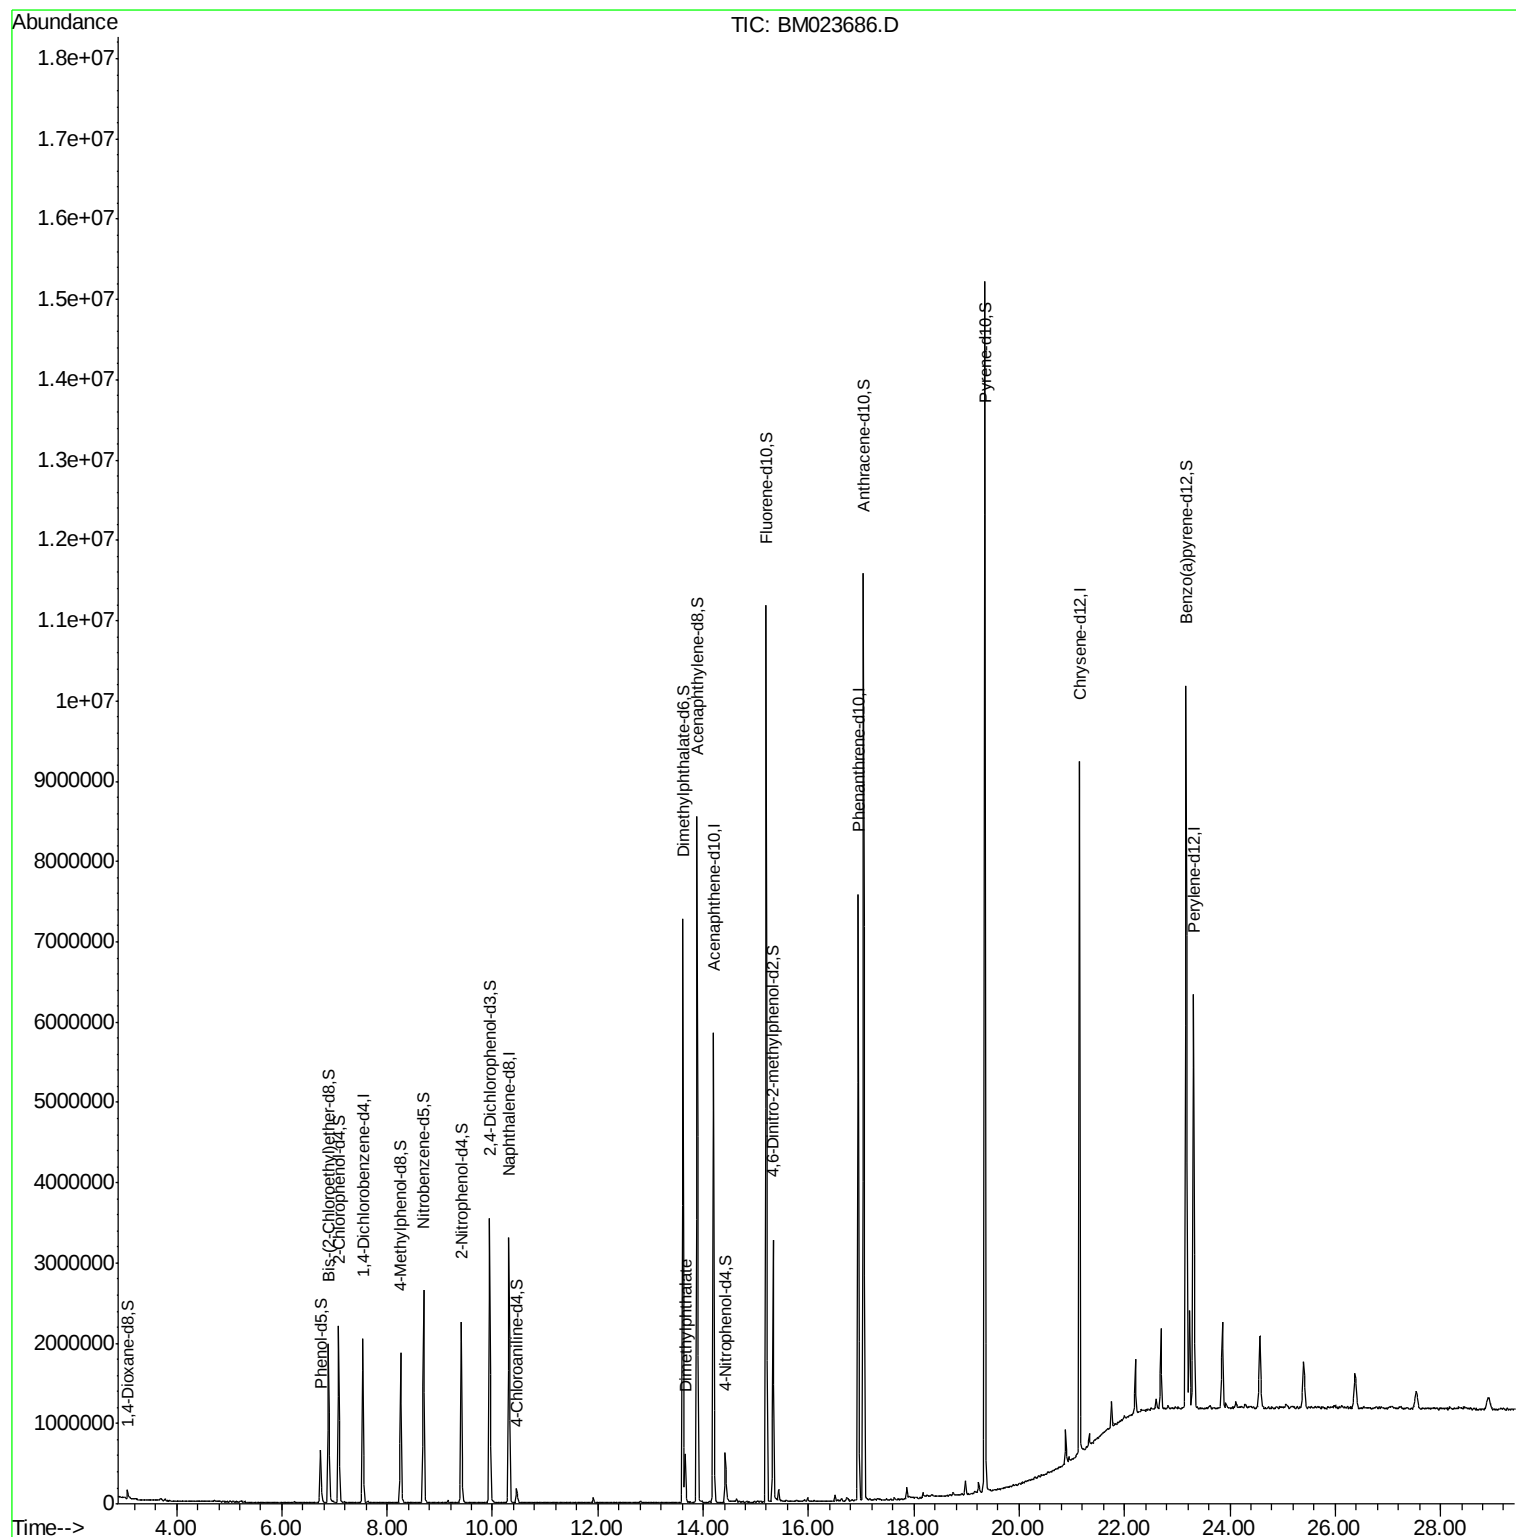

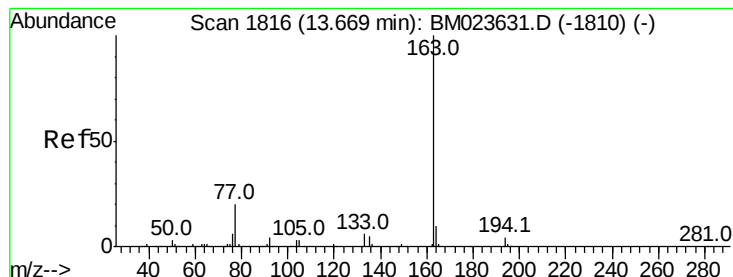

#45

Dimethylphthalate

Concen: 2.443 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM023686.D

Acq: 13 Nov 2019 04:37

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 370645

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 11.0 8.0 12.0

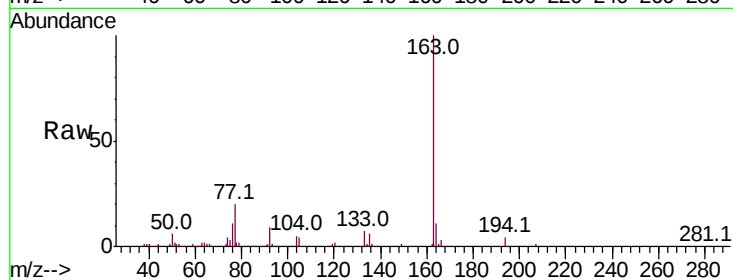

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

