

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
 Data File : BM023663.D
 Acq On : 12 Nov 2019 14:15
 Operator : JU
 Sample : K5559-03DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CP8DL

Quant Time: Nov 12 14:49:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 05:56:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	377144	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1713940	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1259581	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	2894026	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	2841382	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2740925	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.07	96	213	0.02	ng/uL	0.00
5) Phenol-d5	6.73	99	36023	1.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	110789	5.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	108406	4.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	71783	2.62	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	64619	5.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	71436	5.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	144815	4.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	13143	0.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	630703	6.42	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	624501	5.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	13574	0.81	ng/ul	0.00
58) Fluorene-d10	15.20	176	544278	6.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	65145	3.89	ng/ul	0.00
71) Anthracene-d10	17.04	188	963864	7.02	ng/ul	0.00
79) Pyrene-d10	19.35	212	1151501	7.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1029419	7.14	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) Nitrobenzene	8.73	77	733952	22.627	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	12.99	216	48644	1.186	ng/uL	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
Data File : BM023663.D
Acq On : 12 Nov 2019 14:15
Operator : JU
Sample : K5559-03DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CP8DL

Quant Time: Nov 12 14:49:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 05:56:01 2019
Response via : Initial Calibration




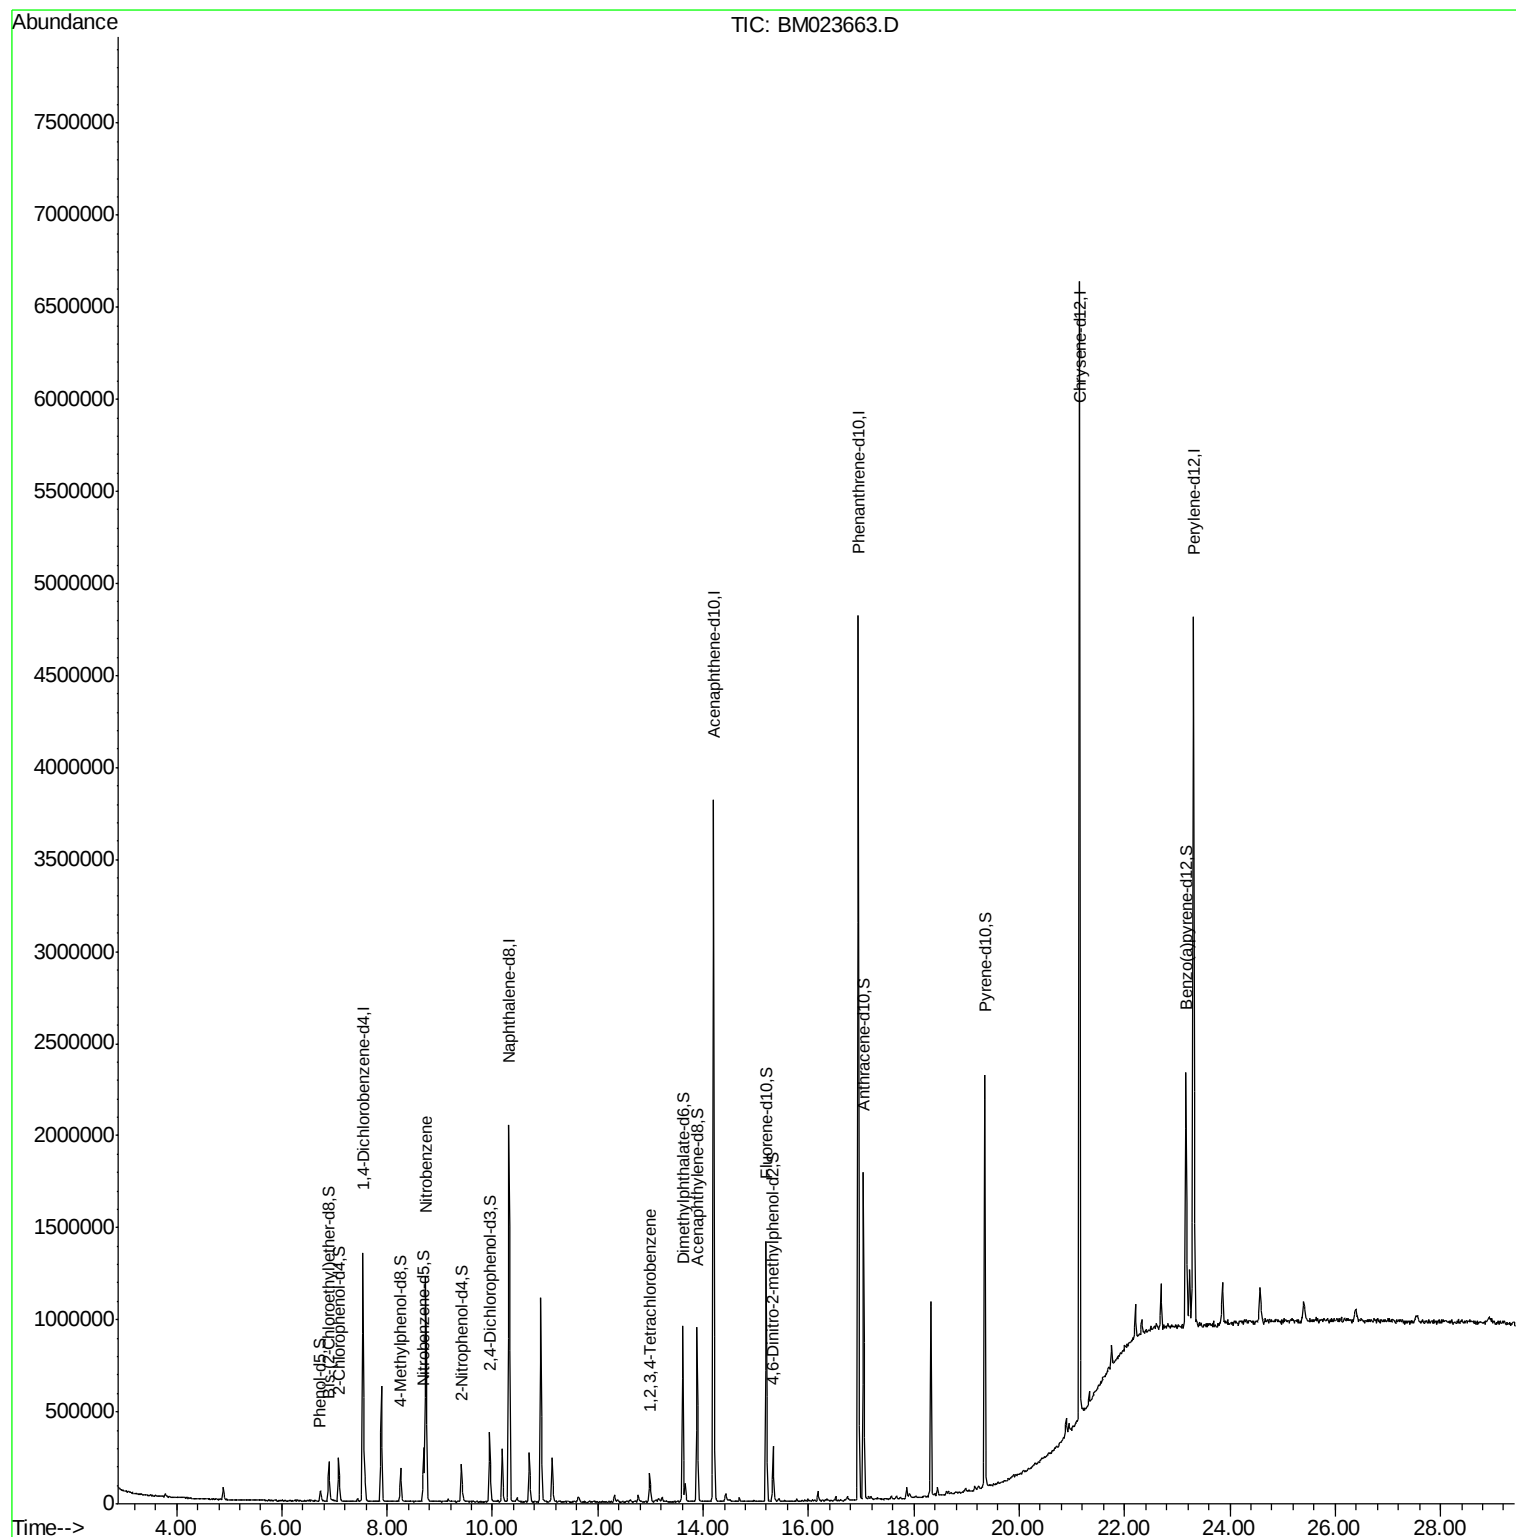


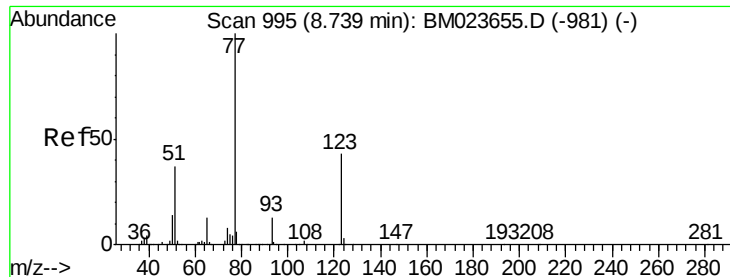

#20
Nitrobenzene
Concen: 22.627 ng/ul
RT: 8.73 min Scan# 994
Delta R.T. -0.01 min
Lab File: BM023663.D
Acq: 12 Nov 2019 14:15

Instrument :
BNA_M
ClientSampleId :
C0CP8DL

Tot Ion	Ratio	Lower	Upper
77	100		
123	41.1	33.1	49.7
65	12.6	9.8	14.8

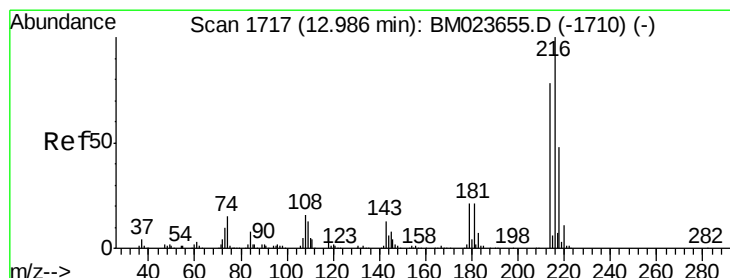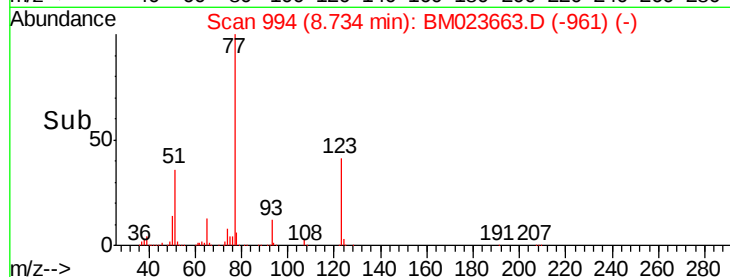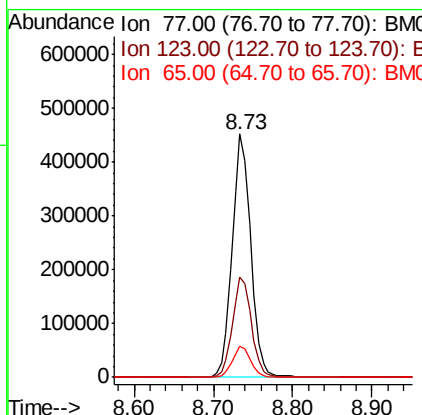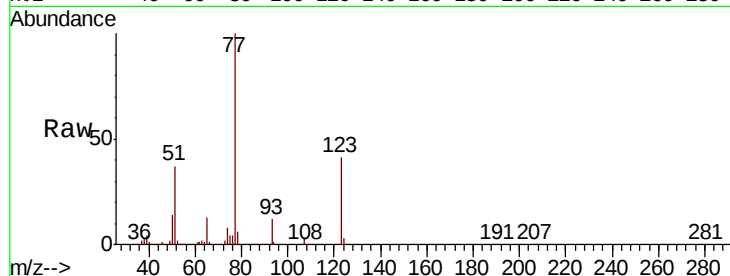

#73
1,2,3,4-Tetrachlorobenzene
Concen: 1.186 ng/uL
RT: 12.99 min Scan# 1717
Delta R.T. -0.01 min
Lab File: BM023663.D
Acq: 12 Nov 2019 14:15

Tgt Ion	Ratio	Lower	Upper
216	100		
214	79.0	63.1	94.7
218	47.5	38.6	57.8

