

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
 Data File : BM023664.D
 Acq On : 12 Nov 2019 14:51
 Operator : JU
 Sample : K5559-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CQ1

Quant Time: Nov 12 15:23:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 05:56:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	354858	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1618856	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1179746	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	2701460	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2542848	20.00	ng/ul	-0.01
86) Perylene-d12	23.31	264	2400536	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	2786	0.32	ng/uL	0.01
5) Phenol-d5	6.73	99	436970	13.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	405545	21.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	455123	19.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	449460	17.42	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	255557	22.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	287074	23.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	571541	20.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	490989	16.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	2291460	24.91	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	2549151	24.28	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	178040	11.34	ng/ul	0.00
58) Fluorene-d10	15.20	176	1986935	24.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	309306	19.79	ng/ul	0.00
71) Anthracene-d10	17.04	188	3465725	27.04	ng/ul	0.00
79) Pyrene-d10	19.35	212	3915190	29.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3466419	27.44	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.66	163	134059	1.487	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
Data File : BM023664.D
Acq On : 12 Nov 2019 14:51
Operator : JU
Sample : K5559-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CQ1

Quant Time: Nov 12 15:23:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 05:56:01 2019
Response via : Initial Calibration

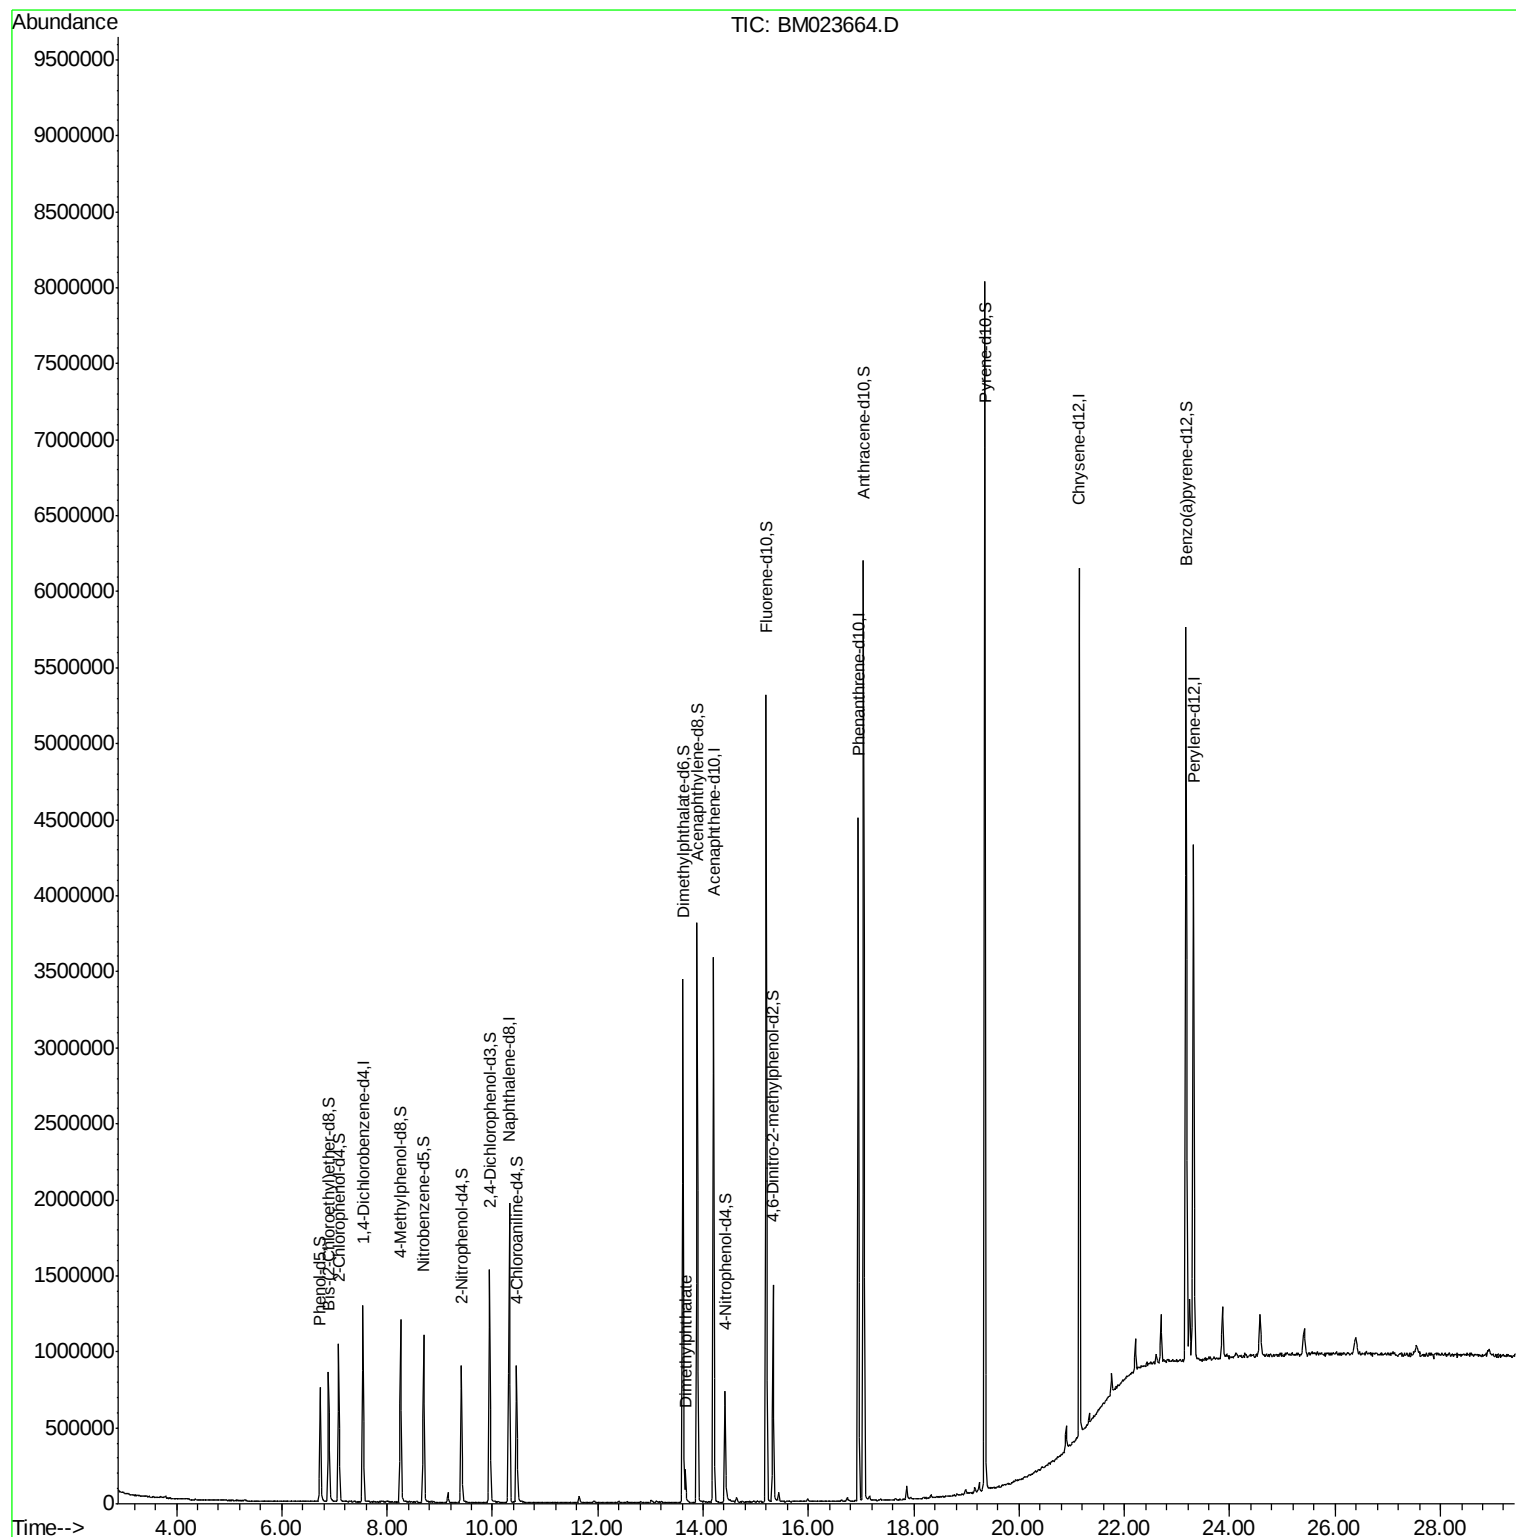

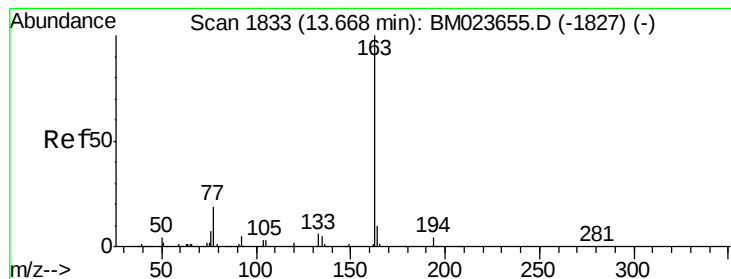

#45

Dimethylphthalate

Concen: 1.487 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM023664.D

Acq: 12 Nov 2019 14:51

Instrument :

BNA_M

ClientSampleId :

C0CQ1


Tot Ion:163 Resp: 134059

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.2

164 10.1 8.0 12.0

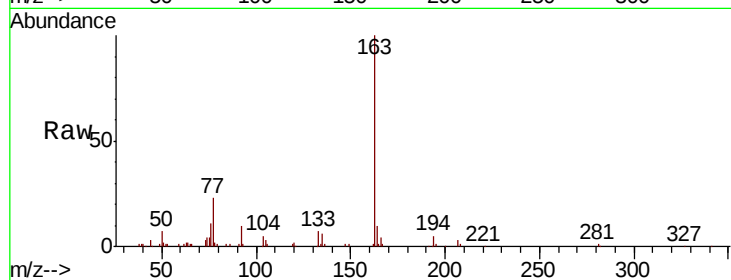

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

