

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
 Data File : BM023671.D
 Acq On : 12 Nov 2019 19:03
 Operator : JU
 Sample : K5565-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNA4

Quant Time: Nov 13 00:05:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 05:56:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	783333	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	3312222	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	2229942	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	4604325	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	2874003	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2976873	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	35118	1.85	ng/uL	0.00
5) Phenol-d5	6.73	99	844460	11.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	527306	12.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	680950	13.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	721563	12.67	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	359615	15.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	410761	16.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	795538	14.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	448688	7.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	2643104	15.20	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	3065181	15.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	212066	7.14	ng/ul	0.00
58) Fluorene-d10	15.20	176	2306025	15.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	296596	11.14	ng/ul	0.00
71) Anthracene-d10	17.04	188	3307633	15.14	ng/ul	0.00
79) Pyrene-d10	19.35	212	3064511	20.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2455275	15.67	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.67	163	522858	3.068	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
Data File : BM023671.D
Acq On : 12 Nov 2019 19:03
Operator : JU
Sample : K5565-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNA4

Quant Time: Nov 13 00:05:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 05:56:01 2019
Response via : Initial Calibration

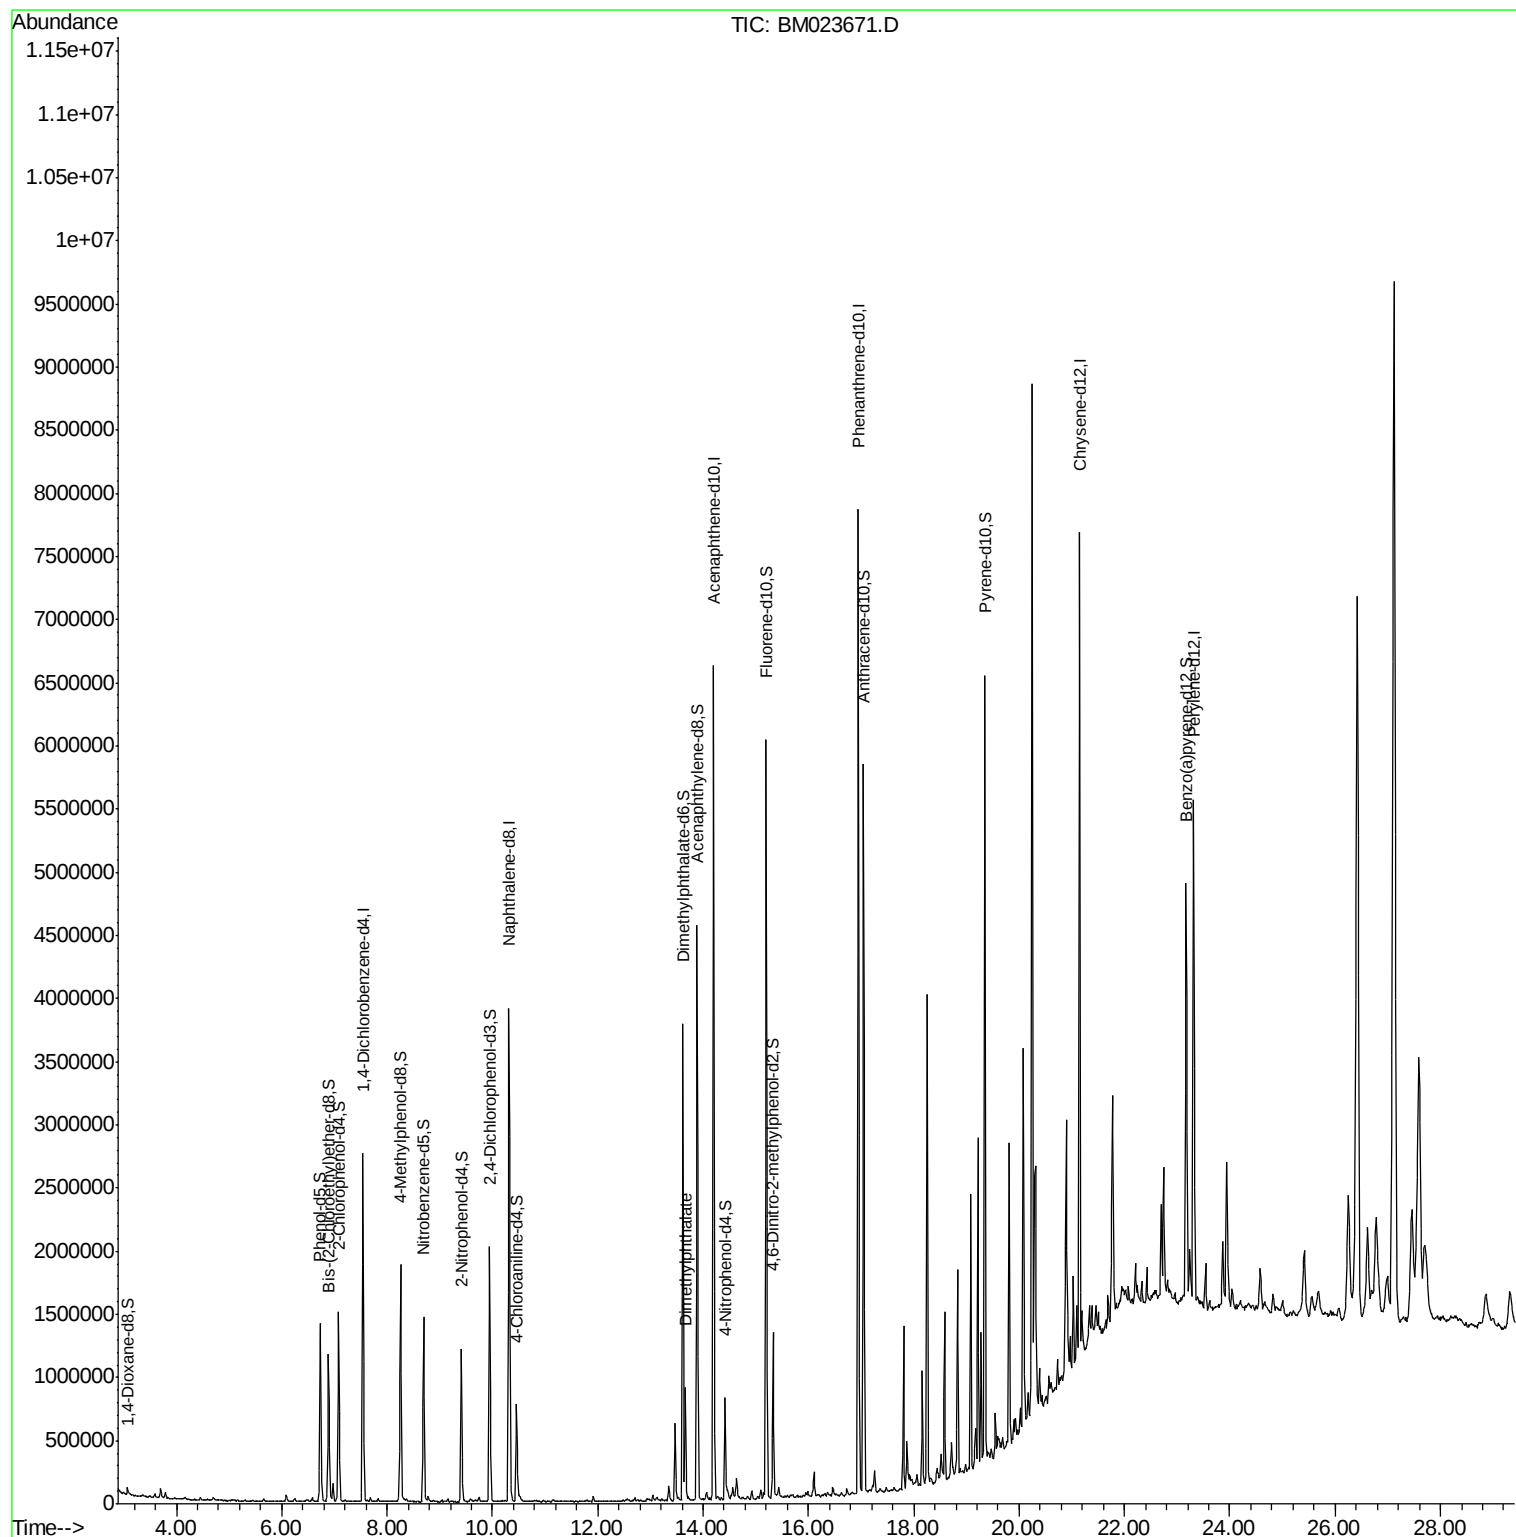

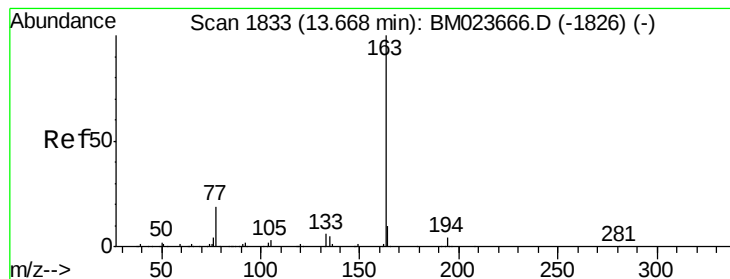

#45

Dimethylphthalate

Concen: 3.068 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: BM023671.D

Acq: 12 Nov 2019 19:03

Instrument :

BNA_M

ClientSampleId :

JLNA4



Tot Ion:163 Resp: 522858

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 9.9 8.0 12.0

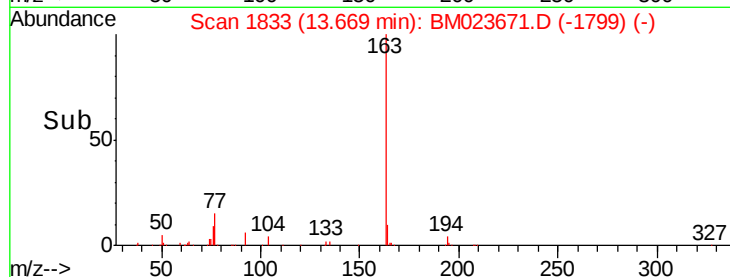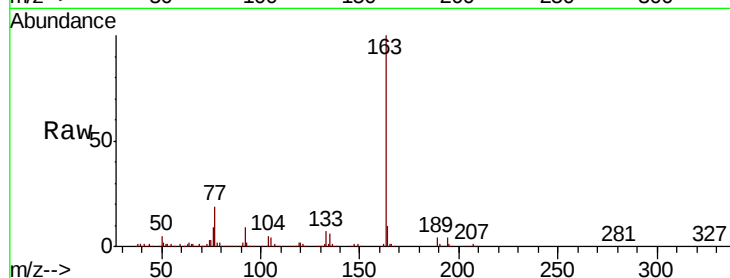

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

