

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
 Data File : BM023676.D
 Acq On : 12 Nov 2019 22:03
 Operator : JU
 Sample : K5565-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLN6

Quant Time: Nov 13 00:06:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 05:56:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	412527	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1918364	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1417657	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	3215754	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2724117	20.00	ng/ul	-0.01
86) Perylene-d12	23.31	264	2460404	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	23123	2.31	ng/uL	0.00
5) Phenol-d5	6.73	99	494089	13.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	310526	14.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	384906	14.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	330206	11.01	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	198293	14.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	221394	15.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	434536	13.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	533509	14.76	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	1610690	14.57	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1743746	13.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	207861	11.01	ng/ul	0.00
58) Fluorene-d10	15.20	176	1369022	14.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	184173	9.90	ng/ul	0.00
71) Anthracene-d10	17.04	188	2228449	14.61	ng/ul	0.00
79) Pyrene-d10	19.35	212	2587274	18.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2032589	15.70	ng/ul	-0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.66	163	294941	2.722	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
Data File : BM023676.D
Acq On : 12 Nov 2019 22:03
Operator : JU
Sample : K5565-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNB6

Quant Time: Nov 13 00:06:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 05:56:01 2019
Response via : Initial Calibration

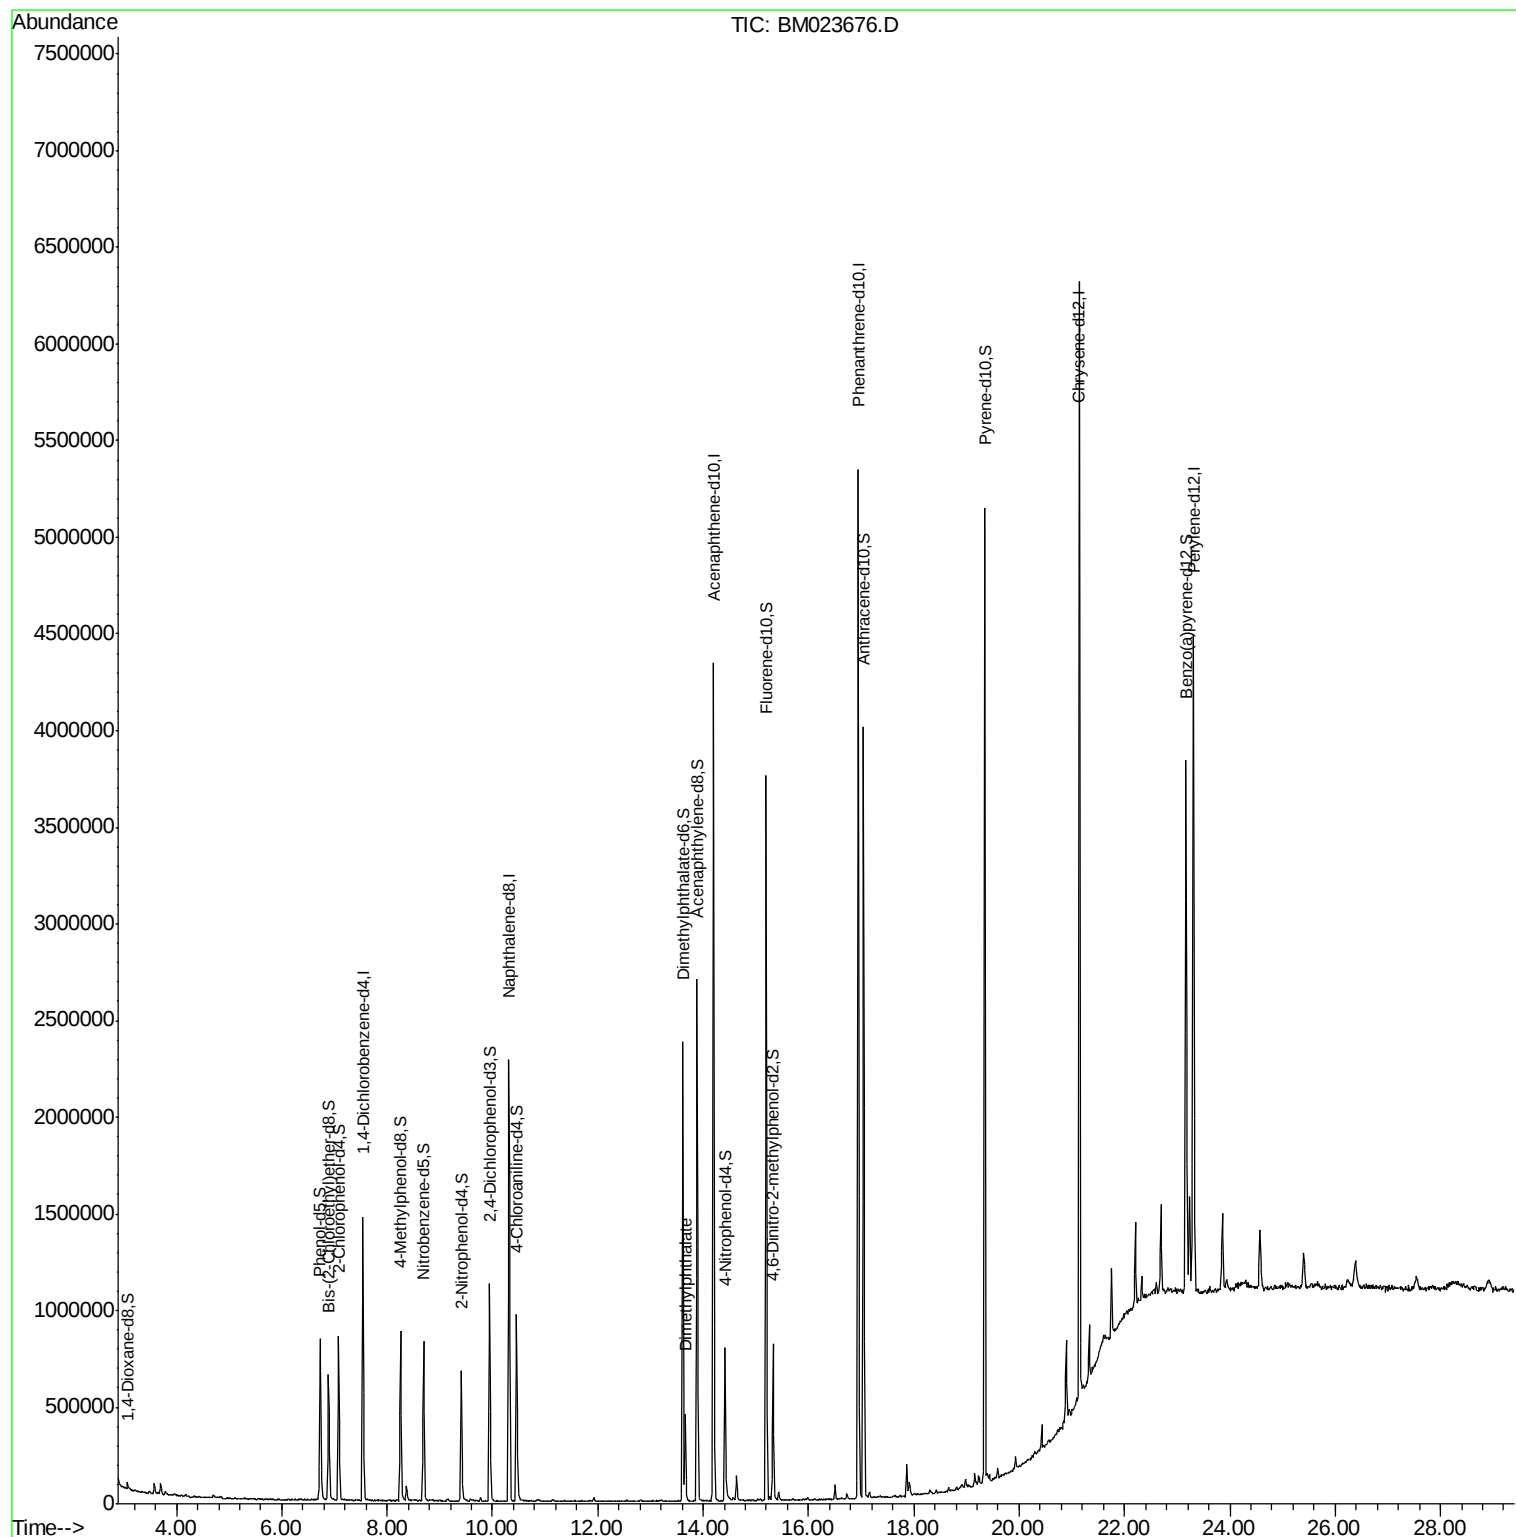

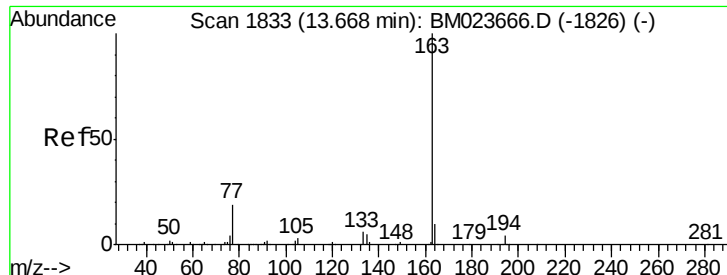

#45

Dimethylphthalate

Concen: 2.722 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM023676.D

Acq: 12 Nov 2019 22:03

Instrument :

BNA_M

ClientSampleId :

JLNB6

Tot Ion:163 Resp: 294941

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.2

164 10.3 8.0 12.0

