

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
 Data File : BM023677.D
 Acq On : 12 Nov 2019 22:39
 Operator : JU
 Sample : K5565-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLN87

Quant Time: Nov 13 00:06:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 05:56:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	403962	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1852485	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1337564	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	3018758	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2420175	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	2218137	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	46997	4.80	ng/uL	0.00
5) Phenol-d5	6.73	99	951888	25.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	588682	27.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	734455	27.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	799641	27.22	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	386723	29.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	437742	31.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	844417	26.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	1158310	33.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	2925656	28.05	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	3312910	27.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	381587	21.43	ng/ul	0.00
58) Fluorene-d10	15.20	176	2546351	27.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	343058	19.65	ng/ul	0.00
71) Anthracene-d10	17.04	188	3989517	27.86	ng/ul	0.00
79) Pyrene-d10	19.35	212	4212713	33.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3283847	28.13	ng/ul	-0.02


Target Compounds					Ovalue	
6) Phenol	6.75	94	76673	2.021	ng/ul	97
45) Dimethylphthalate	13.66	163	1021786	9.996	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111219\
Data File : BM023677.D
Acq On : 12 Nov 2019 22:39
Operator : JU
Sample : K5565-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNB7

Quant Time: Nov 13 00:06:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 05:56:01 2019
Response via : Initial Calibration

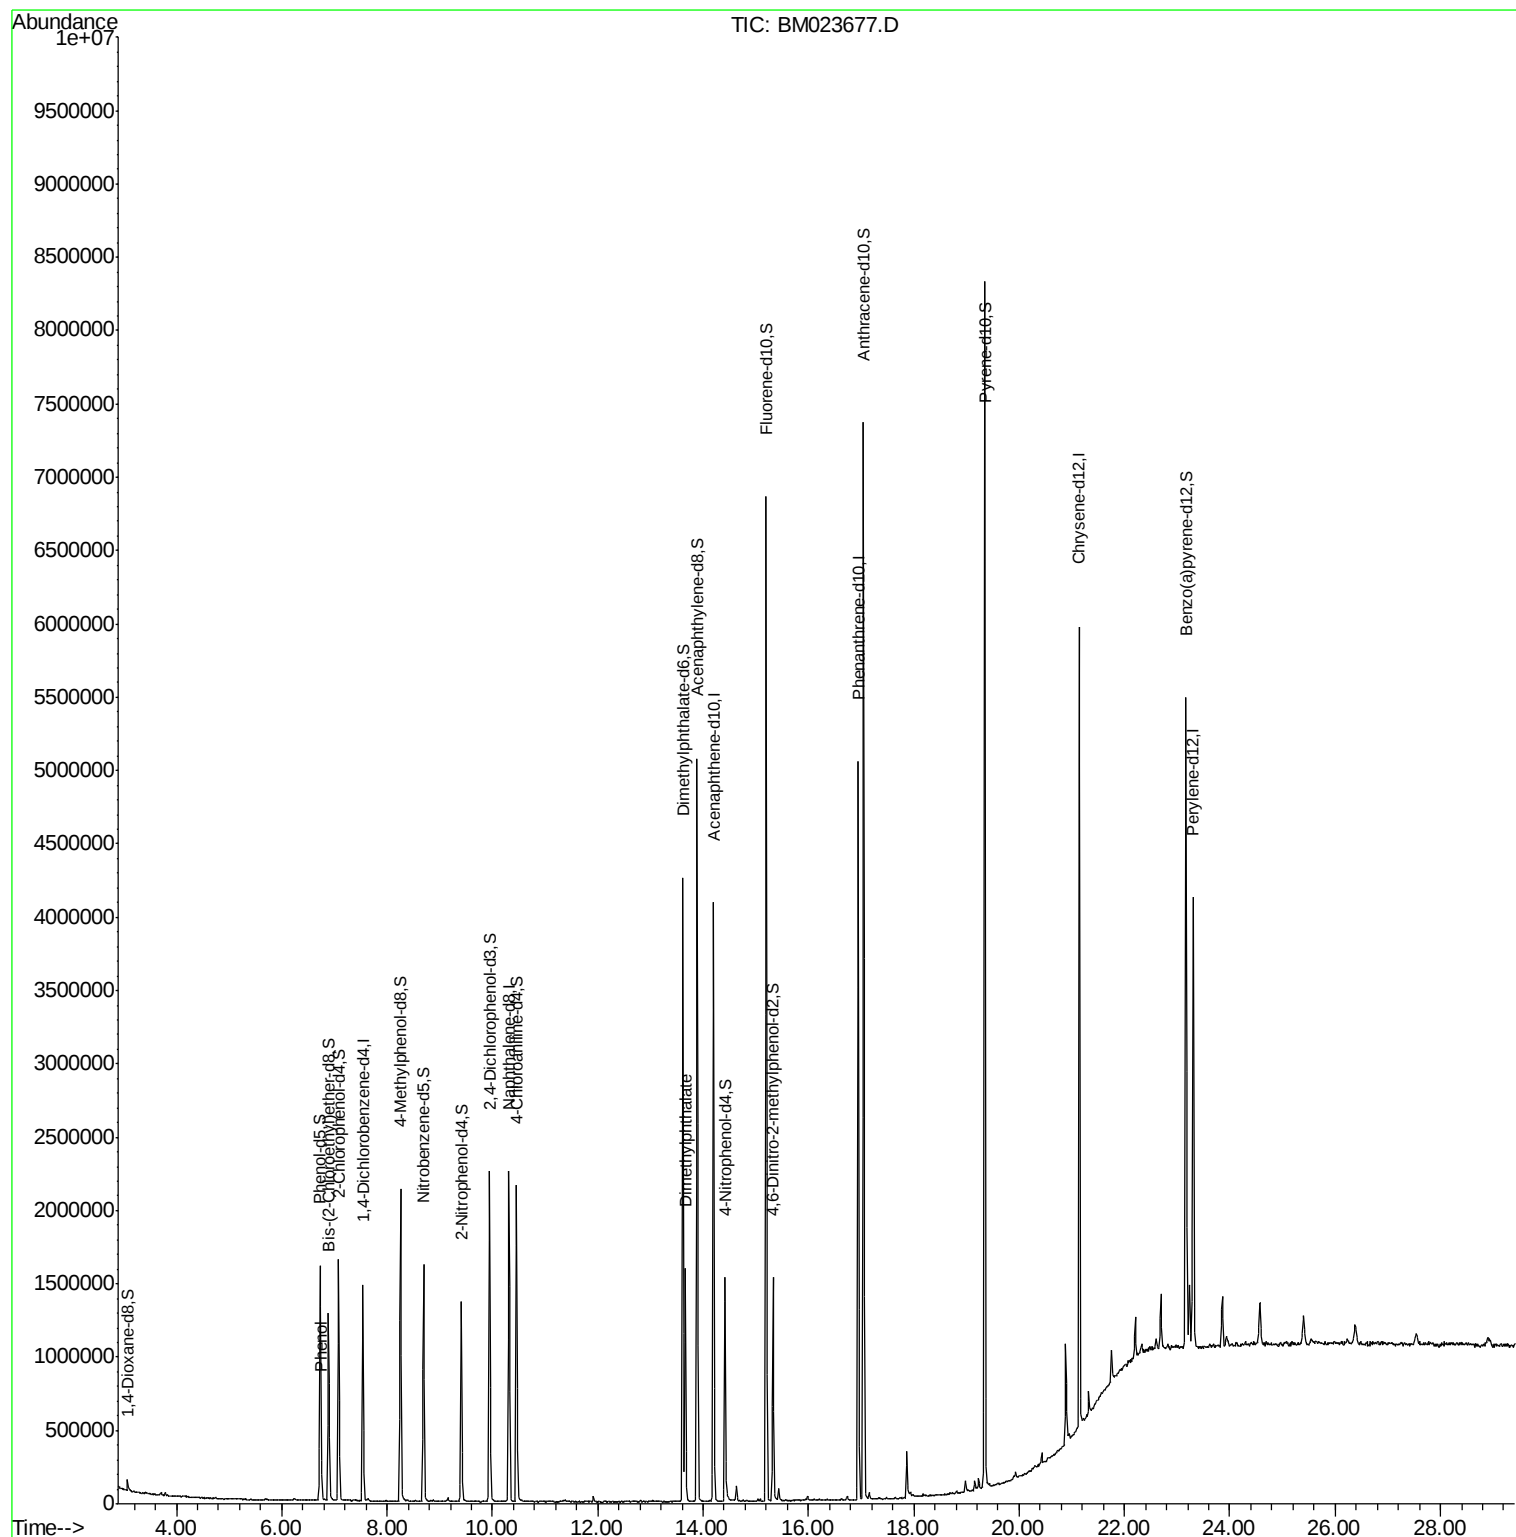

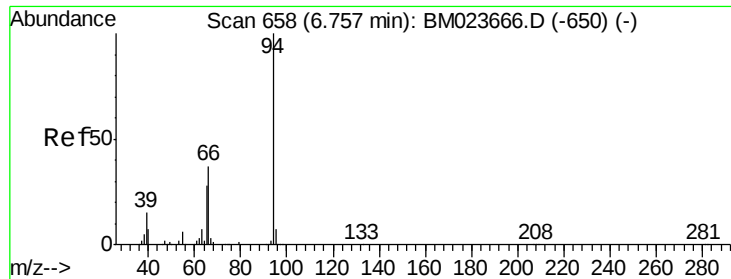





#6

Phenol

Concen: 2.021 ng/ul
 RT: 6.75 min Scan# 657
 Delta R.T. -0.01 min
 Lab File: BM023677.D
 Acq: 12 Nov 2019 22:39

Instrument :
 BNA_M
 ClientSampleId :
 JLN7

Tot Ion: 94 Resp: 76673
 Ion Ratio Lower Upper
 94 100
 65 28.9 21.4 32.2
 66 40.2 30.7 46.1

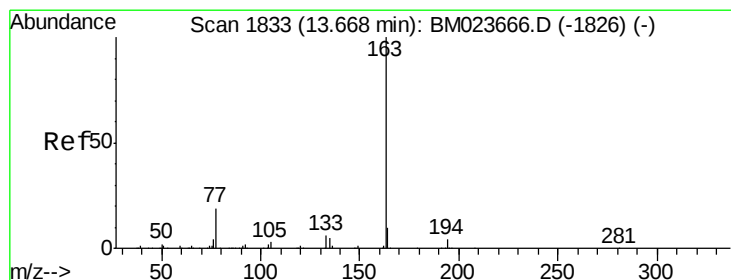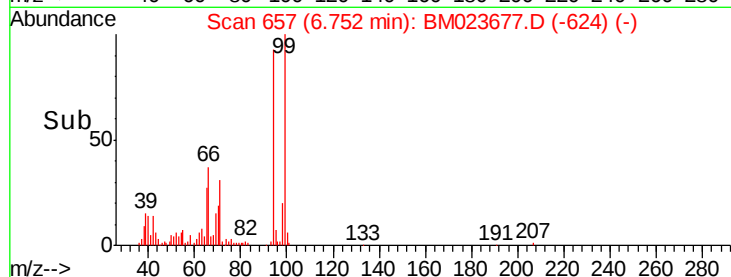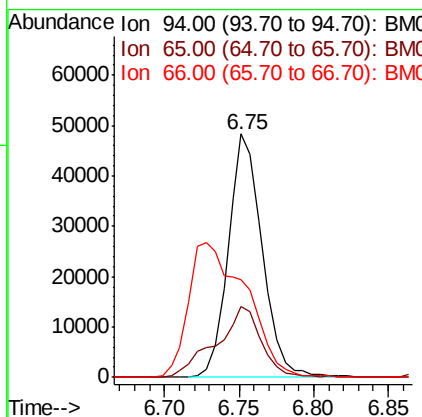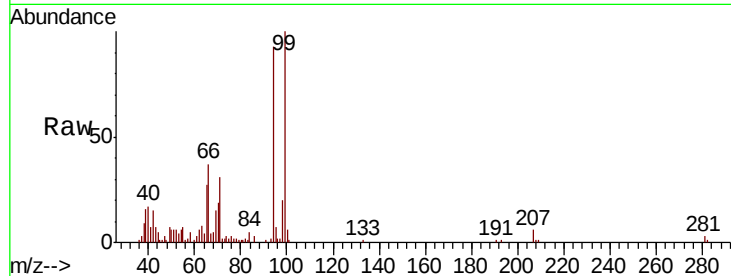

#45

Dimethylphthalate

Concen: 9.996 ng/ul
 RT: 13.66 min Scan# 1832
 Delta R.T. -0.01 min
 Lab File: BM023677.D
 Acq: 12 Nov 2019 22:39

Tgt Ion: 163 Resp: 1021786
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.4 5.2
 164 10.4 8.0 12.0

