
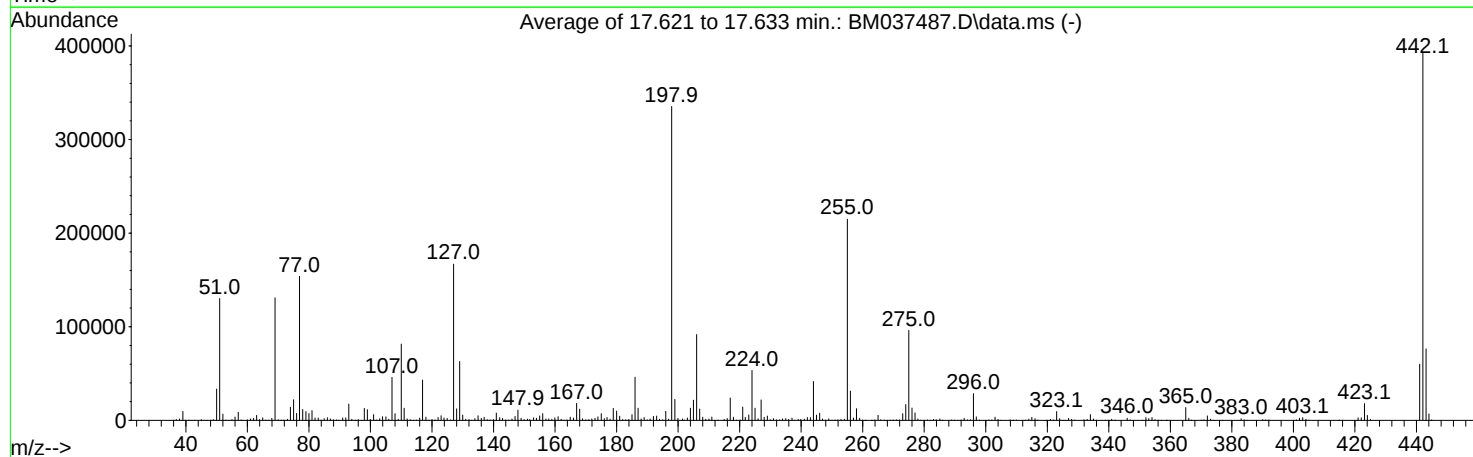


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111222\
 Data File : BM037487.D
 Acq On : 12 Nov 2022 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 14 01:42:00 2022

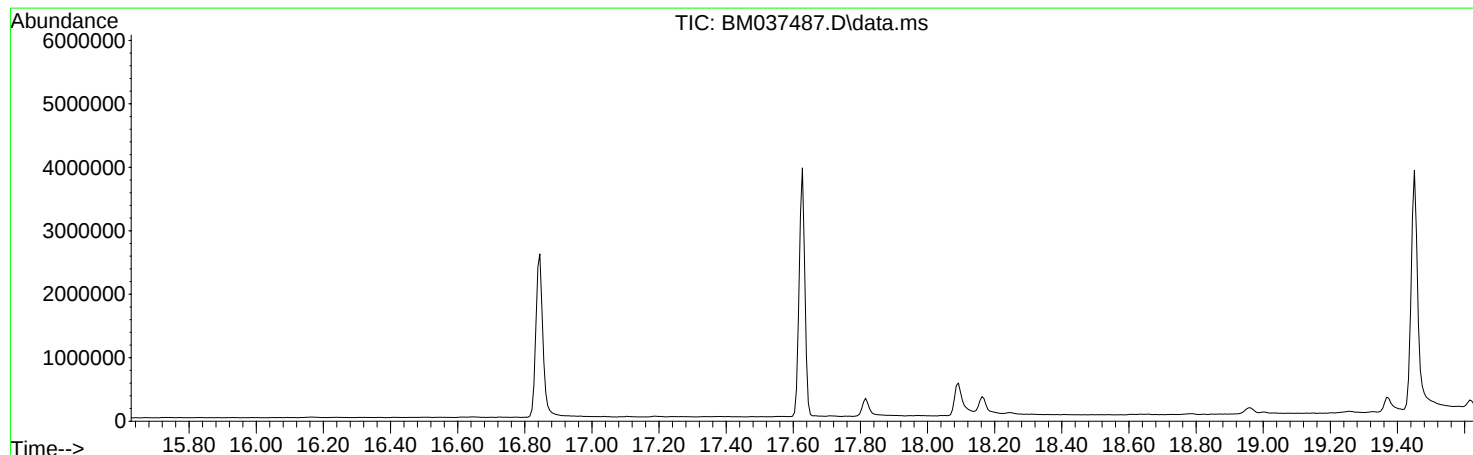




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	130077	PASS
68	69	0.00	2	1.7	2167	PASS
69	198	0.00	100	39.1	130951	PASS
70	69	0.00	2	0.5	618	PASS
127	198	10	80	49.7	166811	PASS
197	198	0.00	2	0.4	1356	PASS
198	198	100	100	100.0	335339	PASS
199	198	5	9	6.7	22403	PASS
275	198	10	60	28.6	96037	PASS
365	198	1	100	4.0	13547	PASS
441	198	0.01	100	17.9	59872	PASS
442	442	50	100	100.0	393109	PASS
443	442	15	24	19.4	76309	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111222\
Data File : BM037487.D
Acq On : 12 Nov 2022 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 14 08:16:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 01:42:00 2022
Response via : Initial Calibration

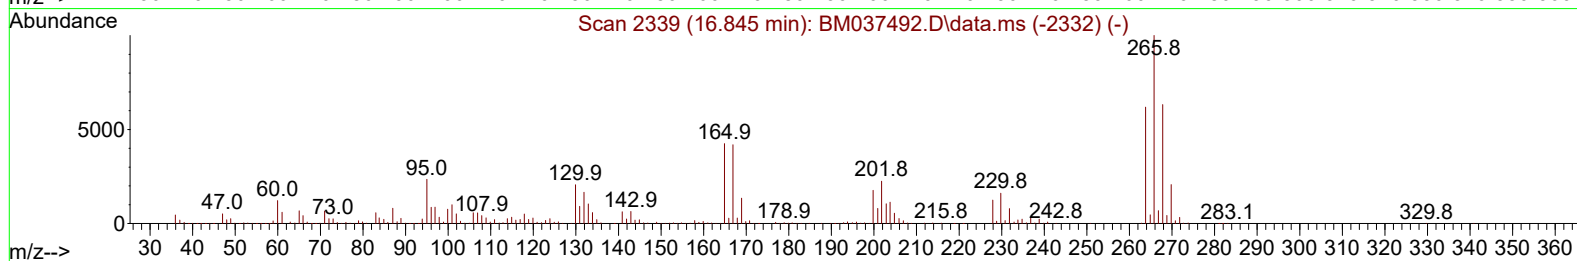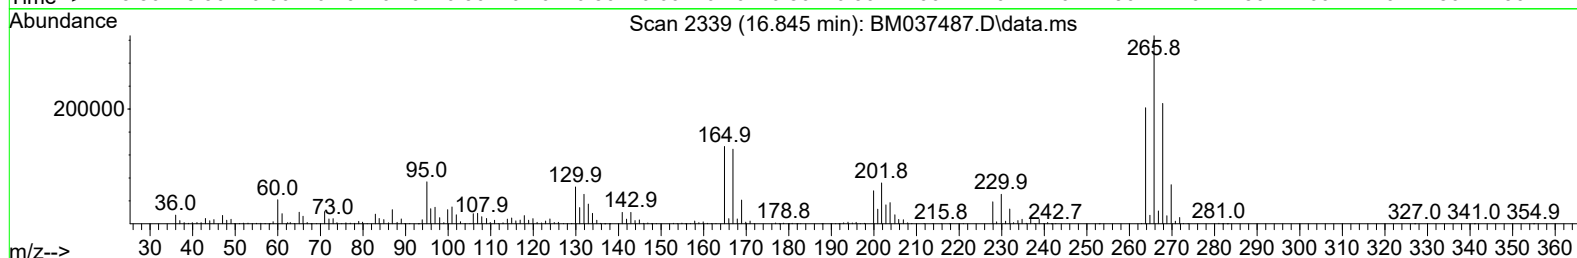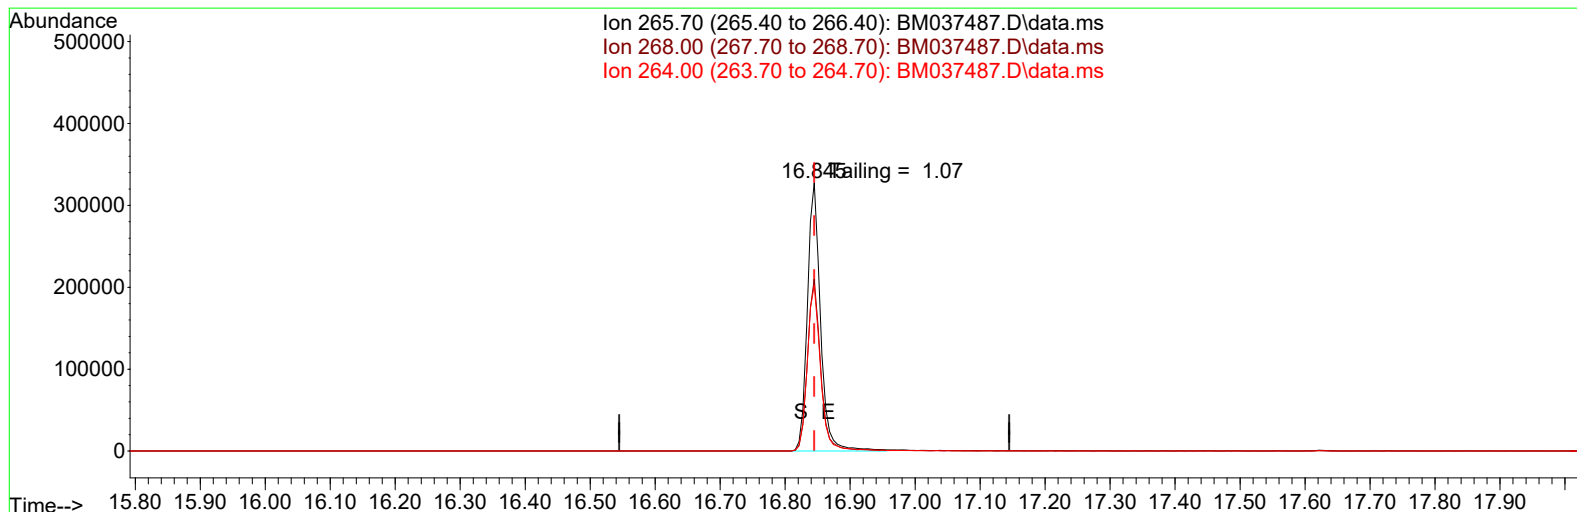

TIC: BM037487.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.000) 702026.83 ng




response 467513

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.02
264.00	61.90	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111222\
Data File : BM037487.D
Acq On : 12 Nov 2022 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 14 08:16:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 01:42:00 2022
Response via : Initial Calibration

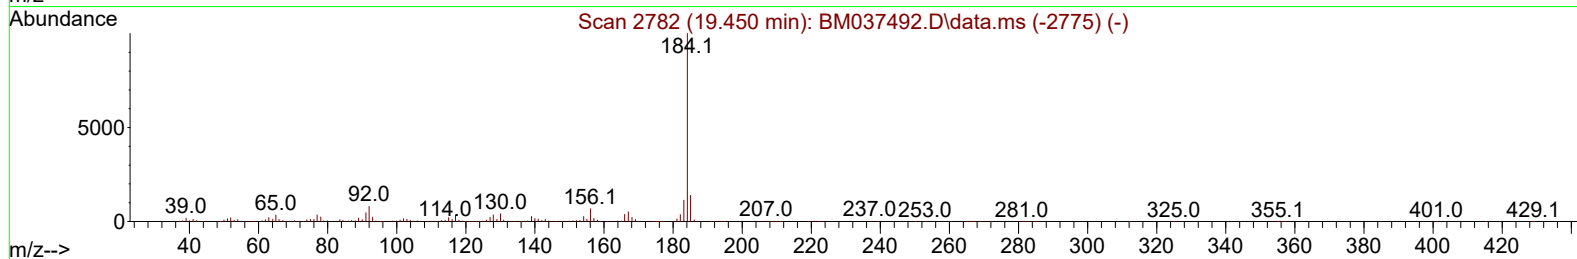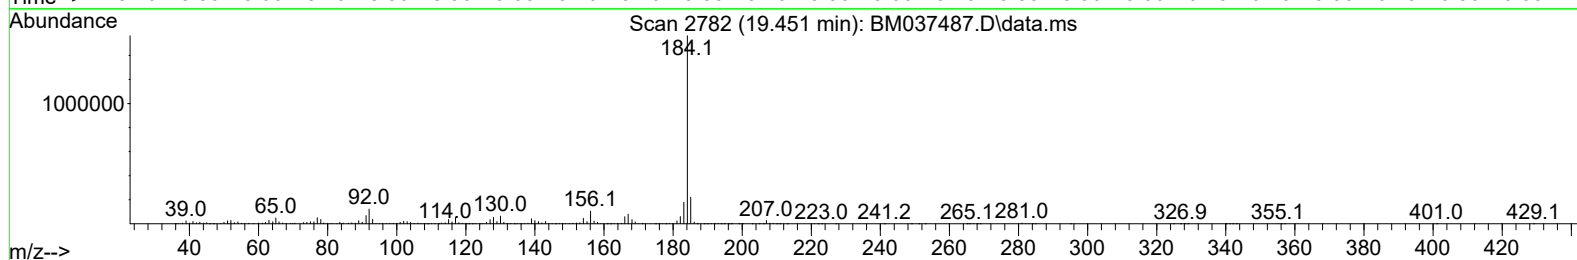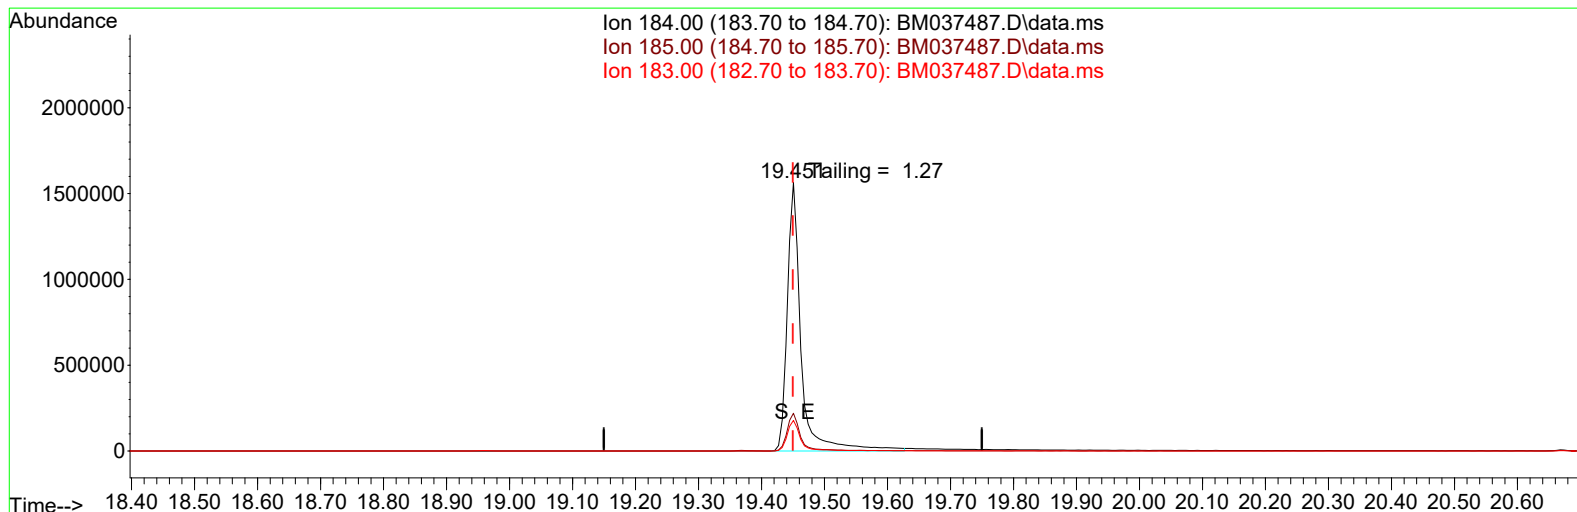

TIC: BM037487.D\data.ms

(77) Benzidine

19.451min (+ 0.001) 4630.22 ng

response 2438364

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.10
183.00	11.30	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2022	BNA_M	<u>BM037487.D</u>
Compound Name	Response	Retention Time
DDT	1323377	20.674
DDD	28966	20.233
DDE	871	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29837	1353214	2.20

Instrument :
BNA_M
ClientSampleId :
DFTPP