

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM111317\
 Data File : BM012943.D
 Acq On : 13 Nov 2017 20:11
 Operator : SJ/JU
 Sample : I6363-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0FB4

Quant Time: Nov 14 03:01:14 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 02:57:44 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	92637	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	360696	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	203066	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	450381	20.00	ng/ul	0.00
77) Chrysene-d12	21.35	240	534639	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	611300	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	7170	4.18	ng/uL	0.00
5) Phenol-d5	6.96	99	134762	19.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	76286	20.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	111822	19.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	110029	18.49	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	53560	20.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	59290	19.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	110973	17.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	122095	20.24	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	338187	20.13	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	405355	19.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	39117	14.53	ng/ul	0.00
57) Fluorene-d10	15.42	176	285198	19.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	33242	11.18	ng/ul	0.00
70) Anthracene-d10	17.27	188	433539	19.92	ng/ul	0.00
78) Pyrene-d10	19.56	212	470504	18.97	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.48	264	575628	19.92	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.99	94	20359	2.877 ng/ul	99
44) Dimethylphthalate	13.87	163	175837	10.545 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM111317\
Data File : BM012943.D
Acq On : 13 Nov 2017 20:11
Operator : SJ/JU
Sample : I6363-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0FB4

Quant Time: Nov 14 03:01:14 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 14 02:57:44 2017
Response via : Initial Calibration

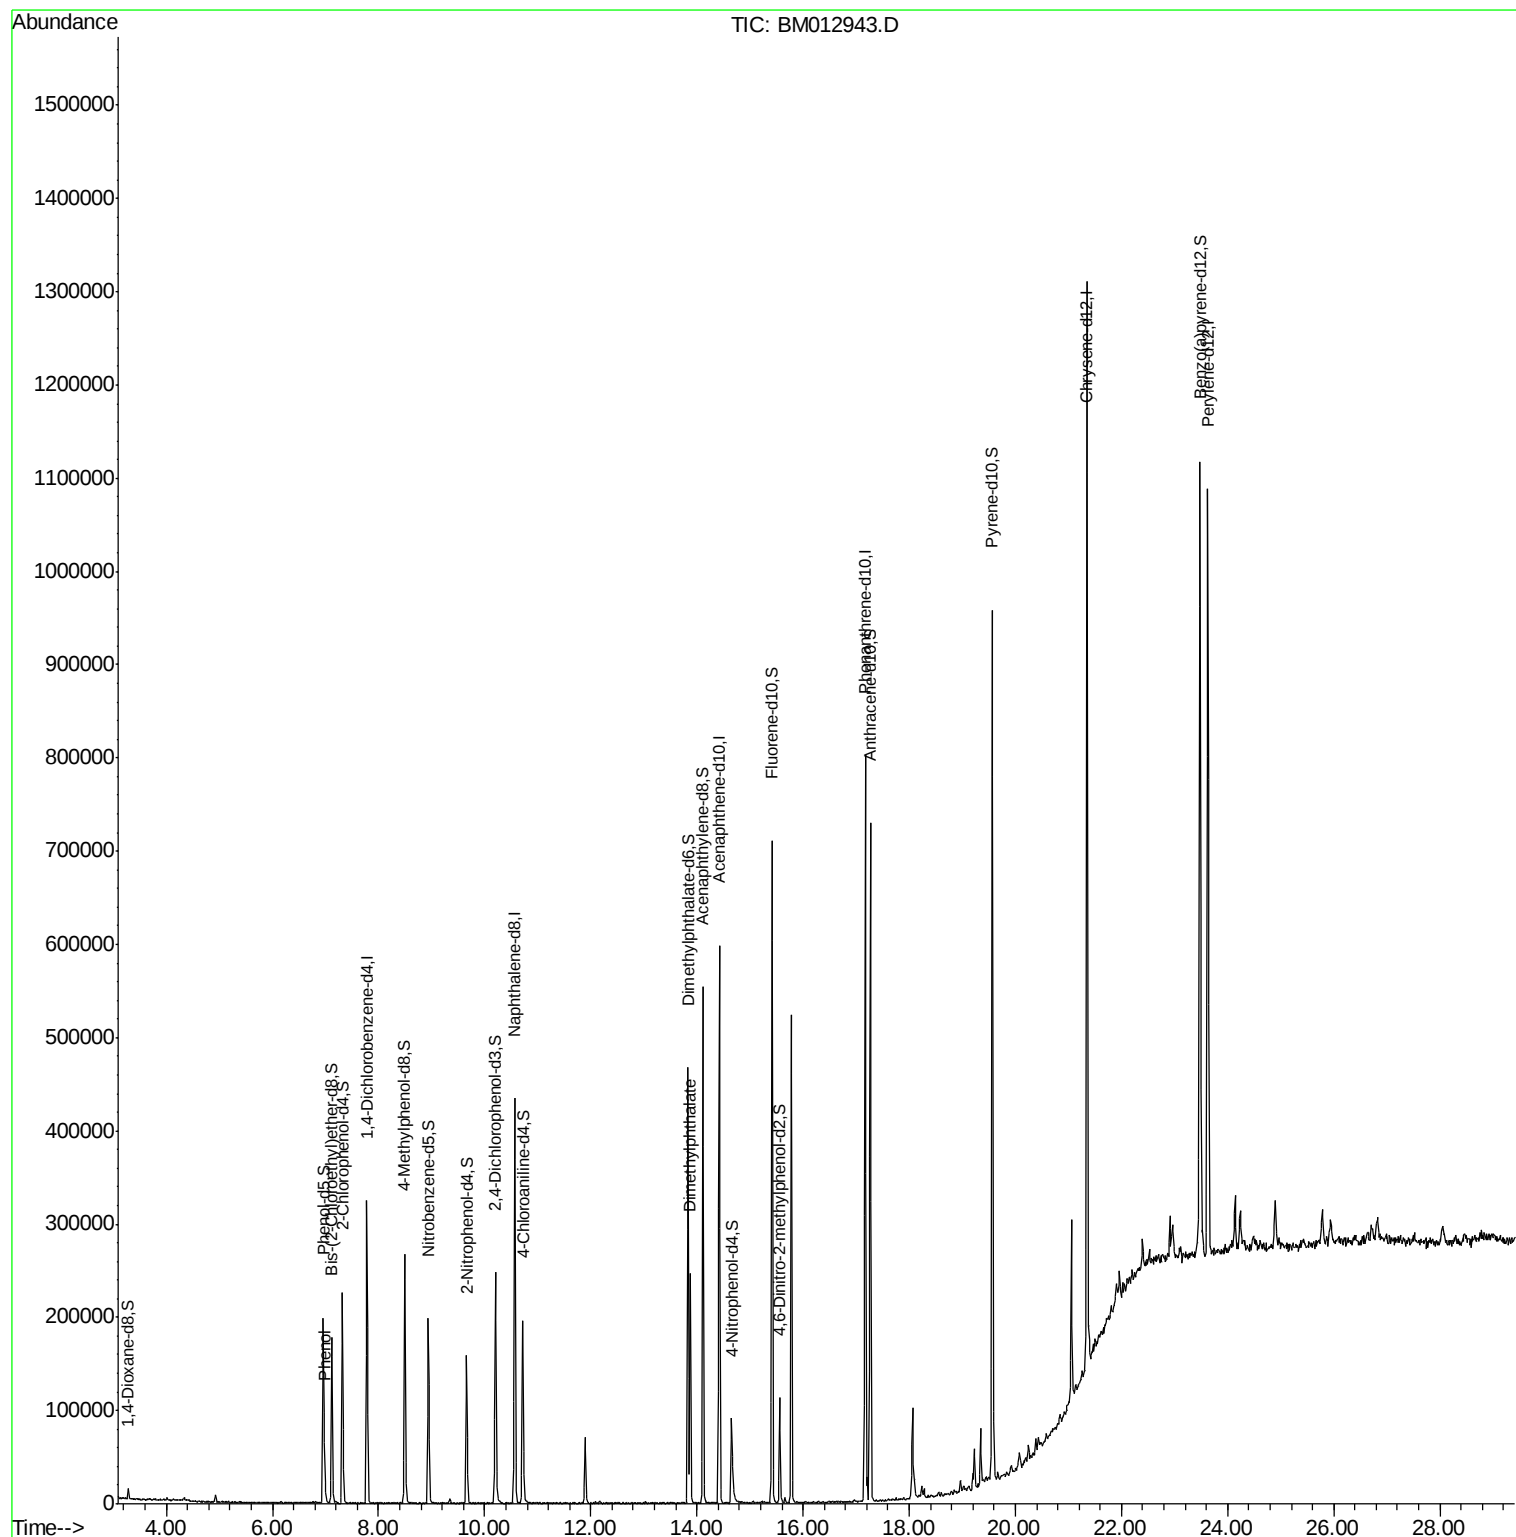

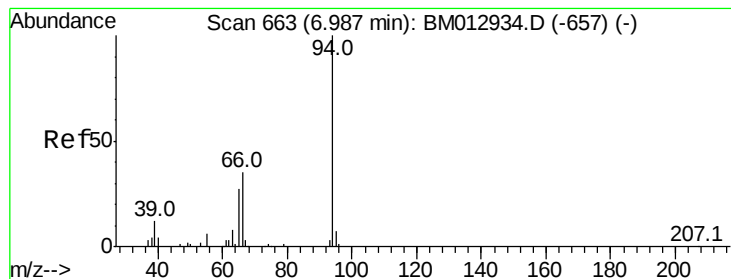

#6

Phenol

Concen: 2.877 ng/ul

RT: 6.99 min Scan# 663

Delta R.T. -0.00 min

Lab File: BM012943.D

Acq: 13 Nov 2017 20:11

Instrument :




BNA_M

ClientSampleId :


B0FB4

Tot Ion: 94 Resp: 20359

Ion	Ratio	Lower	Upper
94	100		
65	26.8	21.0	31.6
66	36.9	29.3	43.9

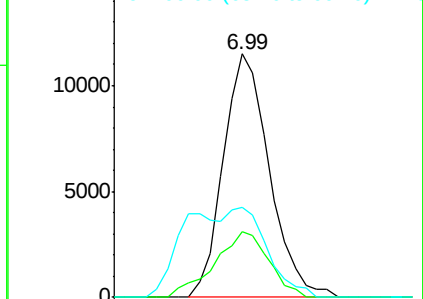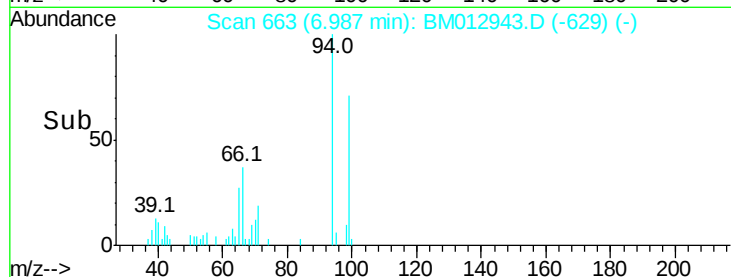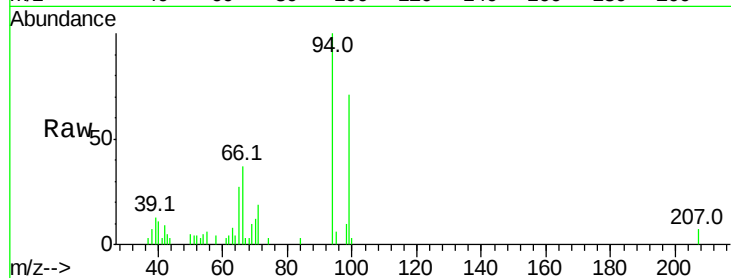

Time-->

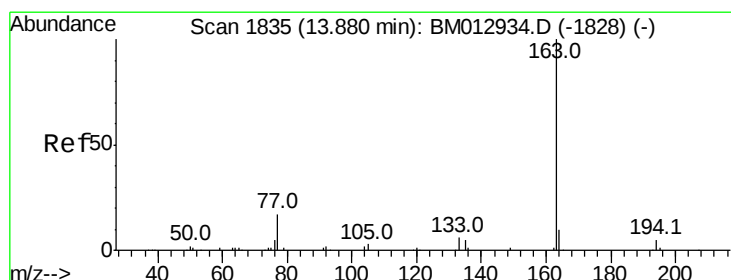

#44

Dimethylphthalate

Concen: 10.545 ng/ul

RT: 13.87 min Scan# 1834





Delta R.T. -0.01 min

Lab File: BM012943.D

Acq: 13 Nov 2017 20:11

Tgt Ion:163 Resp: 175837

Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.2	4.8
164	10.3	7.8	11.8

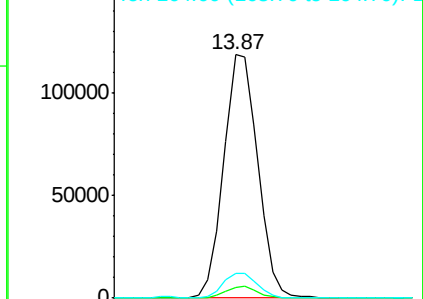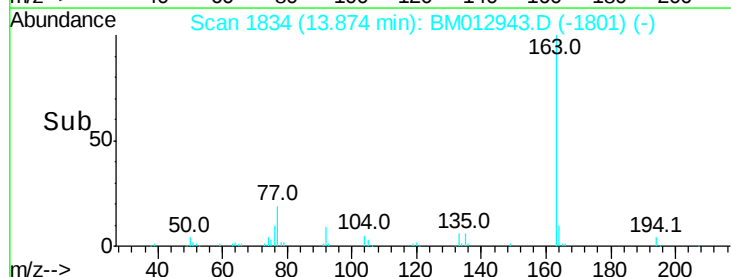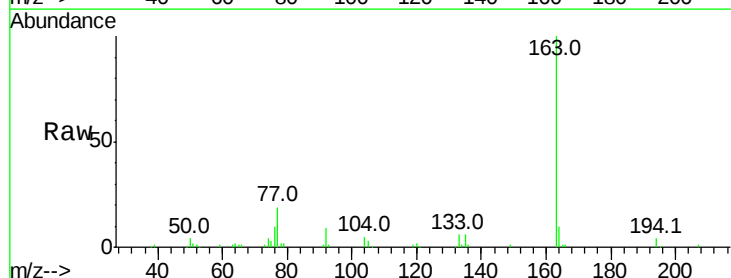

Time-->