

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM111317\
 Data File : BM012955.D
 Acq On : 14 Nov 2017 03:17
 Operator : SJ/JU
 Sample : I6363-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0FE5

Quant Time: Nov 14 04:29:39 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 04:22:37 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	109000	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	420608	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	241185	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	549977	20.00	ng/ul	0.00
77) Chrysene-d12	21.35	240	666381	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	749847	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	8399	4.16	ng/uL	0.00
5) Phenol-d5	6.96	99	171729	21.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	97679	22.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	142536	21.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	137132	19.59	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	67460	21.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	76167	21.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	142416	19.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	130430	18.54	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	442119	22.15	ng/ul	0.00
46) Acenaphthylene-d8	14.11	160	541760	21.95	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	56789	17.76	ng/ul	0.00
57) Fluorene-d10	15.42	176	385225	22.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	52494	14.46	ng/ul	0.00
70) Anthracene-d10	17.27	188	619420	23.31	ng/ul	0.00
78) Pyrene-d10	19.56	212	702333	22.71	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.48	264	867382	24.46	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.99	94	24912	2.992	ng/ul 94
44) Dimethylphthalate	13.87	163	82006	4.141	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM111317\
Data File : BM012955.D
Acq On : 14 Nov 2017 03:17
Operator : SJ/JU
Sample : I6363-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0FE5

Quant Time: Nov 14 04:29:39 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 14 04:22:37 2017
Response via : Initial Calibration

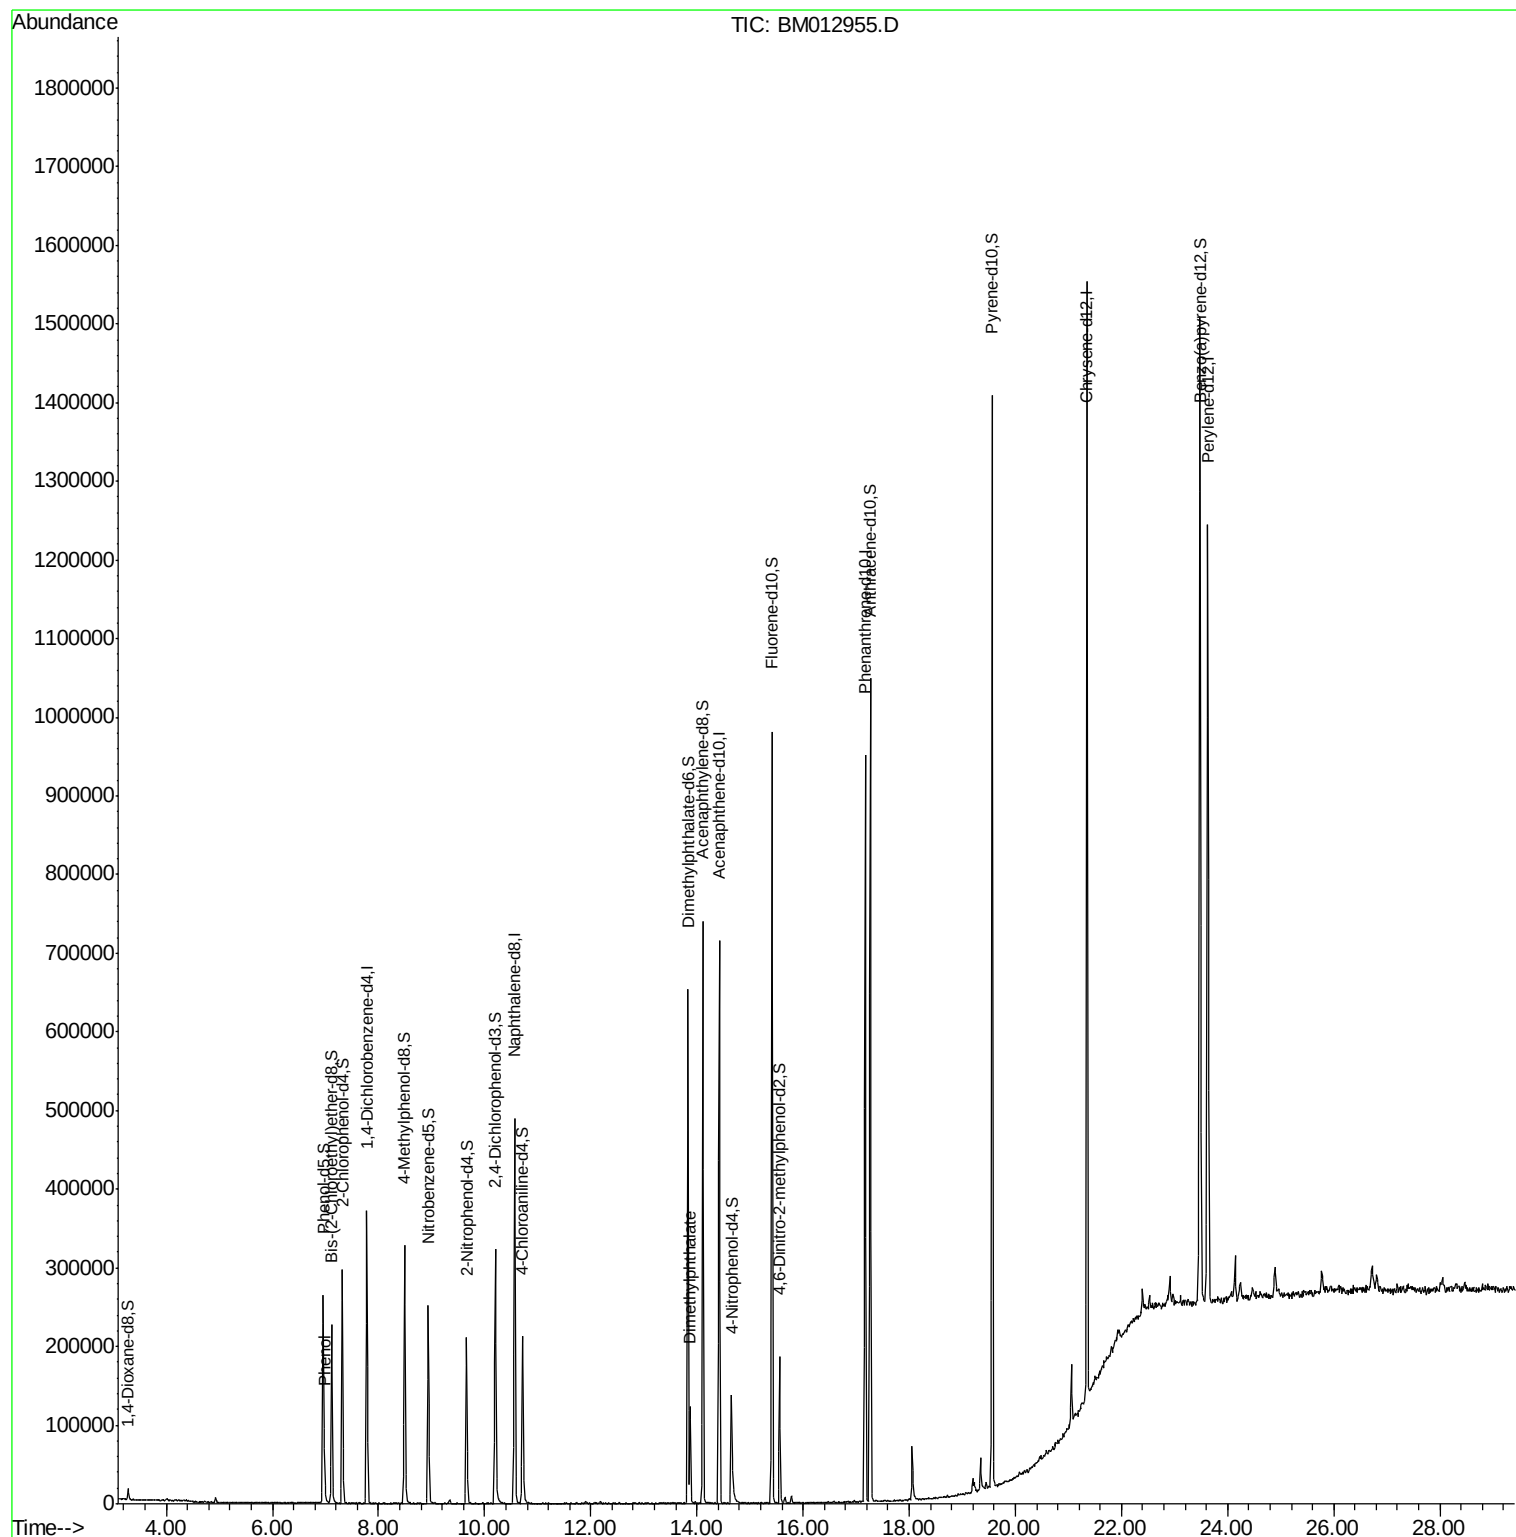

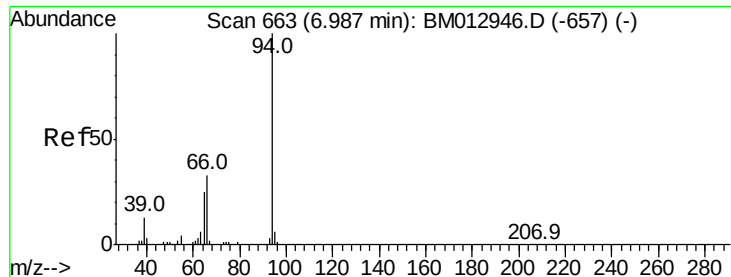

#6

Phenol

Concen: 2.992 ng/ul

RT: 6.99 min Scan# 663

Delta R.T. -0.00 min

Lab File: BM012955.D

Acq: 14 Nov 2017 03:17

Instrument :

BNA_M

ClientSampleId :

B0FE5


Tot Ion: 94 Resp: 24912

Ion Ratio Lower Upper

94 100

65 27.1 21.0 31.6




66 41.9 29.3 43.9

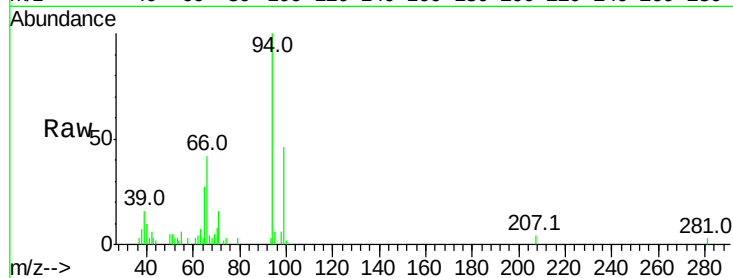

Abundance Ion 94.00 (93.70 to 94.70): BM012946.D (-657) (-)

Ion 65.00 (64.70 to 65.70): BM012946.D (-657) (-)

Ion 66.00 (65.70 to 66.70): BM012946.D (-657) (-)

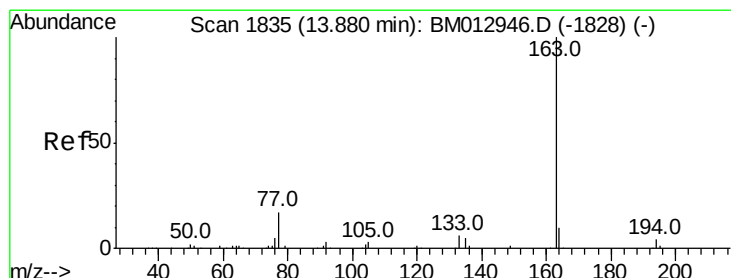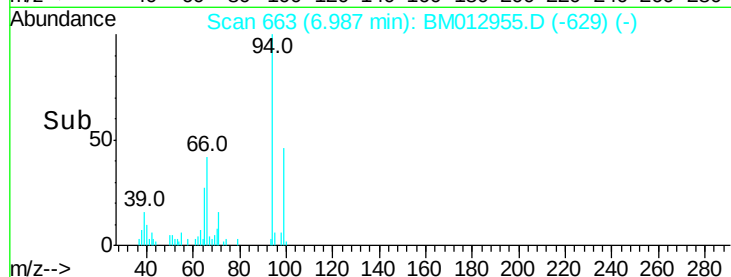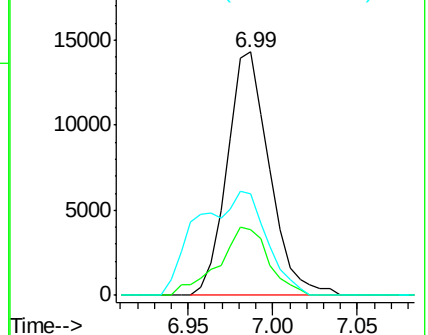

#44

Dimethylphthalate

Concen: 4.141 ng/ul

RT: 13.87 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM012955.D

Acq: 14 Nov 2017 03:17


Tgt Ion:163 Resp: 82006

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.4 7.8 11.8

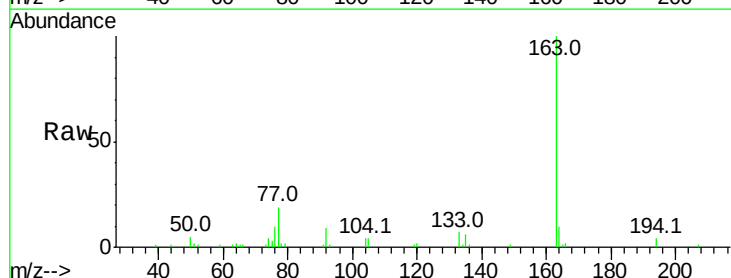

Abundance Ion 163.00 (162.70 to 163.70): BM012946.D (-1828) (-)

Ion 194.00 (193.70 to 194.70): BM012946.D (-1828) (-)

Ion 164.00 (163.70 to 164.70): BM012946.D (-1828) (-)

