

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111321\
 Data File : BM033043.D
 Acq On : 13 Nov 2021 15:48
 Operator : CG/JU
 Sample : M4412-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG373

Quant Time: Nov 15 03:15:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 03:11:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.438	152	1636	0.400	ng/ul	0.00
4) Naphthalene-d8	10.208	136	6389	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.095	164	4247	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.841	188	8383	0.400	ng/ul	0.00
17) Chrysene-d12	21.035	240	5267	0.400	ng/ul	# 0.00
23) Perylene-d12	23.139	264	4875	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.850	96	12417	5.944	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.809	152	3597	0.396	ng/ul	0.00
18) Fluoranthene-d10	18.873	212	9362	0.586	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	16.883	178	720	0.026	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111321\
Data File : BM033043.D
Acq On : 13 Nov 2021 15:48
Operator : CG/JU
Sample : M4412-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG373


Quant Time: Nov 15 03:15:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:11:31 2021
Response via : Initial Calibration

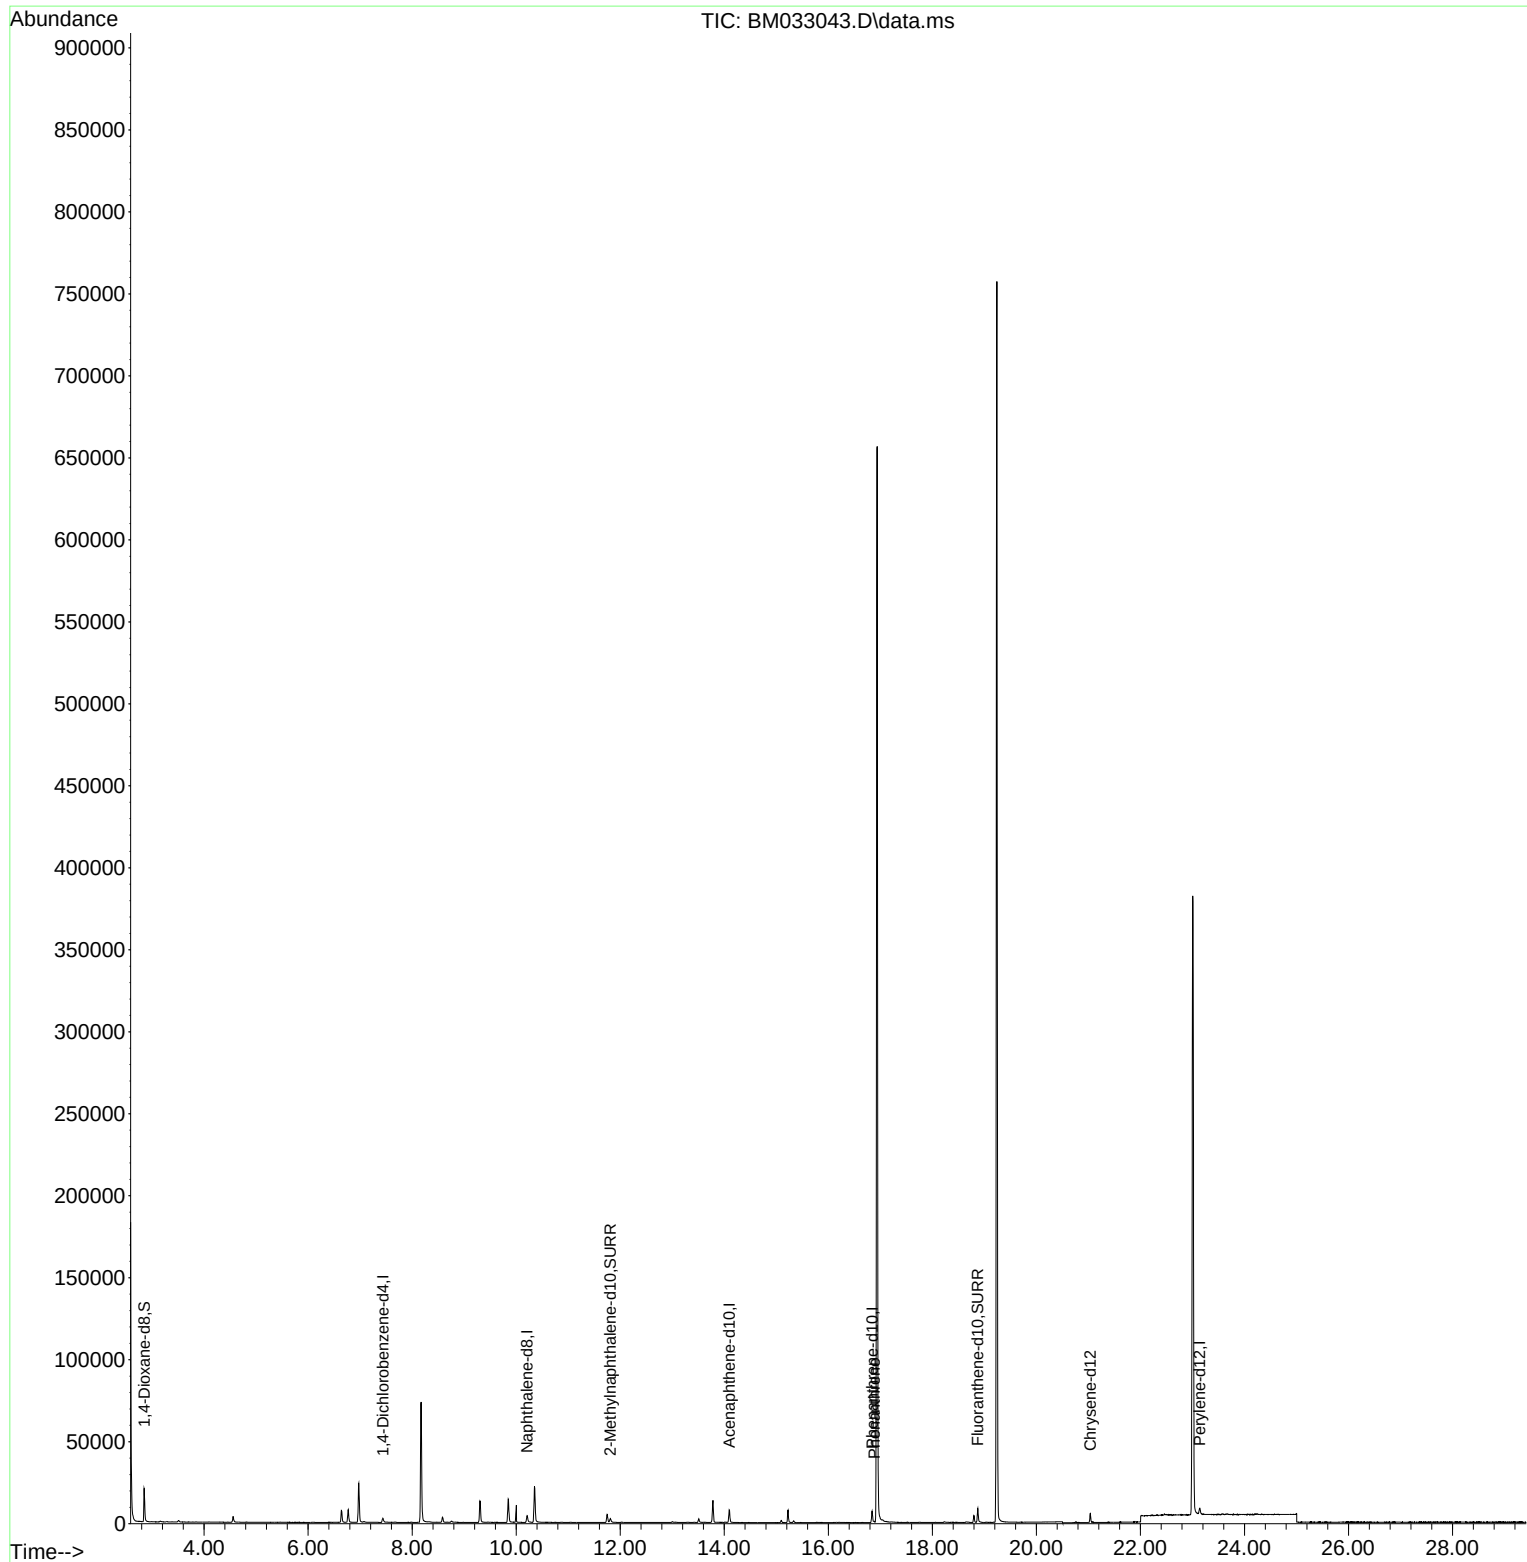

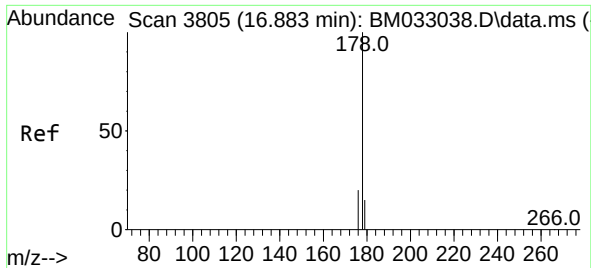

#15
 Phenanthrene
 Concen: 0.026 ng/ul
 RT: 16.883 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM033043.D
 Acq: 13 Nov 2021 15:48

Instrument :
 BNA_M
 ClientSampleId :
 BG373

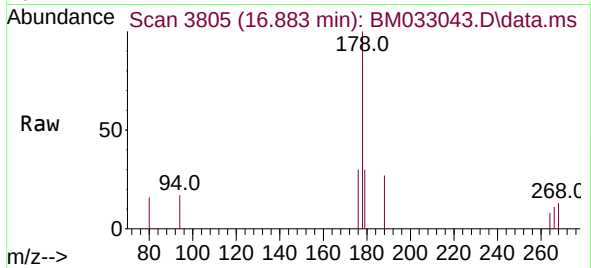

Tgt Ion	Ratio	Lower	Upper
178	100		
179	29.5	12.9	19.3#
176	30.4	16.0	24.0#

