


Data Path : Z:\HPCHEM1\BNA_M\Data\BM111416\
Data File : BM007857.D
Acq On : 14 Nov 2016 16:27
Operator : UM/SJ
Sample : H5594-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDQN8

Manual Integrations
APPROVED

umangi
11/15/2016 3:08:06 PM

Quant Time: Nov 15 03:02:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 02:47:54 2016
Response via : Initial Calibration

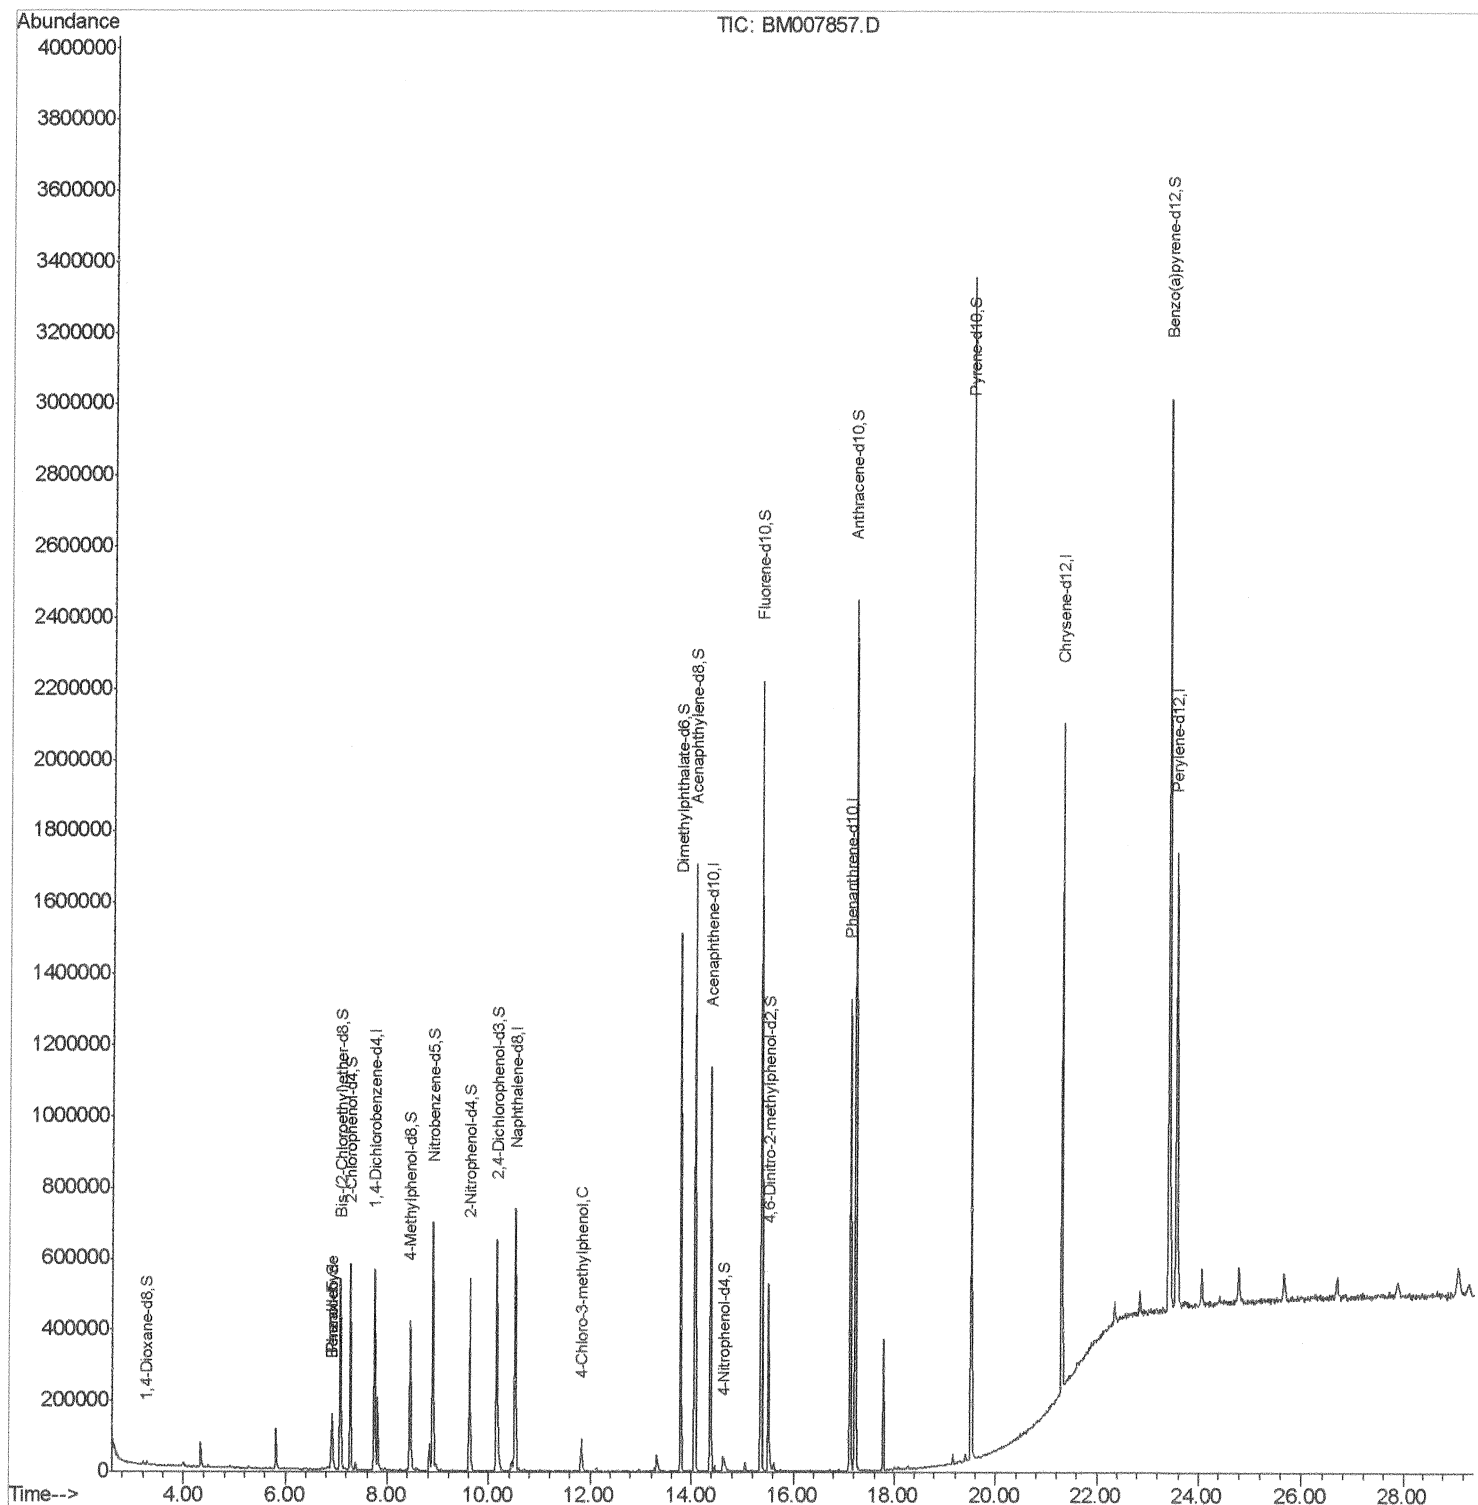




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111416\
Data File : BM007857.D
Acq On : 14 Nov 2016 16:27
Operator : UM/SJ
Sample : H5594-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDQN8

Manual Integrations
APPROVED

umangi
11/15/2016 3:08:06 PM

Quant Time: Nov 15 02:49:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 02:47:54 2016
Response via : Initial Calibration

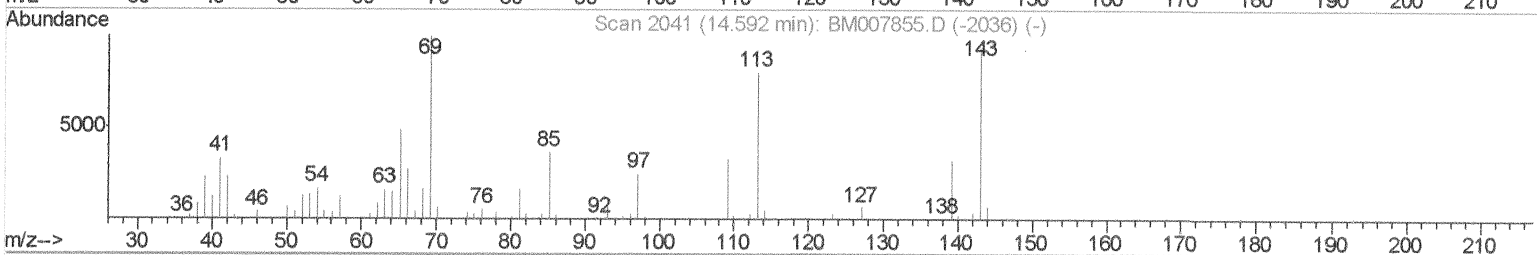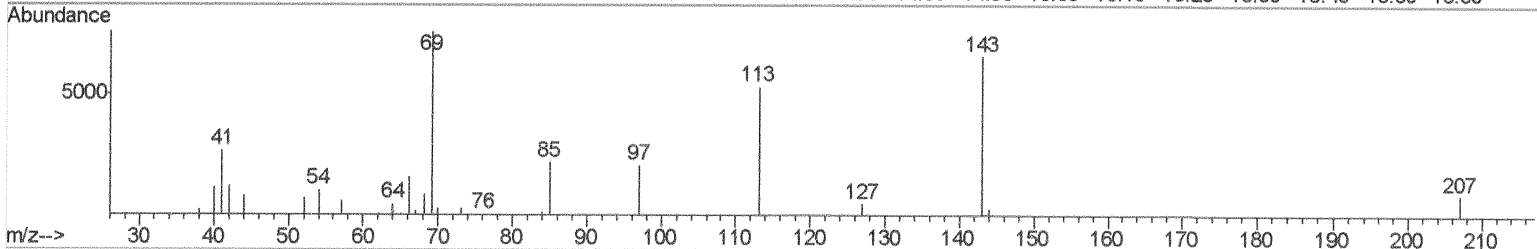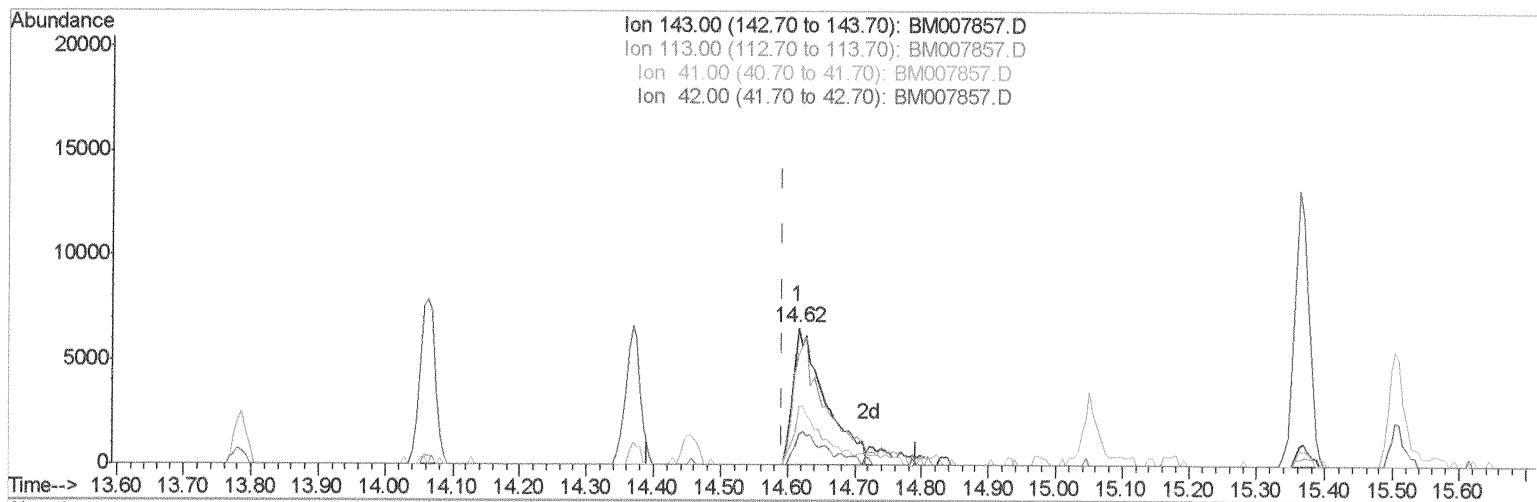

TIC: BM007857.D

(51) 4-Nitrophenol-d4 (S)

14.615min (+0.023) 5.26ng/ul

response 21894

Ion	Exp%	Act%
143.00	100	100
113.00	93.70	81.48
41.00	36.40	42.86
42.00	22.60	22.17




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111416\
Data File : BM007857.D
Acq On : 14 Nov 2016 16:27
Operator : UM/SJ
Sample : H5594-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDQN8

Manual Integrations
APPROVED

umangi
11/15/2016 3:08:06 PM

Quant Time: Nov 15 02:49:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 02:47:54 2016
Response via : Initial Calibration

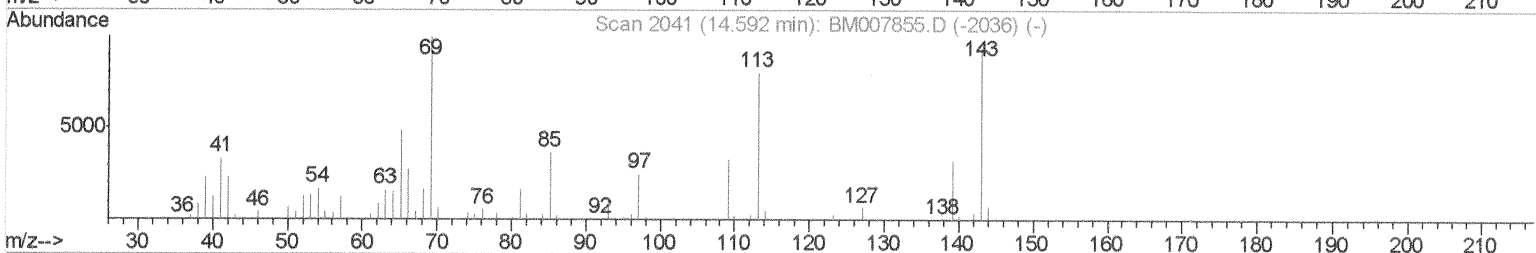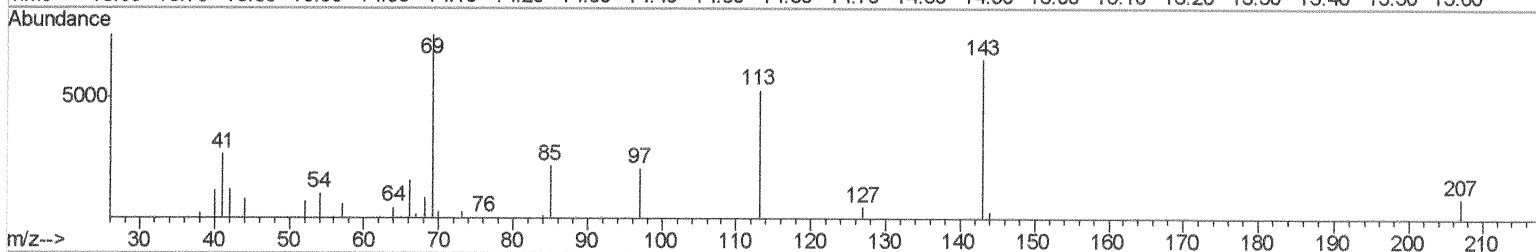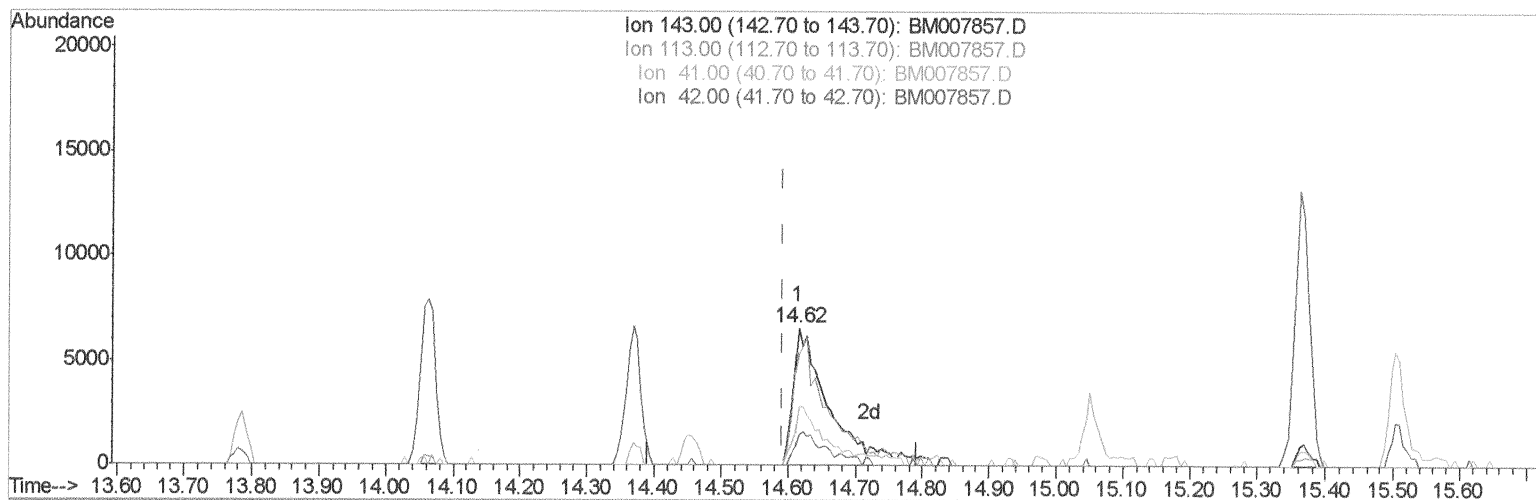

TIC: BM007857.D

(51) 4-Nitrophenol-d4 (S)

14.615min (+0.023) 6.01ng/ul m

SJ 11/15/16

response 25007

Ion	Exp%	Act%
143.00	100	100
113.00	93.70	81.48
41.00	36.40	42.86
42.00	22.60	22.17

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111416\
 Data File : BM007857.D
 Acq On : 14 Nov 2016 16:27
 Operator : UM/SJ
 Sample : H5594-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDQN8

Manual Integrations
 APPROVED

umangi
 11/15/2016 3:08:06 PM

Quant Time: Nov 15 03:02:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 02:47:54 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	152652	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	591270	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	386447	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	772658	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	980047	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1004587	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	5701	1.60	ng/uL	0.00
5) Phenol-d5	6.92	99	87990	7.47	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.07	67	240087	34.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	264855	29.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.44	113	164804	17.88	ng/ul	0.00
19) Nitrobenzene-d5	8.89	128	154649	36.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.61	143	166318	36.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	290206	32.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	6095	0.60	ng/ul	0.03
43) Dimethylphthalate-d6	13.79	166	1006750	38.26	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	1171971	37.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	25007m	6.01	ng/ul	0.02
57) Fluorene-d10	15.37	176	896462	38.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	124727	27.17	ng/ul	0.00
70) Anthracene-d10	17.22	188	1451513	41.69	ng/ul	0.00
76) Pyrene-d10	19.52	212	1700074	42.22	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.41	264	1820785	41.52	ng/ul	0.00

51 11/15/16

Target Compounds

					Qvalue
4) Benzaldehyde	6.90	77	14606	1.96	ng/ul 87
33) 4-Chloro-3-methylphenol	11.82	107	43761	4.78	ng/ul 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed