

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111416\
 Data File : BM007847.D
 Acq On : 14 Nov 2016 10:21
 Operator : UM/SJ
 Sample : PB94627BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	114	118	124	rVB	54959	73156	1.65%	0.149%
2	6.910	729	735	754	rBV	849096	1429260	32.31%	2.902%
3	7.075	757	763	776	rBV	706937	1094761	24.75%	2.223%
4	7.269	789	796	811	rVB	908828	1512194	34.18%	3.070%
5	7.734	868	875	885	rBV	785270	1296203	29.30%	2.632%
6	8.440	989	995	1011	rBV	1049885	1788114	40.42%	3.631%
7	8.892	1063	1072	1085	rBV	840816	1433574	32.41%	2.911%
8	9.610	1187	1194	1206	rBV	688856	1169590	26.44%	2.375%
9	10.145	1277	1285	1306	rBV	955144	1784894	40.35%	3.624%
10	10.516	1340	1348	1360	rBV	1020699	1722715	38.94%	3.498%
11	10.663	1366	1373	1391	rBV	871119	1717340	38.82%	3.487%
12	13.786	1897	1904	1917	rBV	1705717	2500163	56.52%	5.076%
13	14.063	1944	1951	1963	rBV	2010101	2909810	65.78%	5.908%
14	14.369	1997	2003	2016	rBV	1445885	2200584	49.74%	4.468%
15	14.592	2035	2041	2065	rBV	408824	950836	21.49%	1.931%
16	15.369	2166	2173	2183	rBV	2562805	3651545	82.54%	7.414%
17	15.504	2190	2196	2210	rBV	529760	859511	19.43%	1.745%
18	15.610	2210	2214	2221	rVB2	30634	46047	1.04%	0.093%
19	17.121	2464	2471	2481	rBV	1759756	2490643	56.30%	5.057%
20	17.215	2481	2487	2499	rBV	2511628	3778802	85.42%	7.672%
21	19.515	2872	2878	2888	rBV	3125174	4423861	100.00%	8.982%
22	21.309	3178	3183	3192	rBV	2257487	3086378	69.77%	6.266%
23	23.415	3535	3541	3551	rVB2	2323652	4338555	98.07%	8.809%
24	23.556	3559	3565	3580	rVB	1488064	2994007	67.68%	6.079%


Sum of corrected areas: 49252543

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111416\
Data File : BM007847.D
Acq On : 14 Nov 2016 10:21
Operator : UM/SJ
Sample : PB94627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

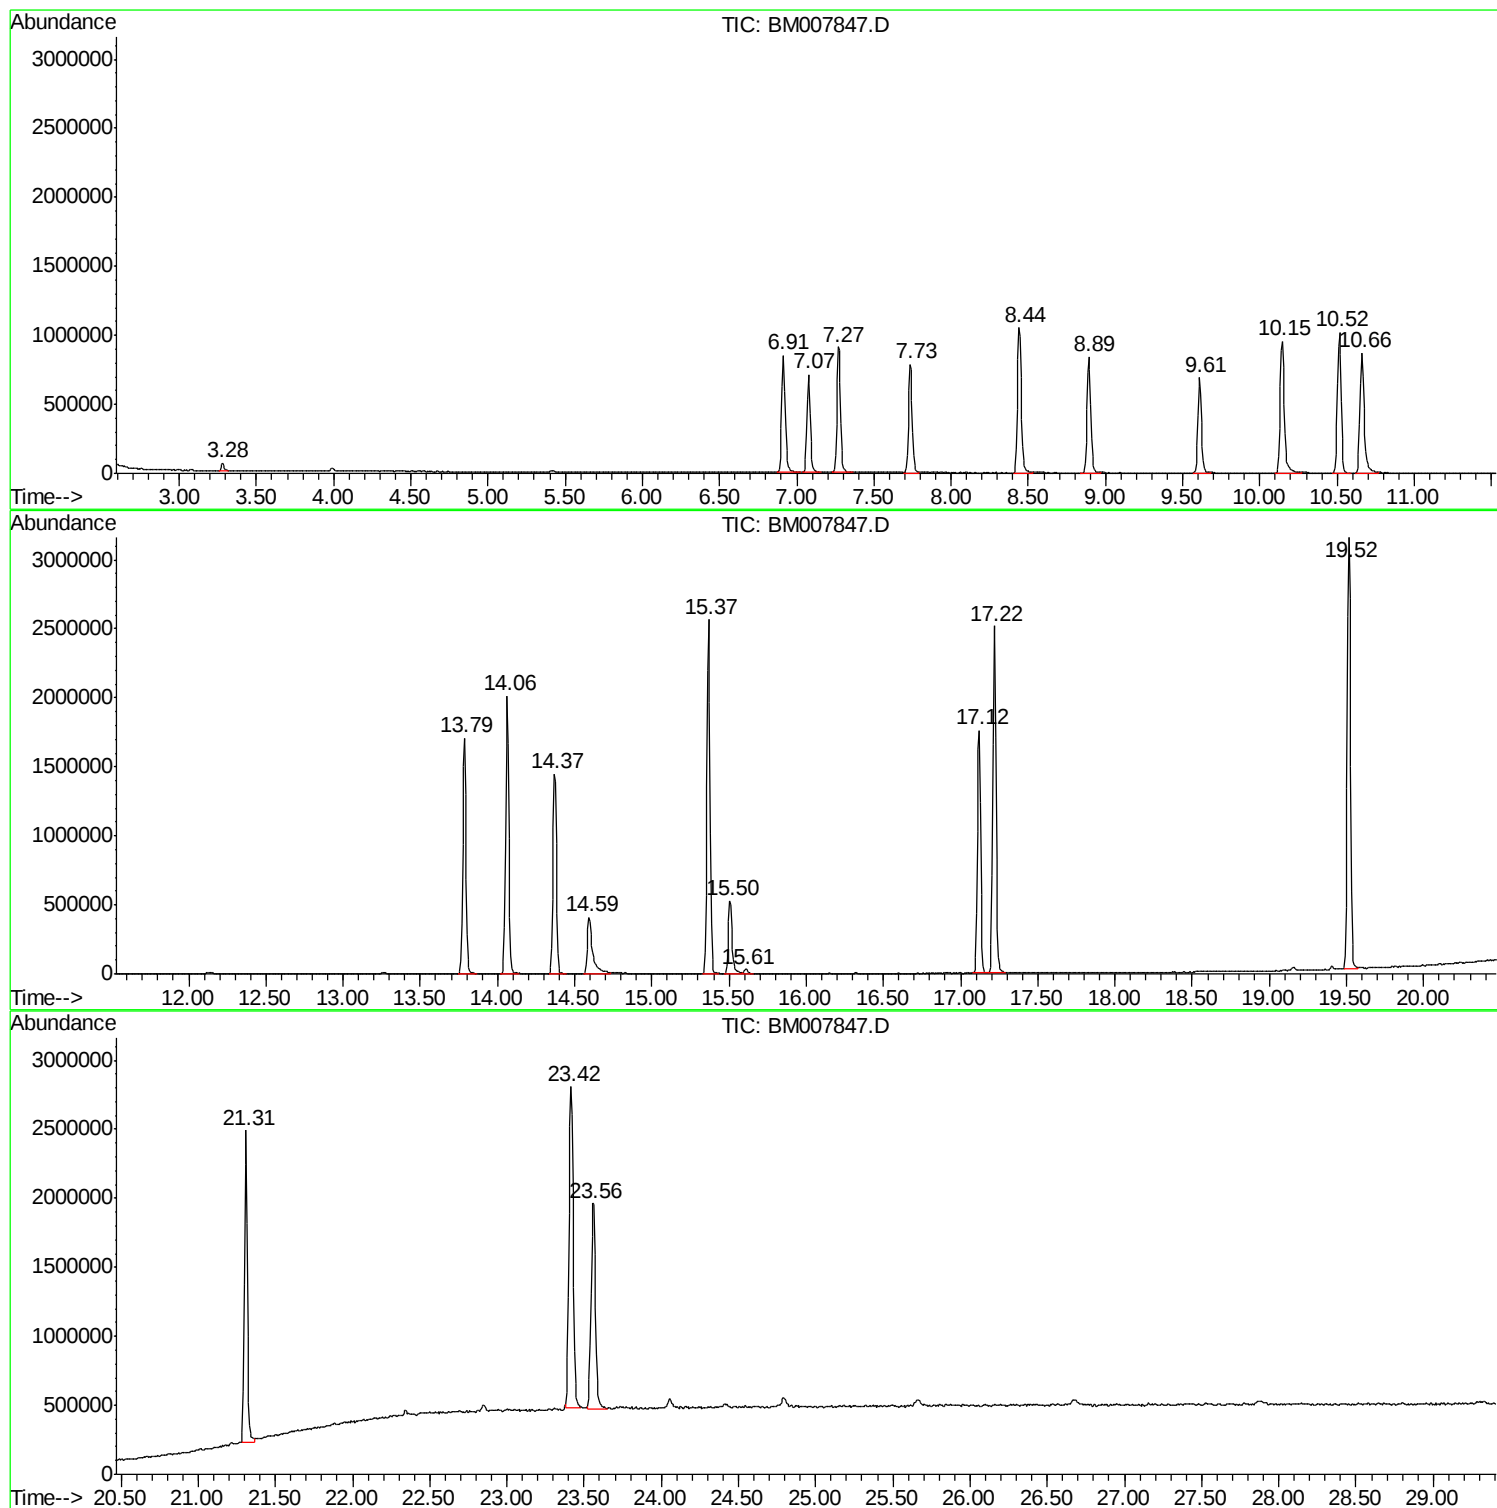

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111416\
Data File : BM007847.D
Acq On : 14 Nov 2016 10:21
Operator : UM/SJ
Sample : PB94627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111416\
Data File : BM007847.D
Acq On : 14 Nov 2016 10:21
Operator : UM/SJ
Sample : PB94627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc