
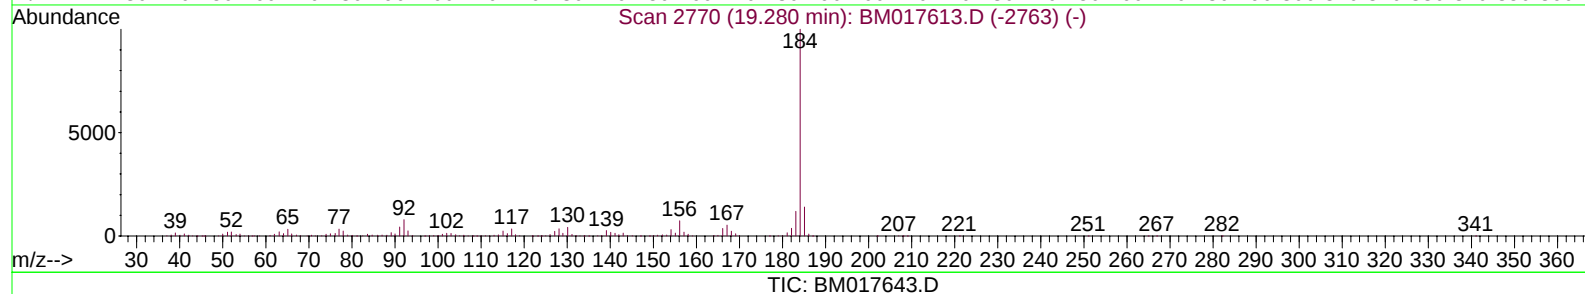
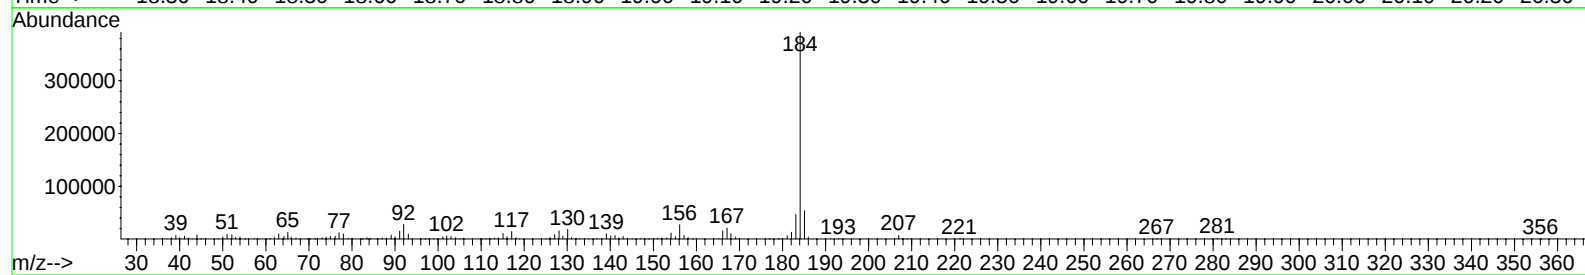


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111418\
Data File : BM017643.D
Acq On : 14 Nov 2018 12:36
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 17:02:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

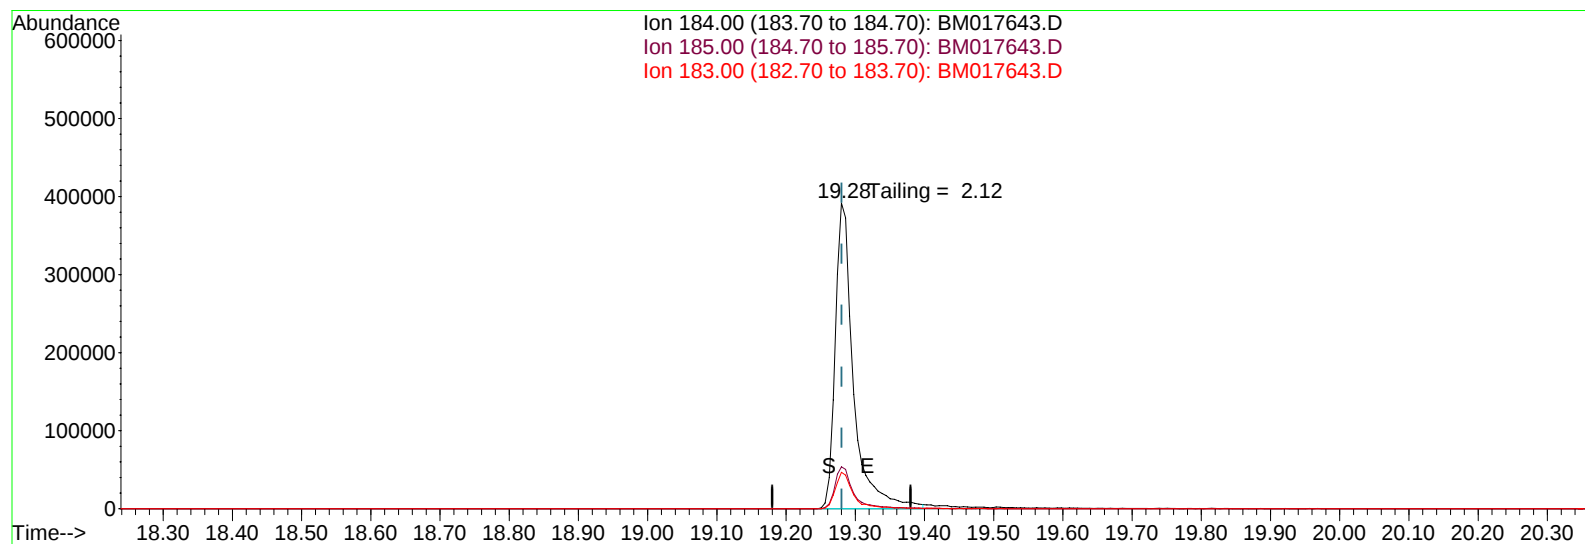

TIC: BM017643.D

(77) Benzidine




19.280min (+0.000) 0.00ng

response 698807

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.69
183.00	11.90	11.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111418\
Data File : BM017643.D
Acq On : 14 Nov 2018 12:36
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 17:02:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

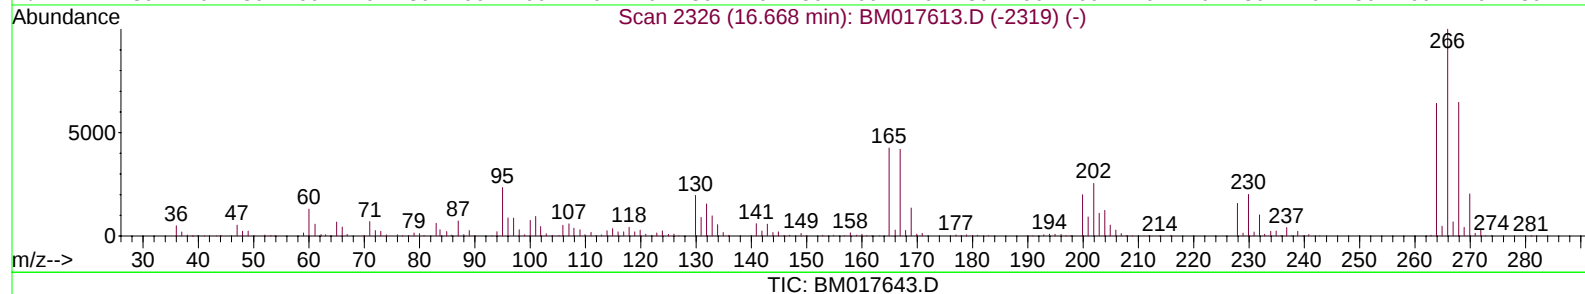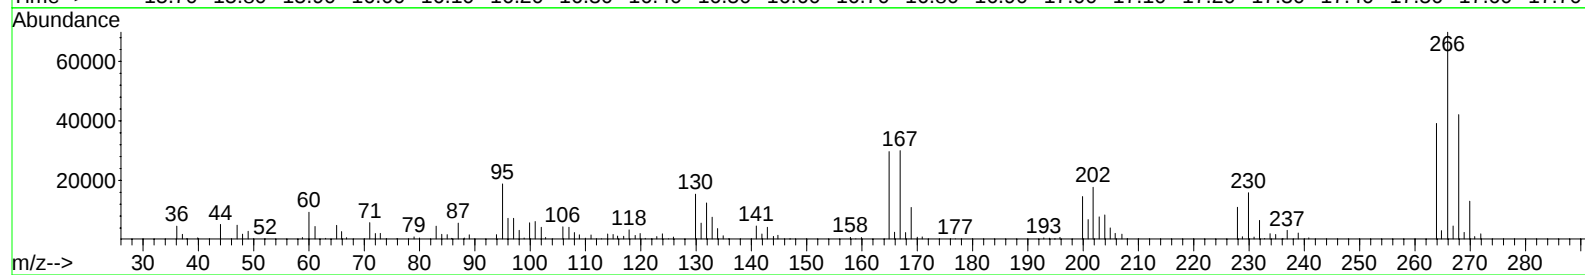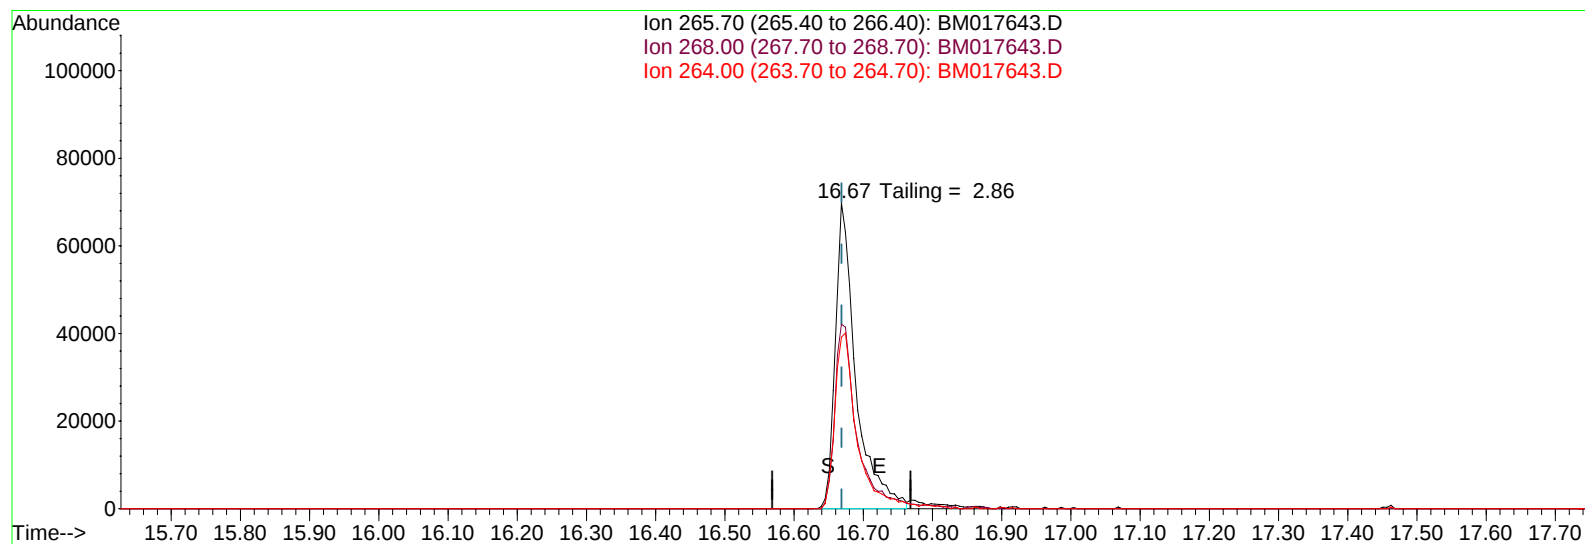

(70) Pentachlorophenol (C)

16.668min (+0.000) 0.00ng

response 141984

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	60.32
264.00	64.10	56.09
0.00	0.00	0.00