


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111418\
 Data File : BM017643.D
 Acq On : 14 Nov 2018 12:36
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

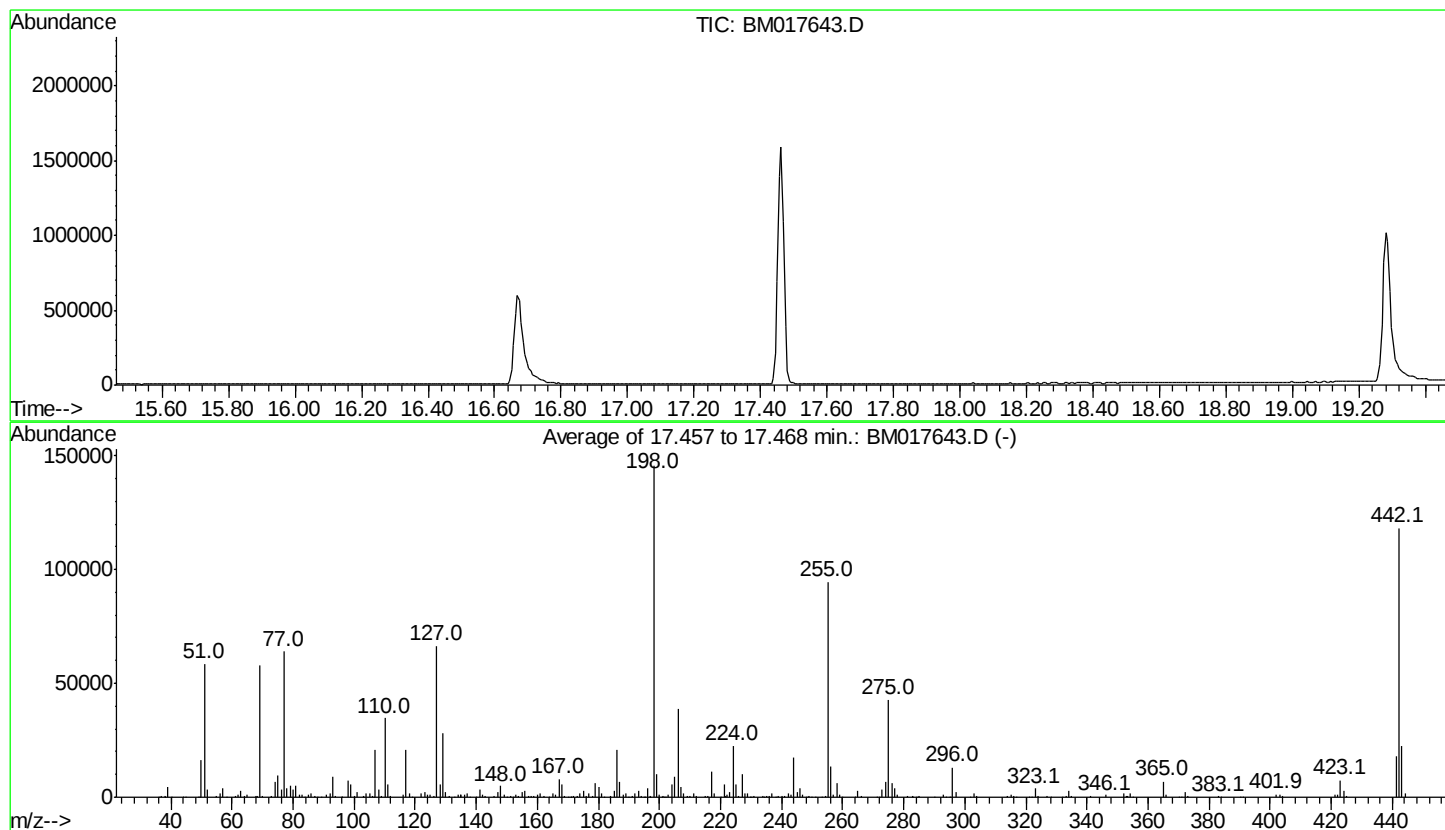

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	58568	PASS
68	69	0.00	2	1.2	701	PASS
69	198	0.00	100	39.9	58106	PASS
70	69	0.00	2	0.6	329	PASS
127	198	10	80	45.6	66426	PASS
197	198	0.00	2	0.6	801	PASS
198	198	100	100	100.0	145586	PASS
199	198	5	9	7.0	10241	PASS
275	198	10	60	29.4	42744	PASS
365	198	1	100	4.8	6979	PASS
441	198	0.01	100	12.3	17926	PASS
442	198	50	100	81.1	118093	PASS
443	442	15	24	19.0	22469	PASS