
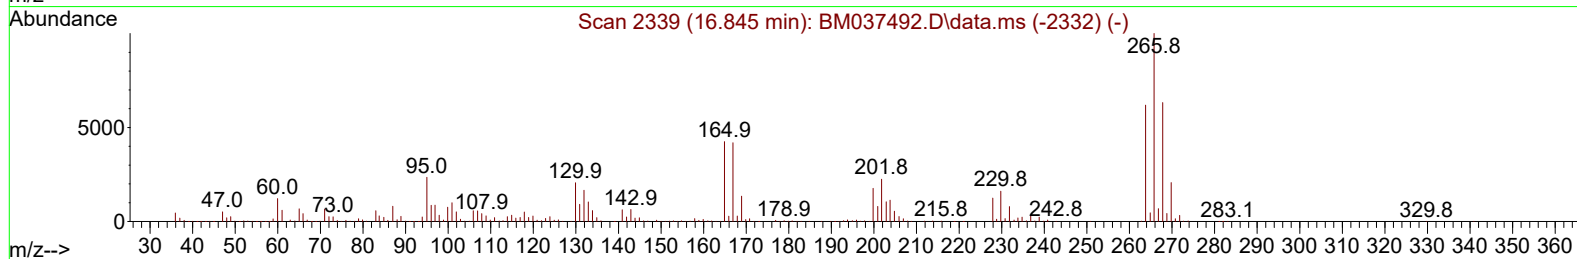
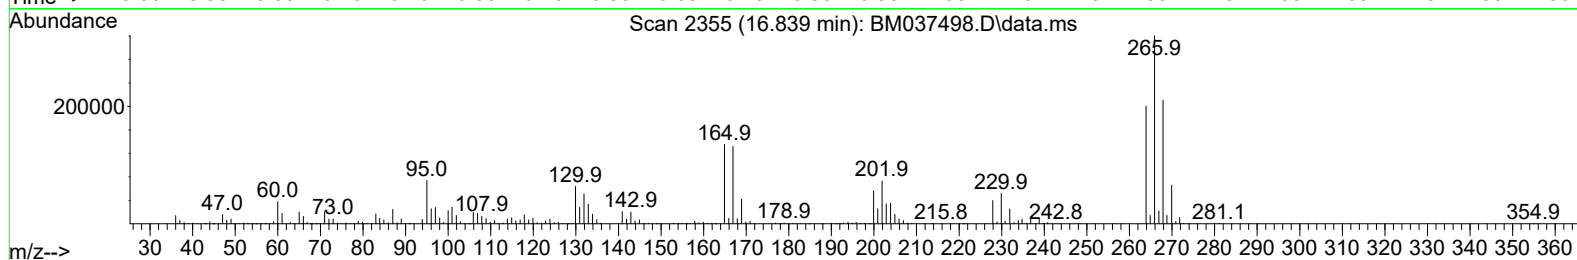


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111422\
Data File : BM037498.D
Acq On : 14 Nov 2022 09:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 13:04:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 01:42:00 2022
Response via : Initial Calibration

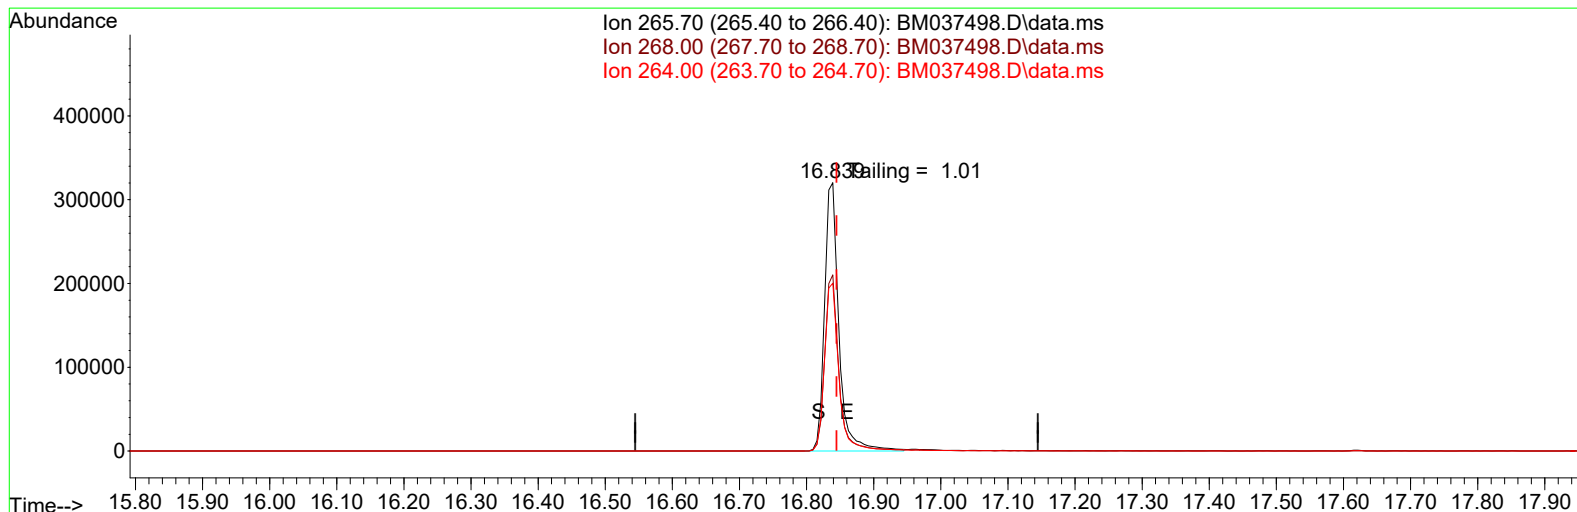

TIC: BM037498.D\data.ms

(70) Pentachlorophenol (C)




16.839min (-0.006) 0.00 ng

response 474426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	65.66
264.00	61.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111422\
Data File : BM037498.D
Acq On : 14 Nov 2022 09:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 13:04:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 01:42:00 2022
Response via : Initial Calibration

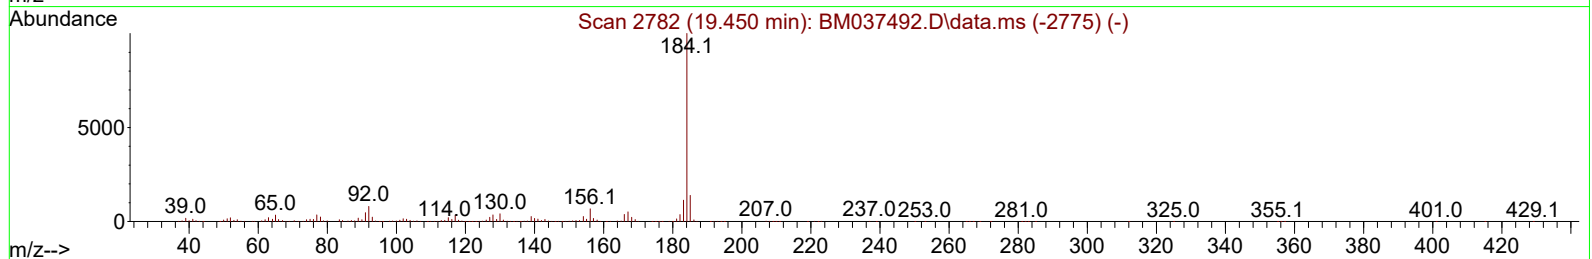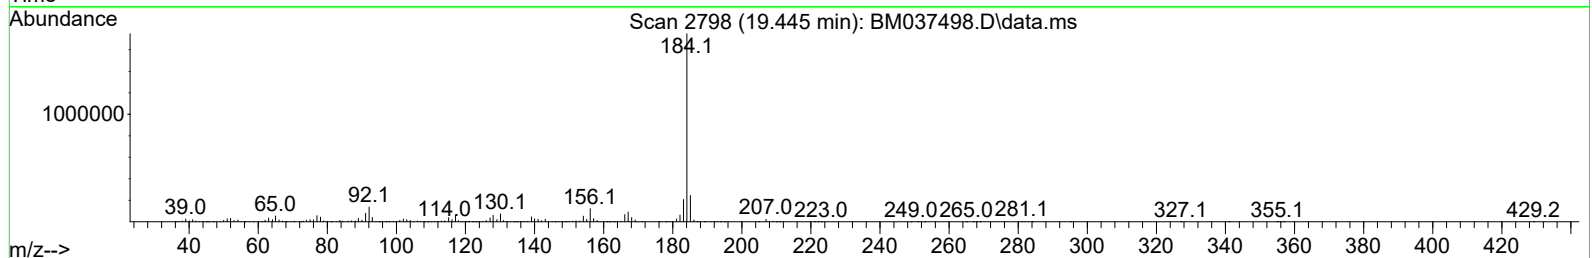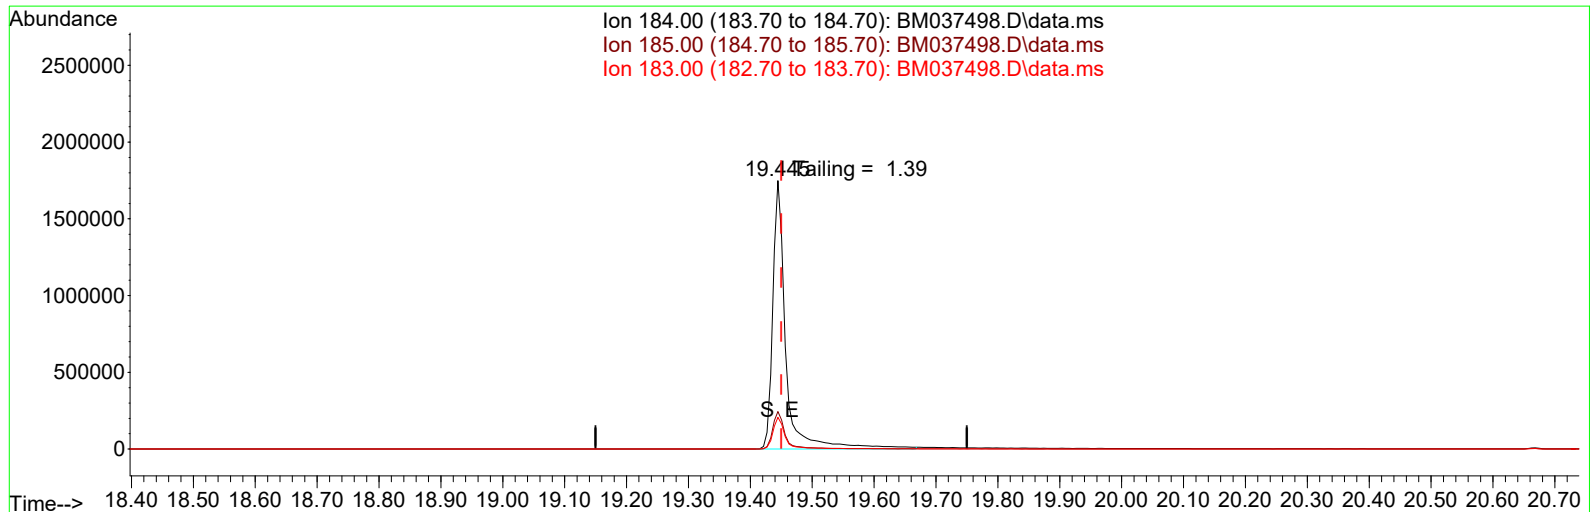

TIC: BM037498.D\data.ms

(77) Benzidine**19.445min (-0.005) 31960.88 ng****response 2619713**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.98
183.00	11.30	11.84
0.00	0.00	0.00