


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111422\
 Data File : BM037498.D
 Acq On : 14 Nov 2022 09:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 14 01:42:00 2022

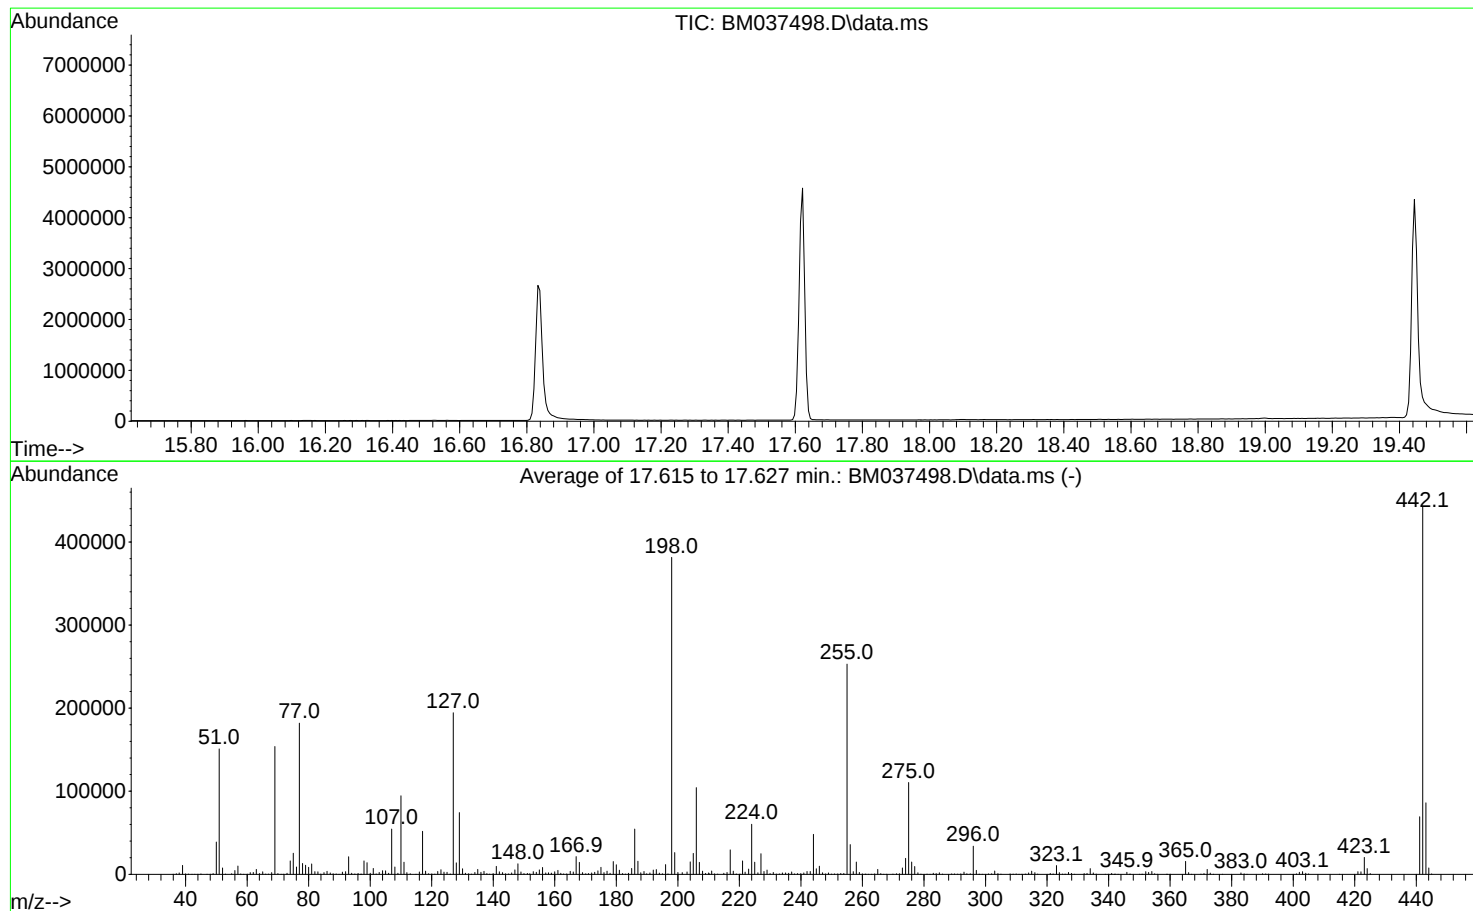




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	150917	PASS
68	69	0.00	2	1.4	2099	PASS
69	198	0.00	100	40.3	153768	PASS
70	69	0.00	2	0.6	932	PASS
127	198	10	80	51.0	194397	PASS
197	198	0.00	2	0.1	555	PASS
198	198	100	100	100.0	381397	PASS
199	198	5	9	6.9	26128	PASS
275	198	10	60	29.0	110523	PASS
365	198	1	100	4.1	15537	PASS
441	198	0.01	100	18.2	69267	PASS
442	442	50	100	100.0	442816	PASS
443	442	15	24	19.4	86043	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111422\
Data File : BM037498.D
Acq On : 14 Nov 2022 09:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 14 13:04:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 01:42:00 2022
Response via : Initial Calibration

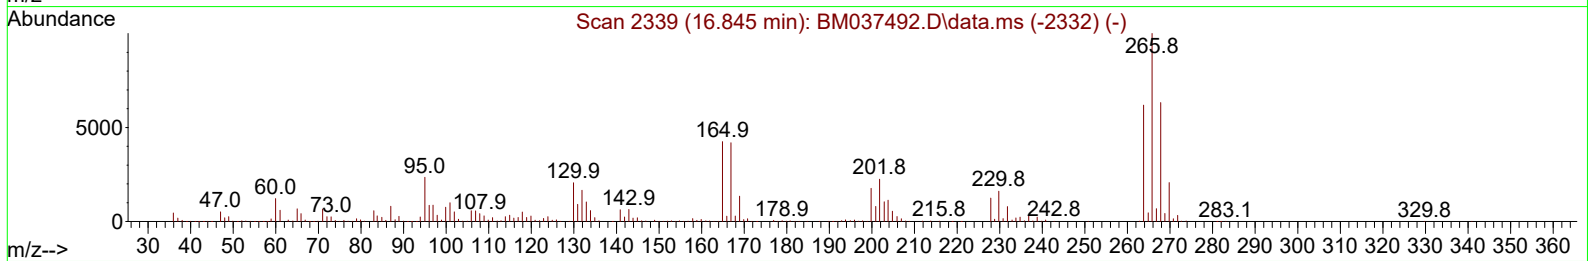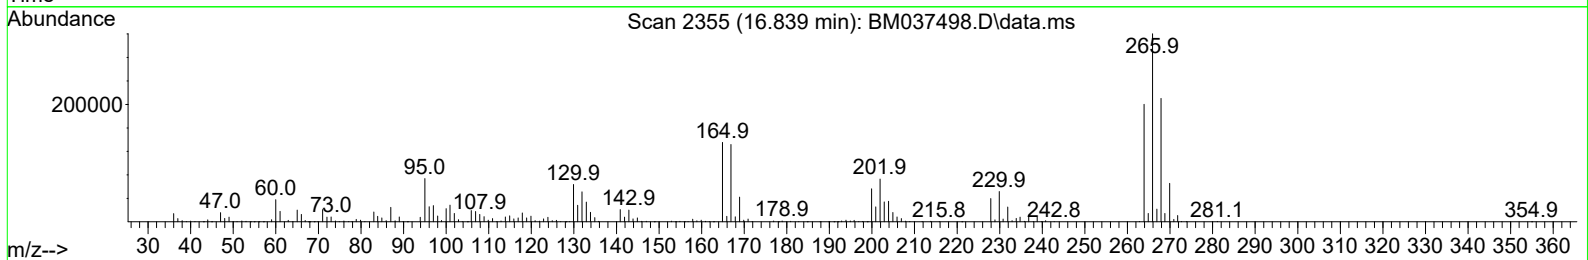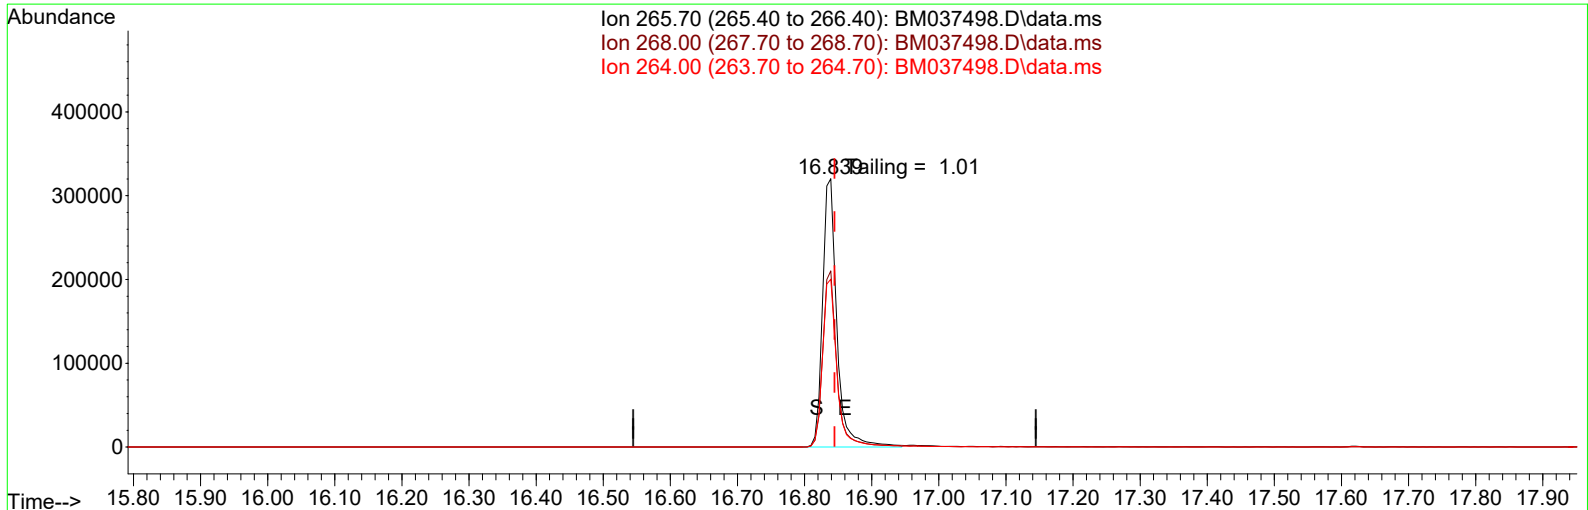

TIC: BM037498.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.006) 0.00 ng




response 474426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	65.66
264.00	61.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111422\
Data File : BM037498.D
Acq On : 14 Nov 2022 09:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 14 13:04:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM111222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 01:42:00 2022
Response via : Initial Calibration

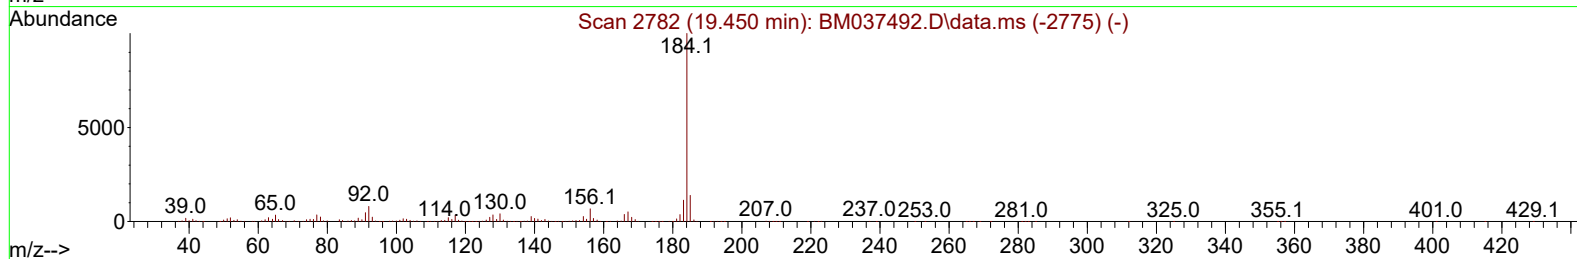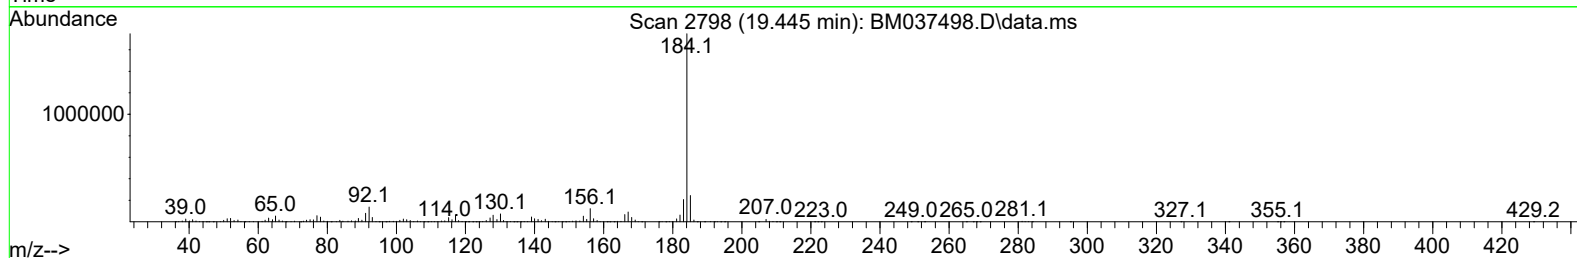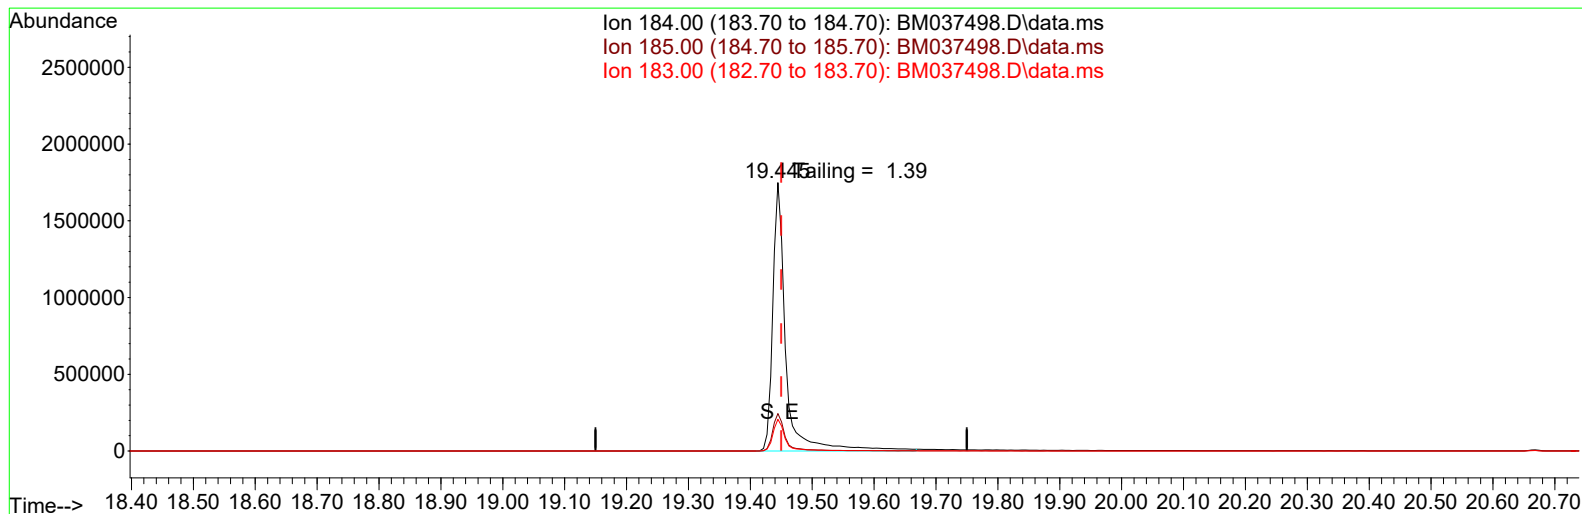

TIC: BM037498.D\data.ms

(77) Benzidine

19.445min (-0.005) 31960.88 ng

response 2619713

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.98
183.00	11.30	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/14/2022	BNA_M	<u>BM037498.D</u>
Compound Name	Response	Retention Time
DDT	1538132	20.668
DDD	19503	20.28
DDE	1423	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20926	1559058	1.34

Instrument :
BNA_M
ClientSampleId :
DFTPP