

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111515\
 Data File : BM003130.D
 Acq On : 15 Nov 2015 13:47
 Operator : UM/IZ
 Sample : G4401-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC790

Quant Time: Nov 16 02:41:50 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	104338	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	454520	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	251902	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.13	188	540063	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	552153	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	573324	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	6351	2.87	ng/uL	0.00
5) Phenol-d5	6.90	99	121036	14.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	73005	15.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	108010	15.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	101975	15.33	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	48207	17.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	48635	17.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	95642	15.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	119461	14.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	315081	16.63	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	342453	14.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	34970	10.95	ng/ul	0.00
58) Fluorene-d10	15.39	176	242735	14.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	18815	7.52	ng/ul	0.00
71) Anthracene-d10	17.23	188	342975	14.33	ng/ul	0.00
79) Pyrene-d10	19.53	212	339786	12.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	331076	12.15	ng/ul	0.00

Target Compounds


						Qvalue
6) Phenol	6.93	94	10328	1.22	ng/ul	94
28) Naphthalene	10.59	128	29712	1.30	ng/ul	99
45) Dimethylphthalate	13.85	163	175583	9.09	ng/ul	99
48) Acenaphthylene	14.11	152	47528	1.85	ng/ul	98
50) Acenaphthene	14.46	153	21096	1.22	ng/ul	97
59) Fluorene	15.44	166	33002	1.76	ng/ul#	97
70) Phenanthrene	17.18	178	466977	15.27	ng/ul	99
72) Anthracene	17.27	178	324263	10.86	ng/ul	99
77) Fluoranthene	19.20	202	1587607	51.34	ng/ul	96
80) Pyrene	19.56	202	1275812	35.32	ng/ul#	93
83) Benzo(a)anthracene	21.37	228	715004	23.58	ng/ul	95
85) Chrysene	21.37	228	714211	23.81	ng/ul	98
88) Benzo(b)fluoranthene	22.92	252	827591	25.06	ng/ul	97
89) Benzo(k)fluoranthene	22.92	252	162134	5.26	ng/ul	96
91) Benzo(a)pyrene	23.40	252	355637	11.37	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.87	276	380064	11.05	ng/ul#	89
93) Dibenzo(a,h)anthracene	25.88	278	105386	3.89	ng/ul	98
94) Benzo(g,h,i)perylene	26.57	276	272646	8.81	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111515\
Data File : BM003130.D
Acq On : 15 Nov 2015 13:47
Operator : UM/IZ
Sample : G4401-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC790

Quant Time: Nov 16 02:41:50 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 16 02:34:54 2015
Response via : Initial Calibration

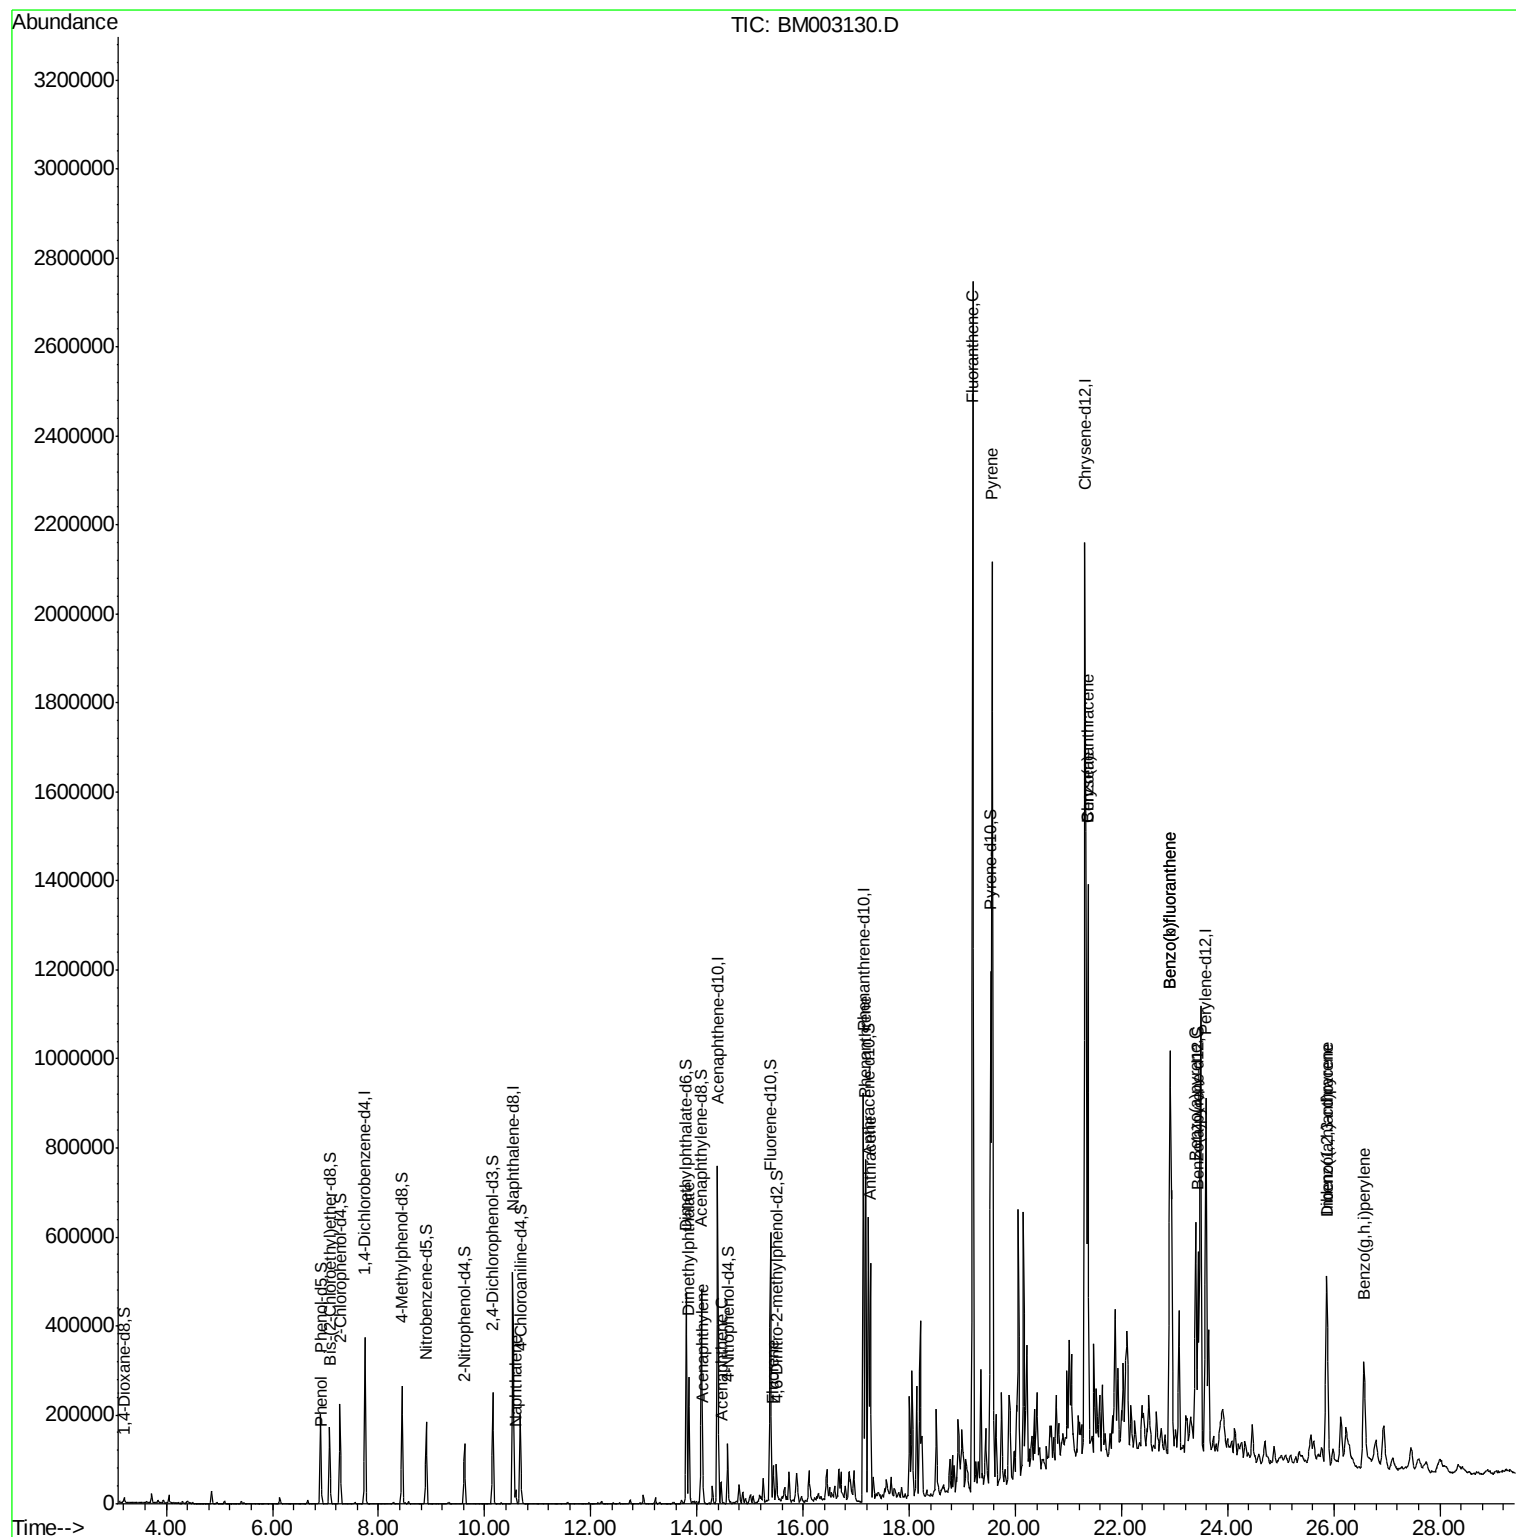

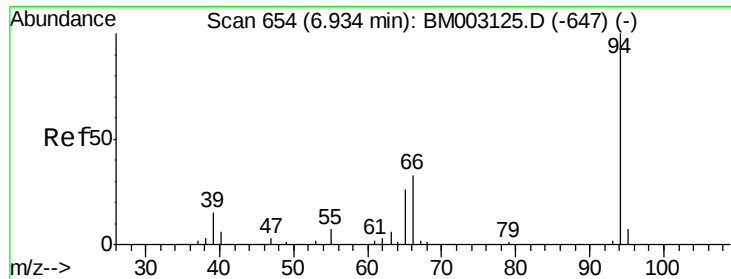

#6

Phenol

Concen: 1.22 ng/ul

RT: 6.93 min Scan# 654

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790


Tgt Ion: 94 Resp: 10328

Ion Ratio Lower Upper

94 100

65 26.6 18.7 28.1




66 33.1 24.2 36.2



Abundance Ion 94.00 (93.70 to 94.70): BM003130.D (-620) (-)

Ion 65.00 (64.70 to 65.70): BM003130.D (-620) (-)

Ion 66.00 (65.70 to 66.70): BM003130.D (-620) (-)

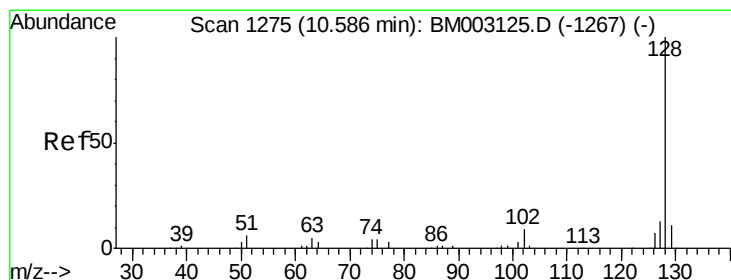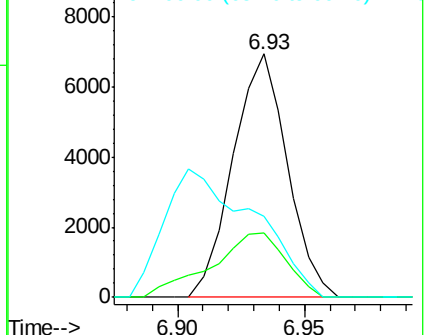

#28

Naphthalene

Concen: 1.30 ng/ul

RT: 10.59 min Scan# 1275

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47


Tgt Ion: 128 Resp: 29712

Ion Ratio Lower Upper

128 100

129 11.7 8.8 13.2



127 13.0 10.5 15.7

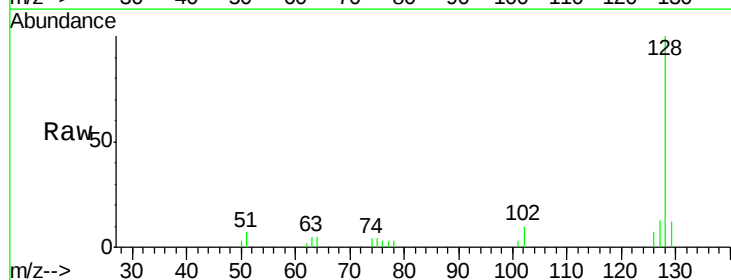


Abundance Ion 128.00 (127.70 to 128.70): BM003130.D (-1241) (-)

Ion 129.00 (128.70 to 129.70): BM003130.D (-1241) (-)

Ion 127.00 (126.70 to 127.70): BM003130.D (-1241) (-)

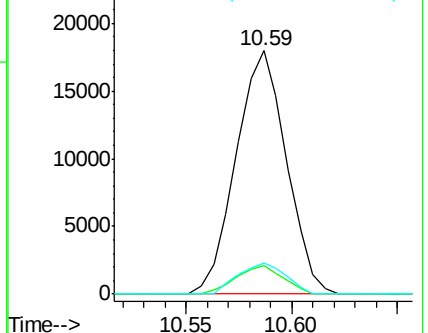

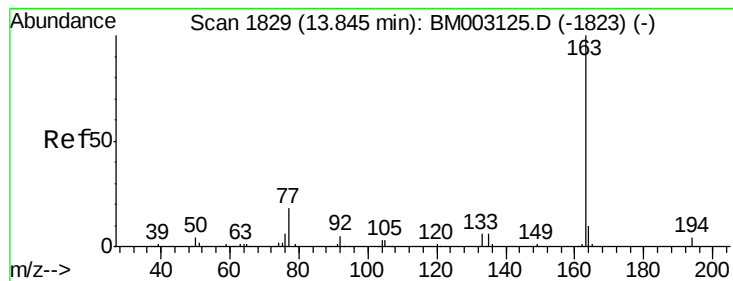

#45

Dimethylphthalate

Concen: 9.09 ng/ul

RT: 13.85 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790


Tgt Ion:163 Resp: 175583

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8




164 10.3 7.8 11.8

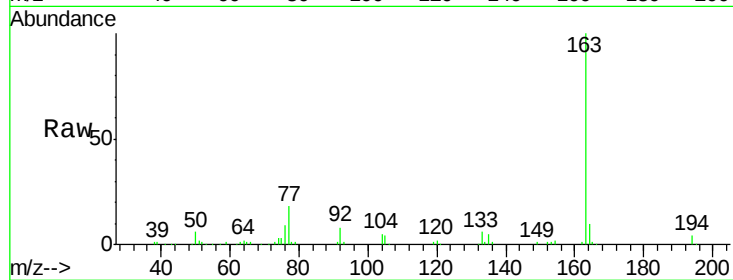

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

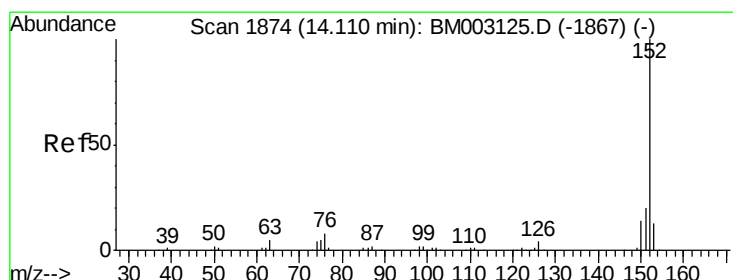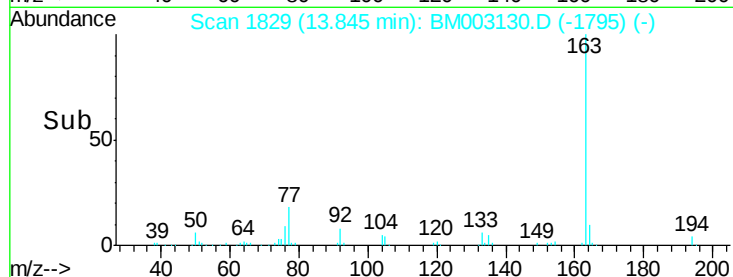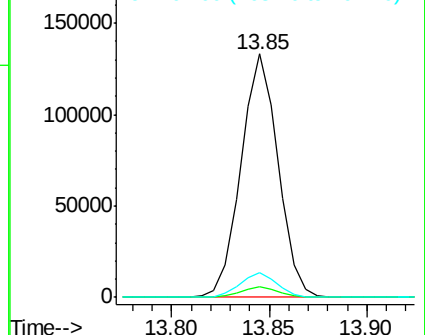

#48

Acenaphthylene

Concen: 1.85 ng/ul

RT: 14.11 min Scan# 1874

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47


Tgt Ion:152 Resp: 47528

Ion Ratio Lower Upper

152 100

151 20.2 15.8 23.6



153 13.9 10.3 15.5

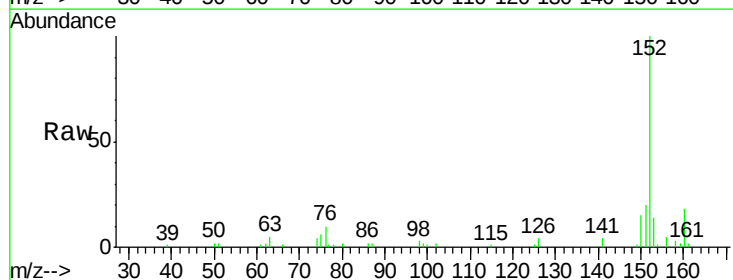


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

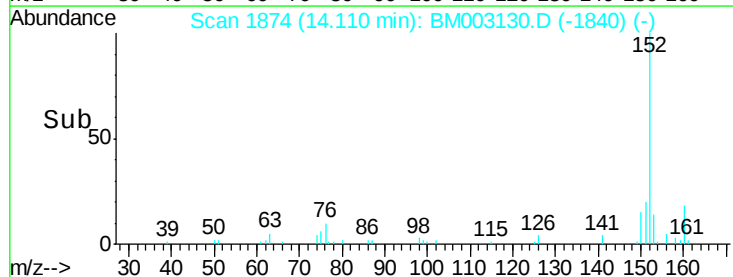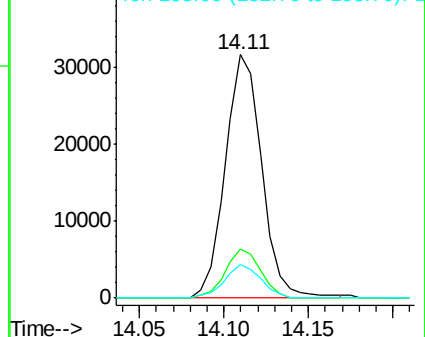

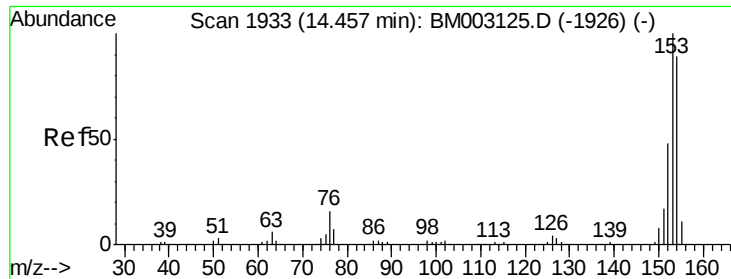

#50

Acenaphthene

Concen: 1.22 ng/ul

RT: 14.46 min Scan# 1933

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790


Tgt Ion:153 Resp: 21096

Ion Ratio Lower Upper

153 100

152 49.2 37.0 55.6




154 87.1 71.0 106.4

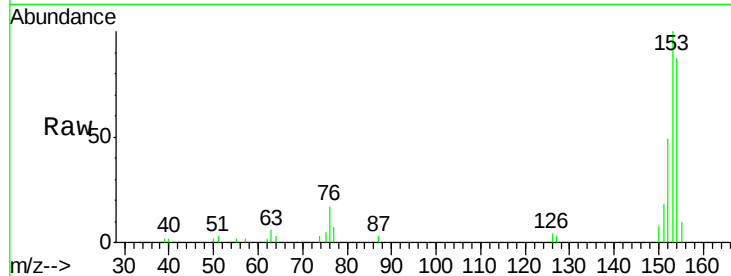

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

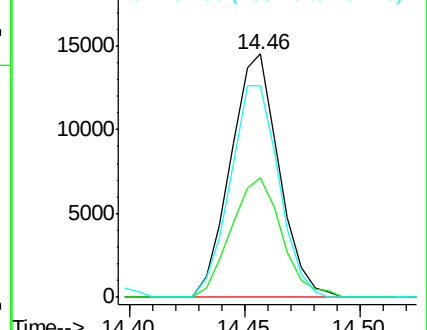

#59

Fluorene

Concen: 1.76 ng/ul

RT: 15.44 min Scan# 2100

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47


Tgt Ion:166 Resp: 33002

Ion Ratio Lower Upper

166 100

165 98.4 77.2 115.8



167 16.1 10.2 15.4#




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

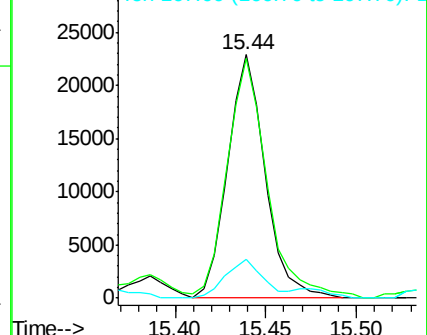

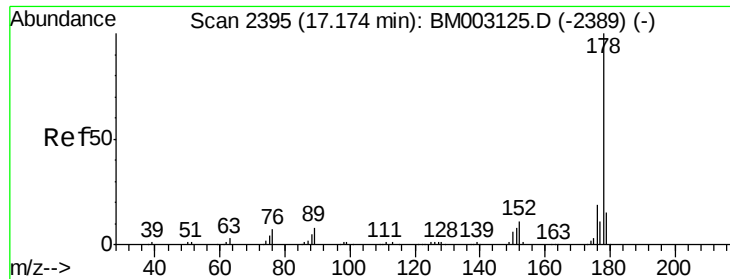

#70

Phenanthrene

Concen: 15.27 ng/ul

RT: 17.18 min Scan# 2396

Delta R.T. 0.01 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790


Tgt Ion:178 Resp: 466977

Ion Ratio Lower Upper

178 100

179 15.4 12.2 18.4




176 19.1 14.7 22.1

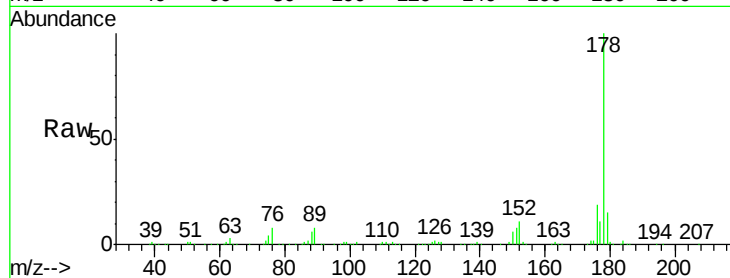

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

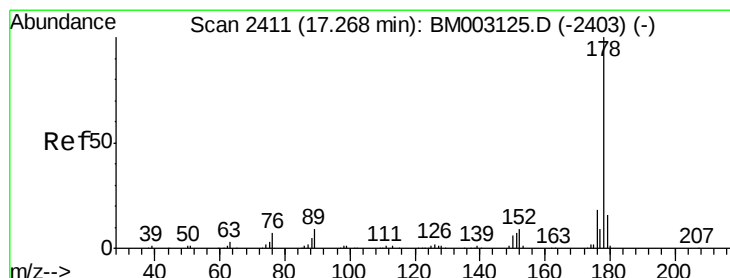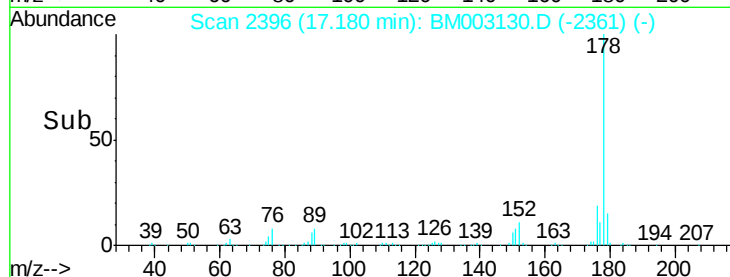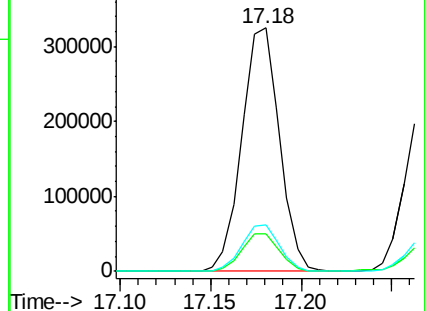

#72

Anthracene

Concen: 10.86 ng/ul

RT: 17.27 min Scan# 2411

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47


Tgt Ion:178 Resp: 324263

Ion Ratio Lower Upper

178 100

179 15.2 12.3 18.5



176 18.2 14.4 21.6

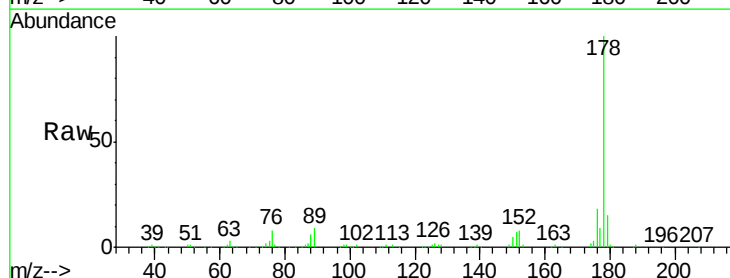


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

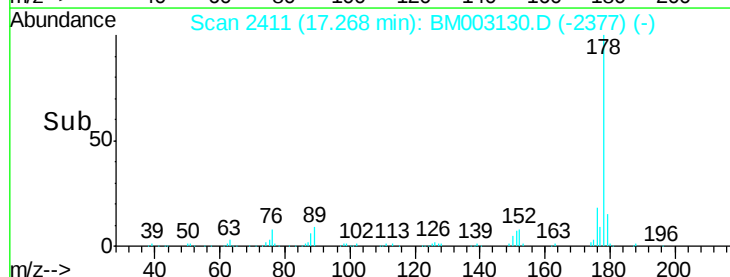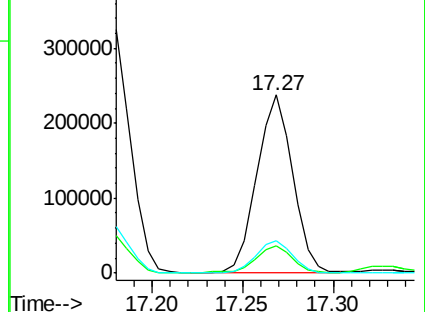

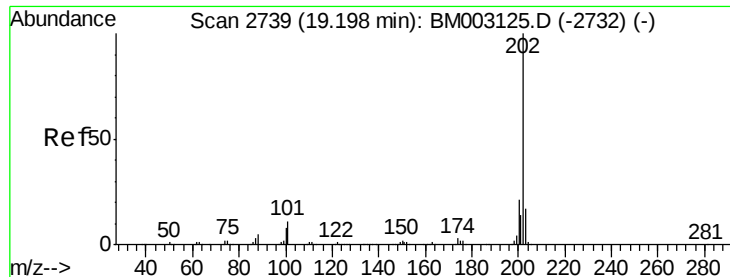

#77

Fluoranthene

Concen: 51.34 ng/ul

RT: 19.20 min Scan# 2739

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790


Tgt Ion:202 Resp: 1587607

Ion Ratio Lower Upper

202 100

101 11.2 10.4 15.6




100 8.5 7.8 11.6

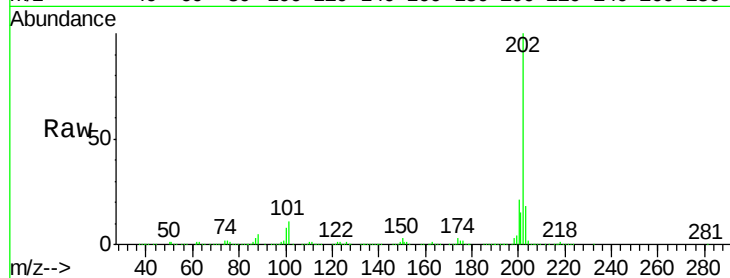

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

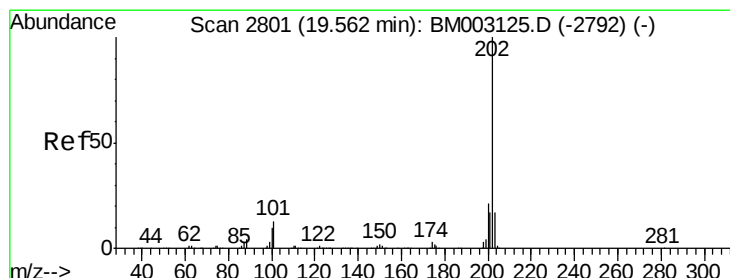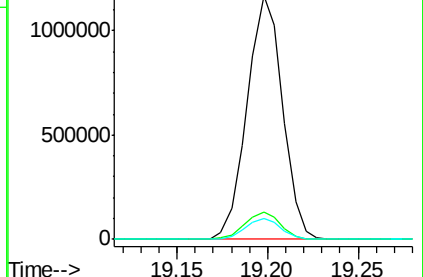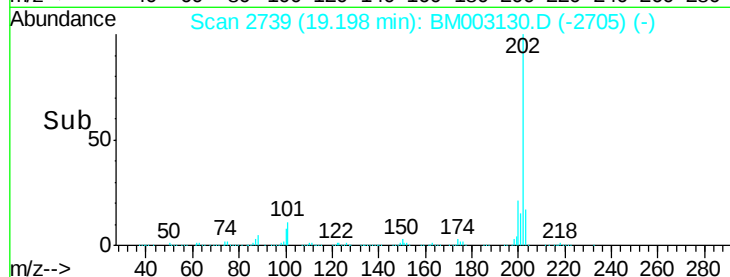

#80

Pyrene

Concen: 35.32 ng/ul

RT: 19.56 min Scan# 2801

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47


Tgt Ion:202 Resp: 1275812

Ion Ratio Lower Upper

202 100

101 13.0 12.6 18.8



100 10.5 10.6 15.8#

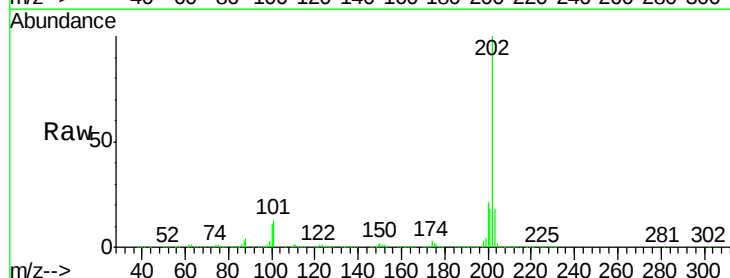


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

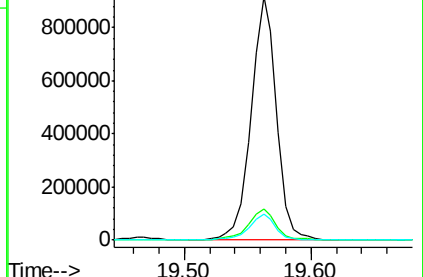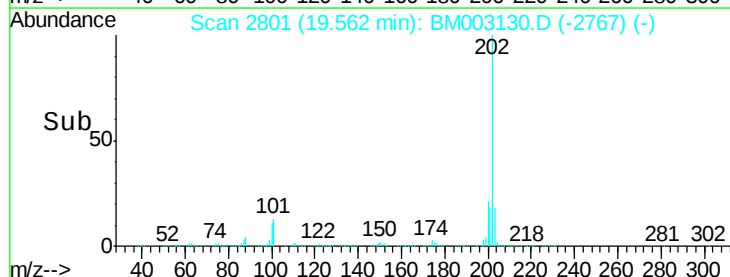



#83

Benzo(a)anthracene

Concen: 23.58 ng/ul

RT: 21.37 min Scan# 3108

Delta R.T. 0.06 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790





Tgt Ion:228 Resp: 715004

Ion Ratio Lower Upper

228 100

229 20.7 15.6 23.4

226 30.1 21.0 31.6

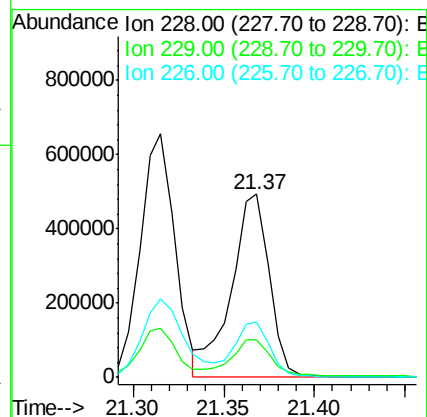

#85

Chrysene

Concen: 23.81 ng/ul

RT: 21.37 min Scan# 3108

Delta R.T. 0.01 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47




Tgt Ion:228 Resp: 714211


Ion Ratio Lower Upper

228 100

226 30.1 23.3 34.9

229 20.7 15.8 23.6

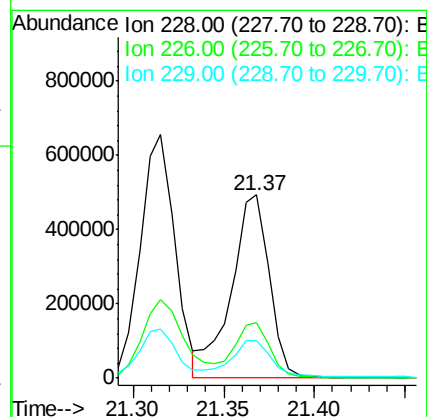



#88

Benzo(b)fluoranthene

Concen: 25.06 ng/u1

RT: 22.92 min Scan# 3371

Delta R.T. 0.01 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790


Tgt Ion:252 Resp: 827591

Ion Ratio Lower Upper

252 100

253 22.6 17.4 26.2




125 11.3 10.7 16.1



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

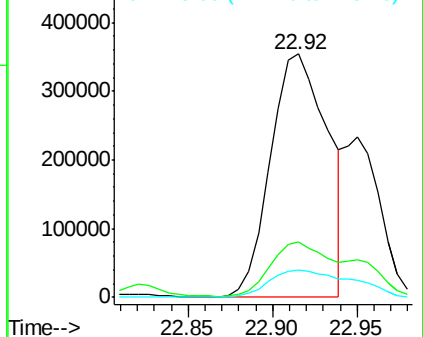

#89

Benzo(k)fluoranthene

Concen: 5.26 ng/u1

RT: 22.92 min Scan# 3371

Delta R.T. -0.04 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47


Tgt Ion:252 Resp: 162134

Ion Ratio Lower Upper

252 100

253 22.6 17.4 26.0



125 11.3 11.1 16.7




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

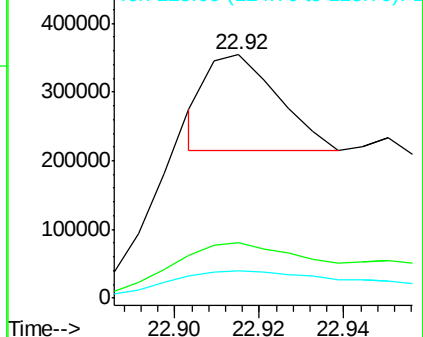

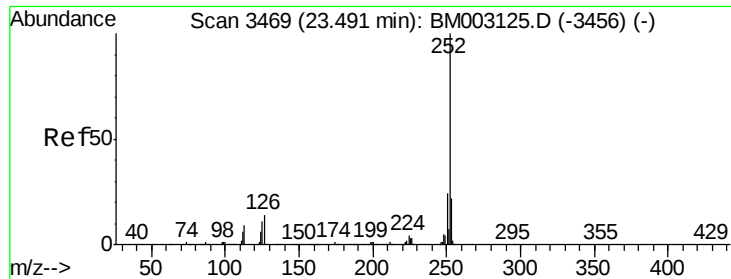

#91

Benzo(a)pyrene

Concen: 11.37 ng/ul

RT: 23.40 min Scan# 3453

Delta R.T. -0.09 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47





Instrument :

BNA_M

ClientSampleId :

BC790

Tgt Ion:	252	Resp:	355637
Ion Ratio	Lower	Upper	
252	100		
253	22.3	17.1	25.7
125	15.1	11.9	17.9

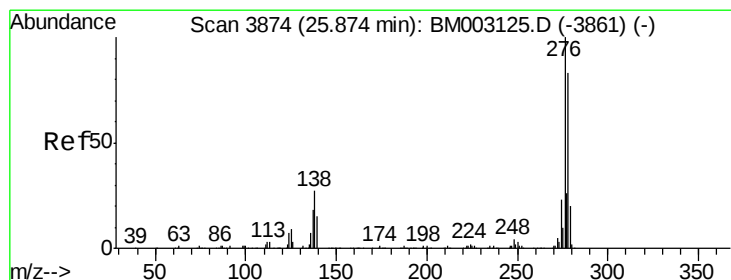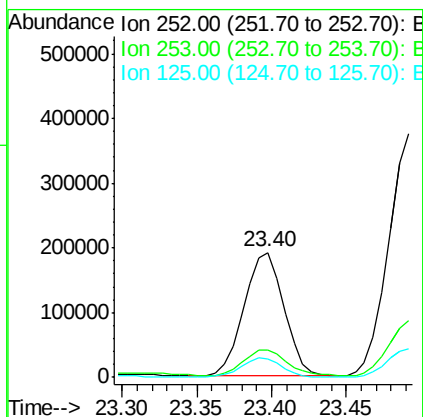

#92

Indeno(1,2,3-cd)pyrene

Concen: 11.05 ng/ul




RT: 25.87 min Scan# 3873


Delta R.T. -0.01 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Tgt Ion:	276	Resp:	380064
Ion Ratio	Lower	Upper	
276	100		
138	22.8	26.6	40.0#
277	25.0	20.2	30.4

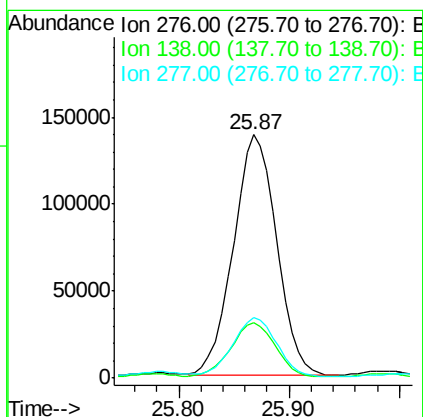

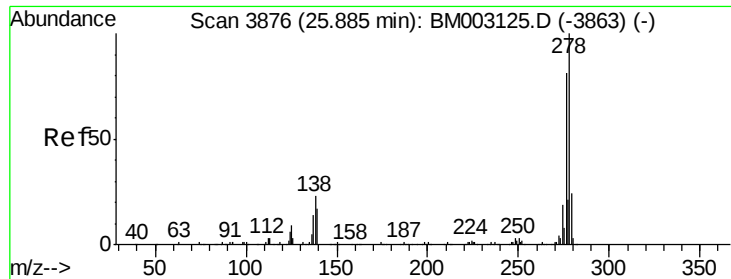

#93

Dibenzo(a,h)anthracene

Concen: 3.89 ng/ul

RT: 25.88 min Scan# 3875

Delta R.T. -0.01 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47

Instrument :

BNA_M

ClientSampleId :

BC790


Tgt Ion:278 Resp: 105386

Ion Ratio Lower Upper

278 100

139 21.9 18.8 28.2




279 24.5 19.3 28.9

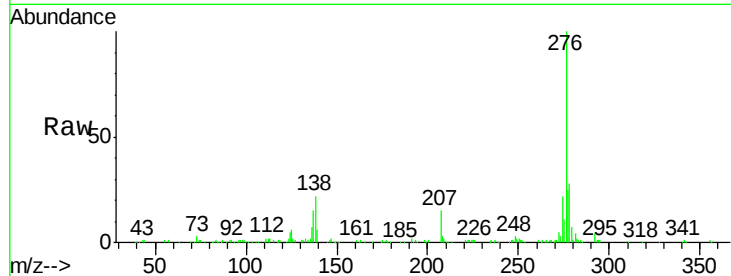

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

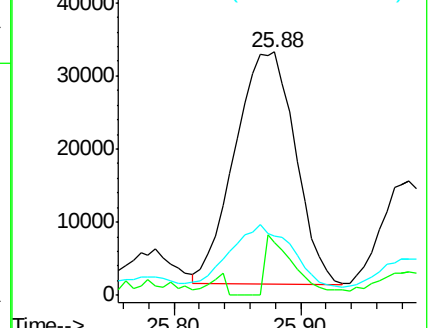

#94

Benzo(g,h,i)perylene

Concen: 8.81 ng/ul

RT: 26.57 min Scan# 3993

Delta R.T. 0.00 min

Lab File: BM003130.D

Acq: 15 Nov 2015 13:47


Tgt Ion:276 Resp: 272646

Ion Ratio Lower Upper

276 100

138 23.8 23.8 35.6

277 24.0 19.4 29.2



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

