


Data Path : Z:\HPCHEM1\BNA_M\Data\BM111515\
Data File : BM003126.D
Acq On : 15 Nov 2015 11:23
Operator : UM/IZ
Sample : G4401-11
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC784

Quant Time: Nov 16 13:25:43 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 16 02:34:54 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:29:12 PM

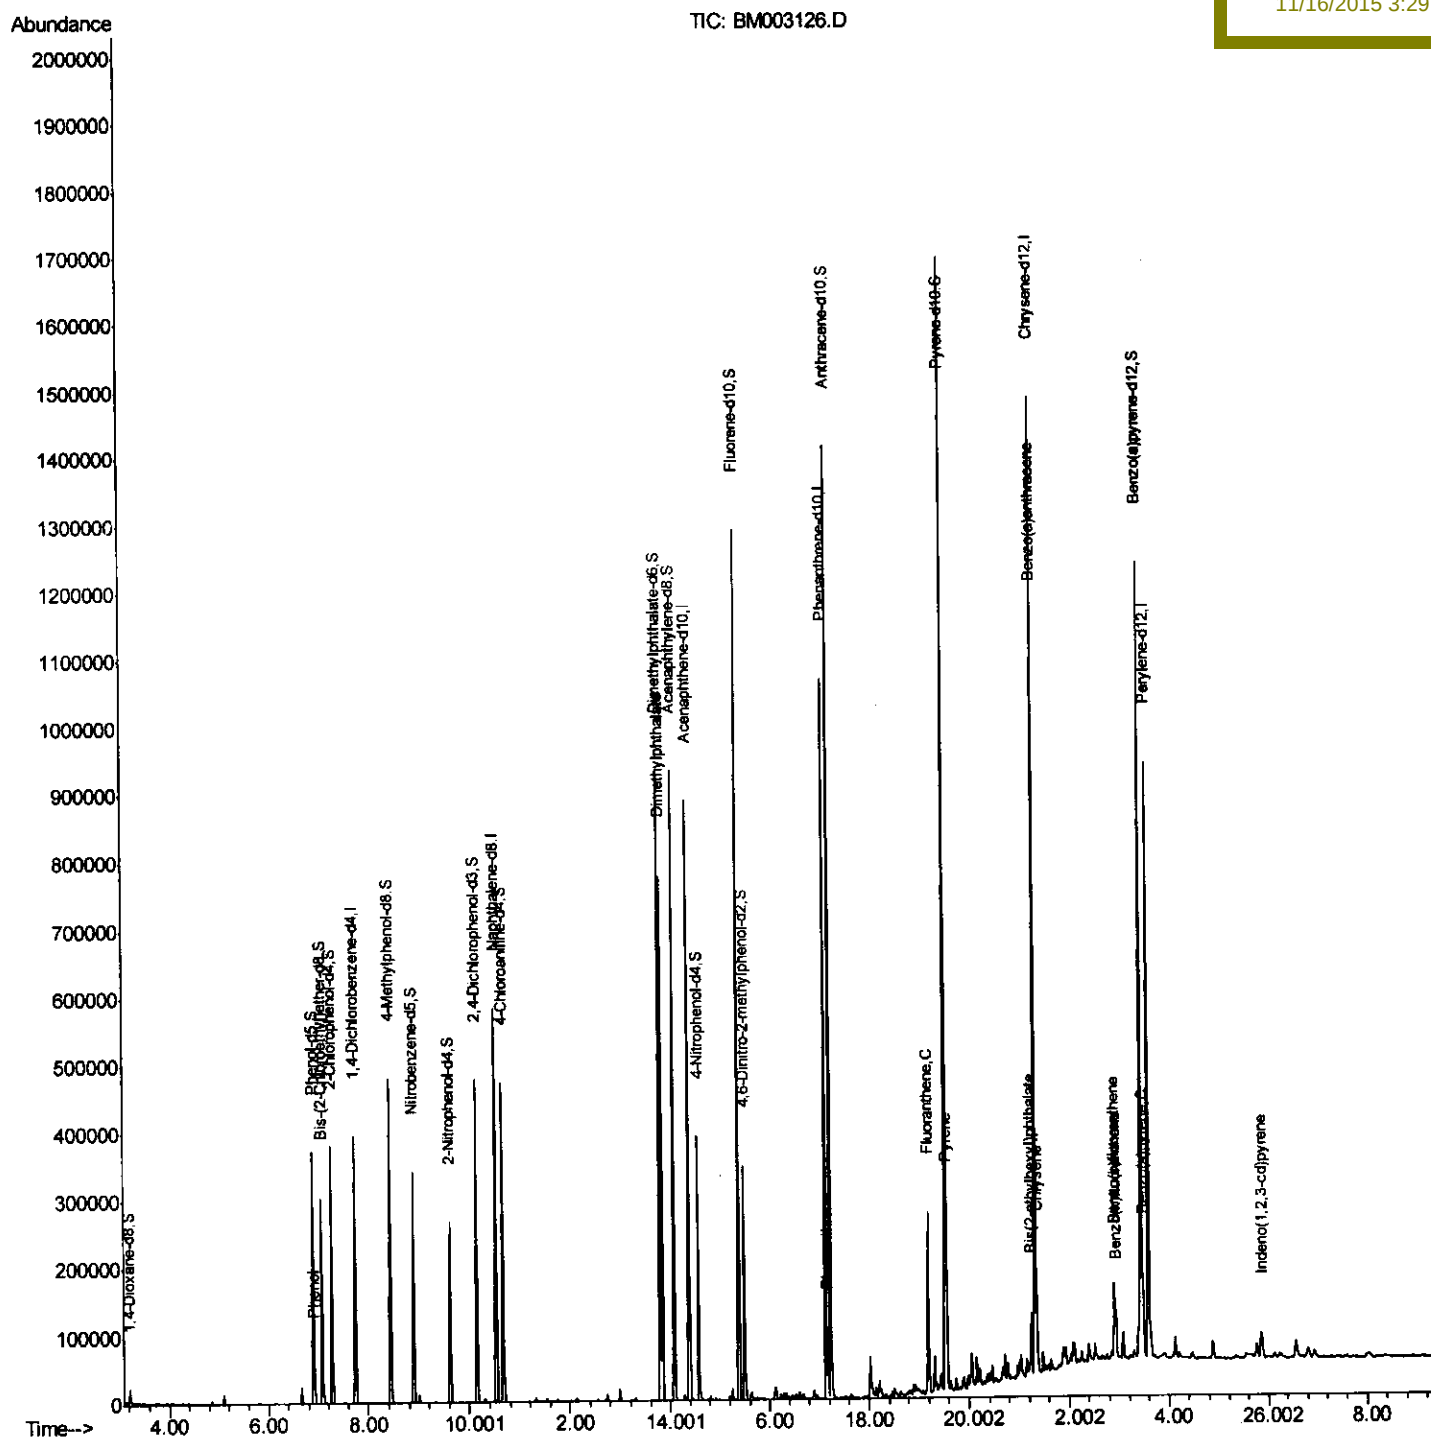

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111515\
 Data File : BM003126.D
 Acq On : 15 Nov 2015 11:23
 Operator : UM/IZ
 Sample : G4401-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC784

Quant Time: Nov 16 02:45:00 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:29:12 PM

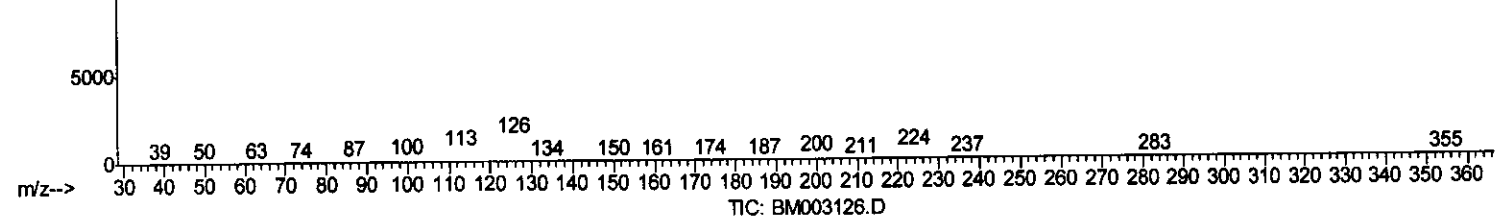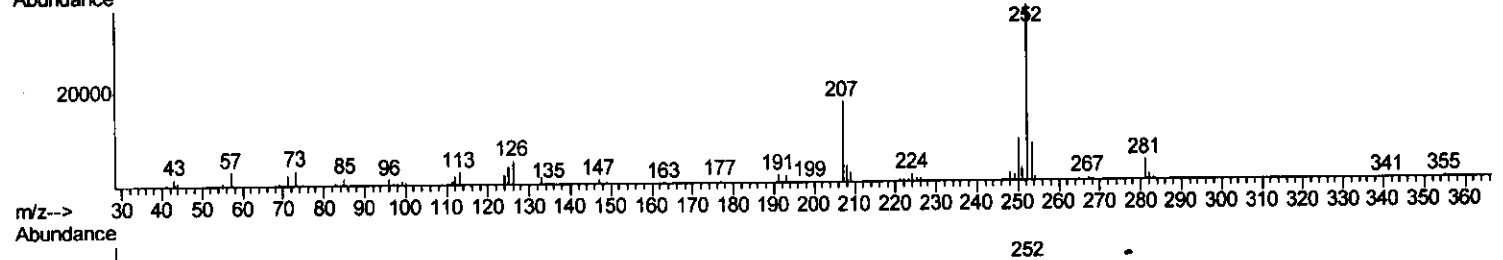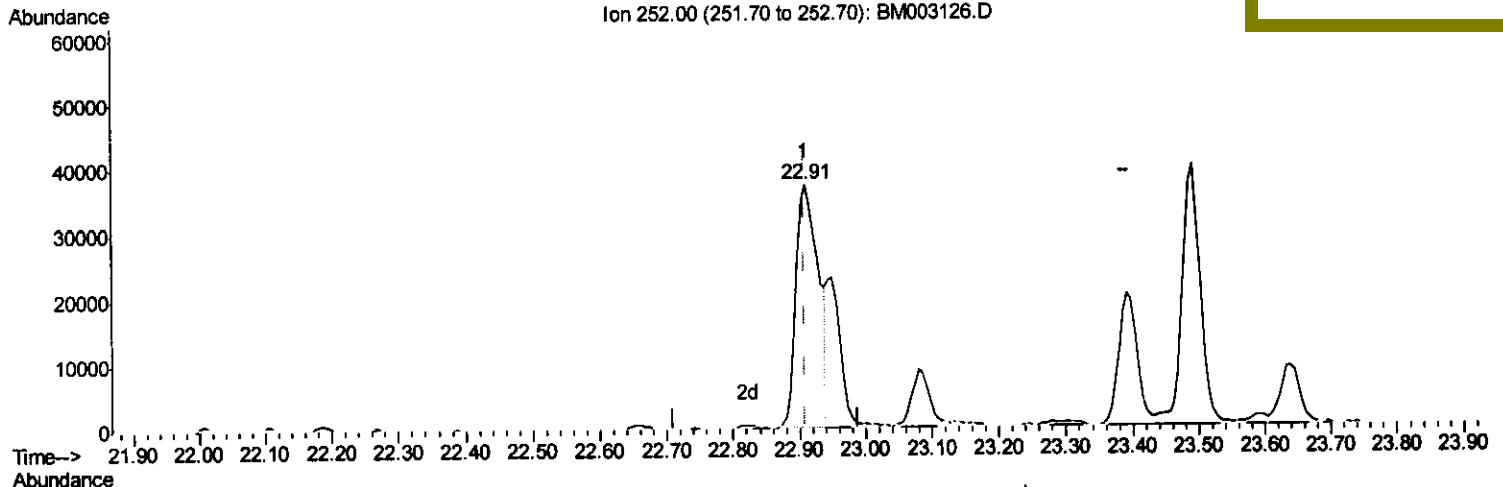

(88) Benzo(b)fluoranthene
 22.909min (+0.000) 2.53ng/ul
 response 89772

Ion	Exp%	Act%
252.00	100	100
253.00	21.80	22.10
125.00	13.40	10.89
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111515\
 Data File : BM003126.D
 Acq On : 15 Nov 2015 11:23
 Operator : UM/IZ
 Sample : G4401-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC784

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:29:12 PM

Quant Time: Nov 16 02:45:00 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

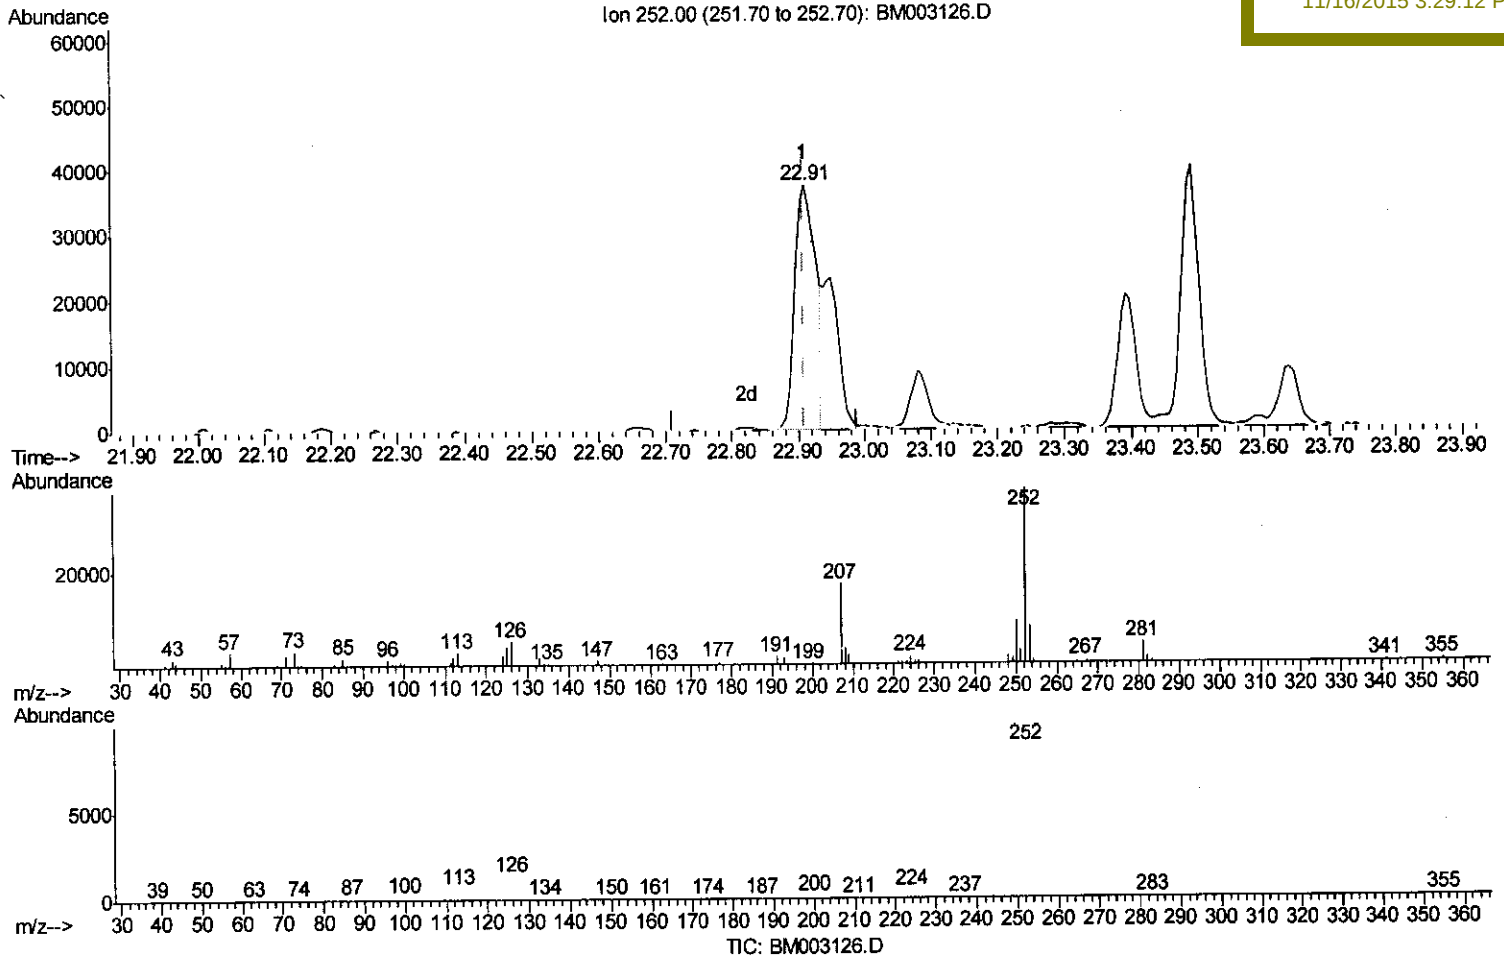

(88) Benzo(b)fluoranthene

22.909min (+0.000) 2.31ng/ul m

response 82172

Ion	Exp%	Act%
252.00	100	100
253.00	21.80	22.10
125.00	13.40	10.89
0.00	0.00	0.00

U.M
 11/17/15

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111515\
 Data File : BM003126.D
 Acq On : 15 Nov 2015 11:23
 Operator : UM/IZ
 Sample : G4401-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC784

Quant Time: Nov 16 02:45:00 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:29:12 PM

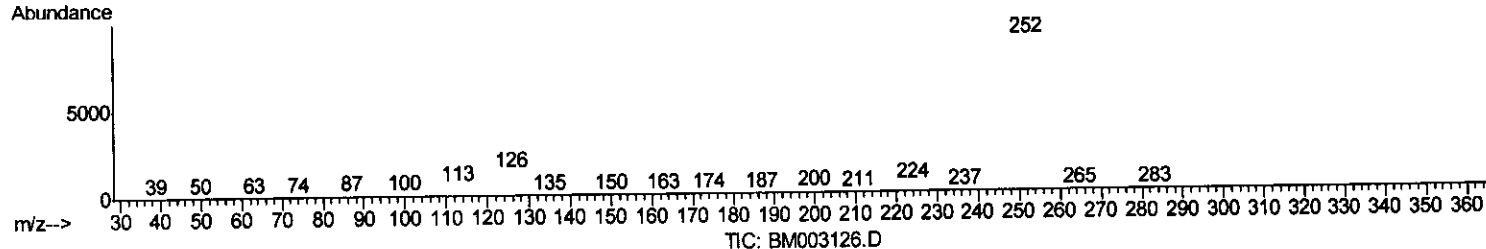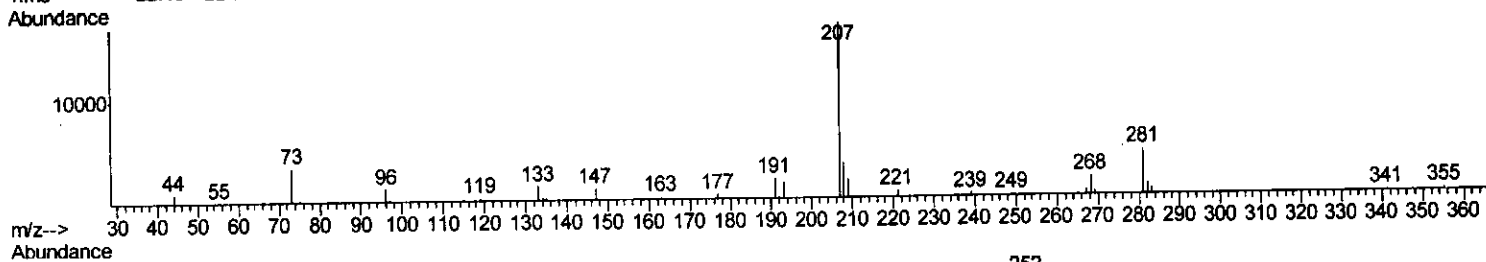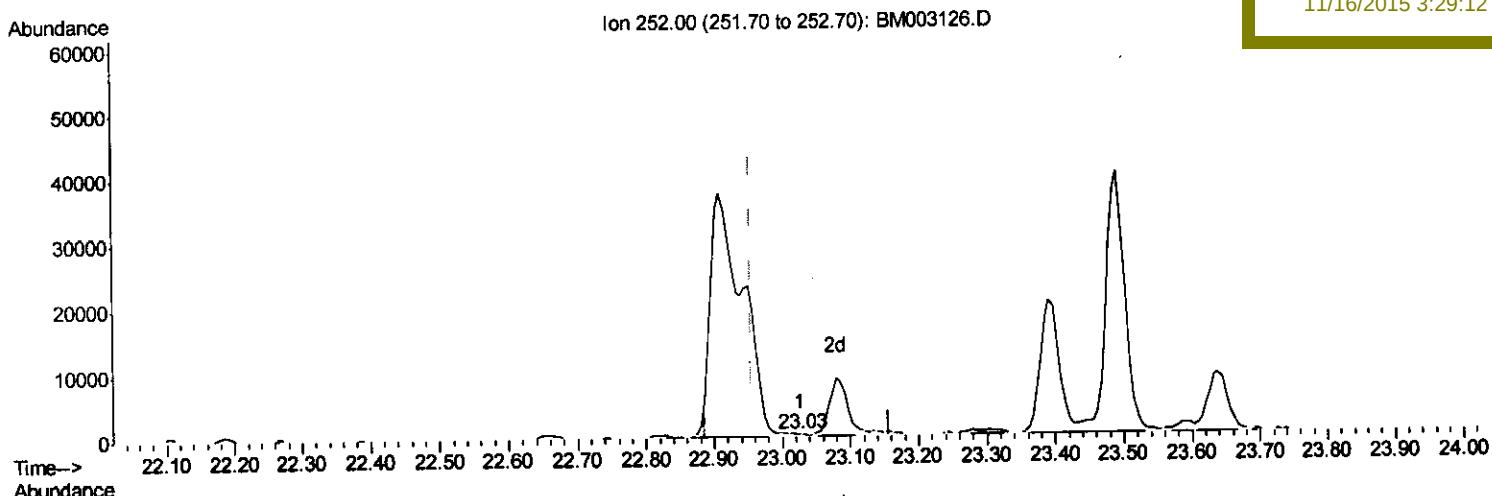

(89) Benzo(k)fluoranthene

23.027min (+0.071) 0.01ng/ul

response 255

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	88.19#
125.00	13.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111515\
 Data File : BM003126.D
 Acq On : 15 Nov 2015 11:23
 Operator : UM/IZ
 Sample : G4401-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC784

Quant Time: Nov 16 02:45:00 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:29:12 PM

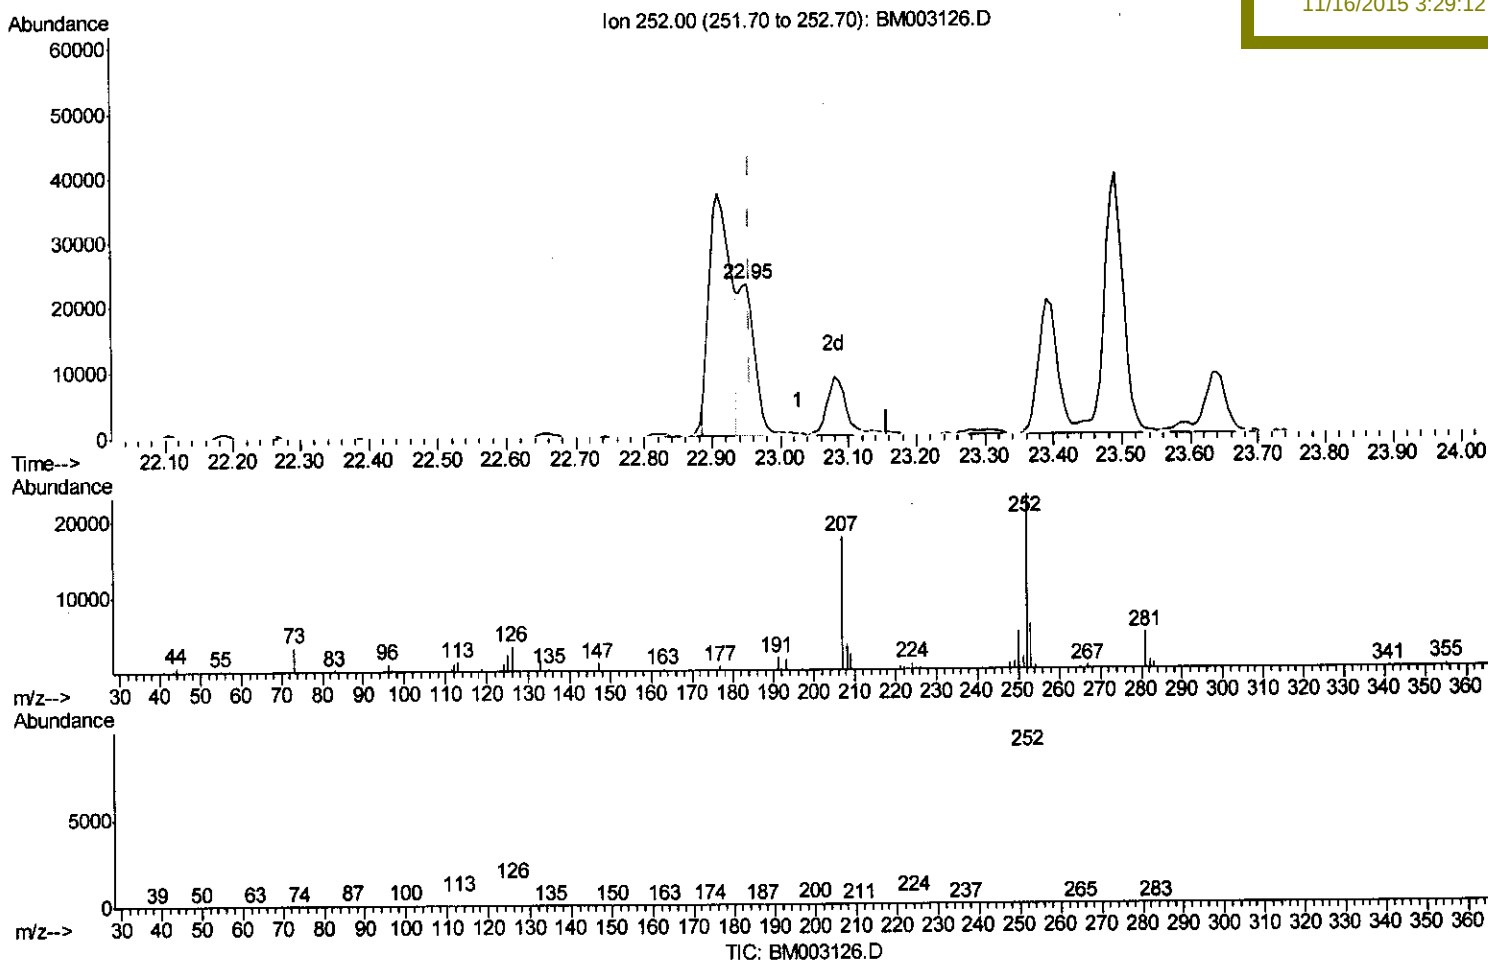

(89) Benzo(k)fluoranthene

22.950min (-0.006) 1.23ng/ul m U.M
 response 40831 11/17/15

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	26.05#
125.00	13.90	10.63#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM111515\
 Data File : BM003126.D
 Acq On : 15 Nov 2015 11:23
 Operator : UM/IZ
 Sample : G4401-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC784

Quant Time: Nov 16 02:49:27 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:29:12 PM

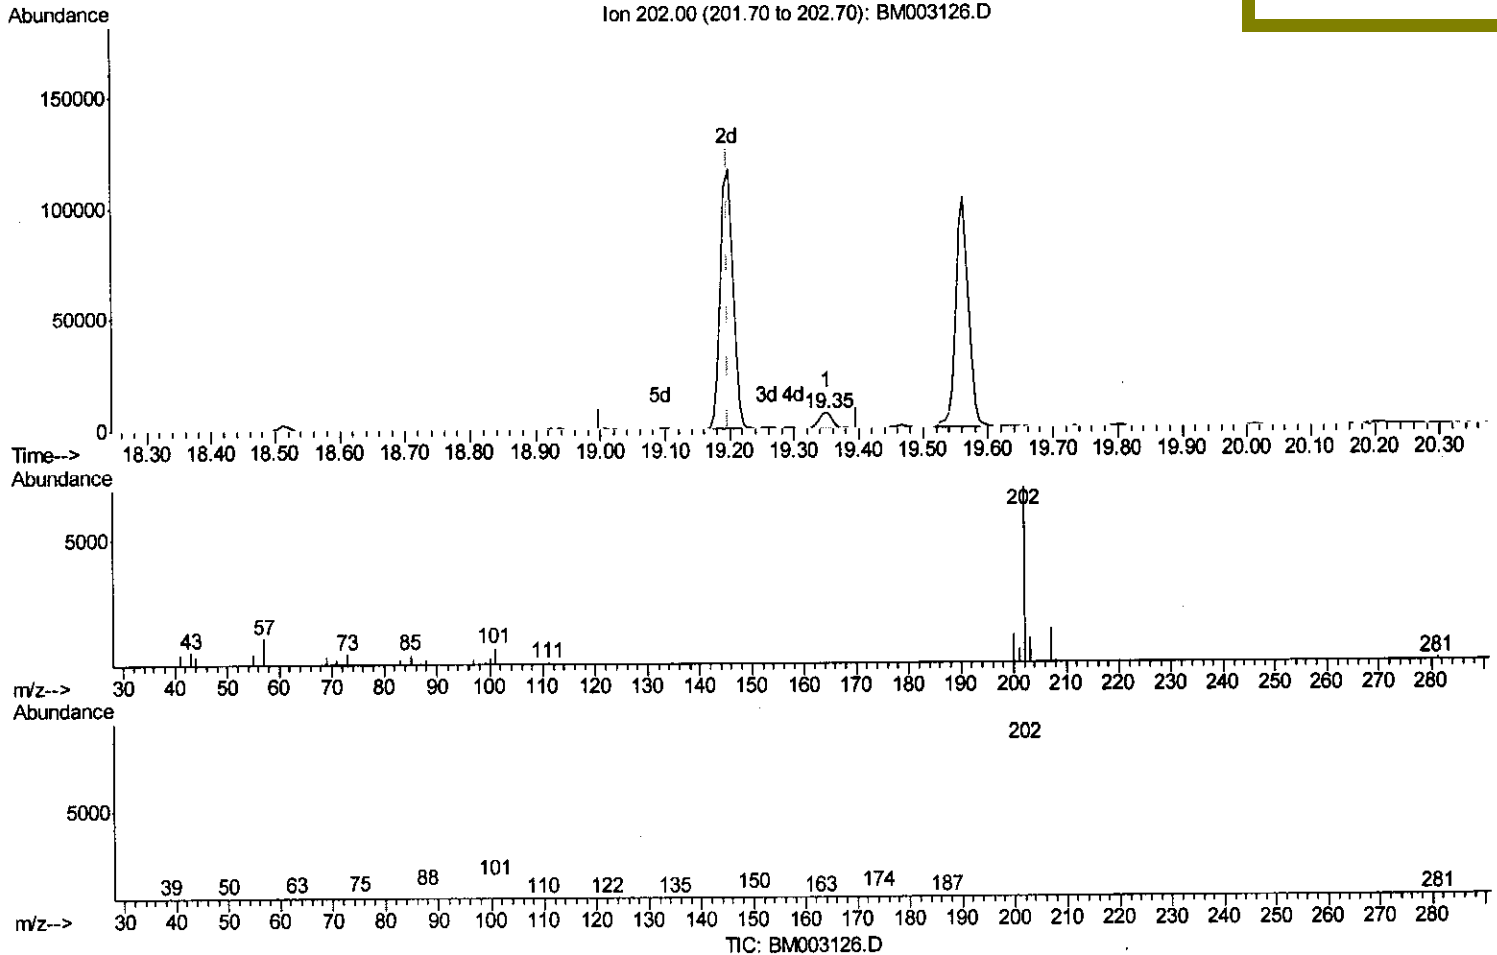

(77) Fluoranthene (C)

19.351min (+0.153) 0.27ng/ul

response 9658

Ion	Exp%	Act%
202.00	100	100
101.00	13.00	13.04
100.00	9.70	7.79
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM111515\
 Data File : BM003126.D
 Acq On : 15 Nov 2015 11:23
 Operator : UM/IZ
 Sample : G4401-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC784

Quant Time: Nov 16 02:49:27 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:29:12 PM

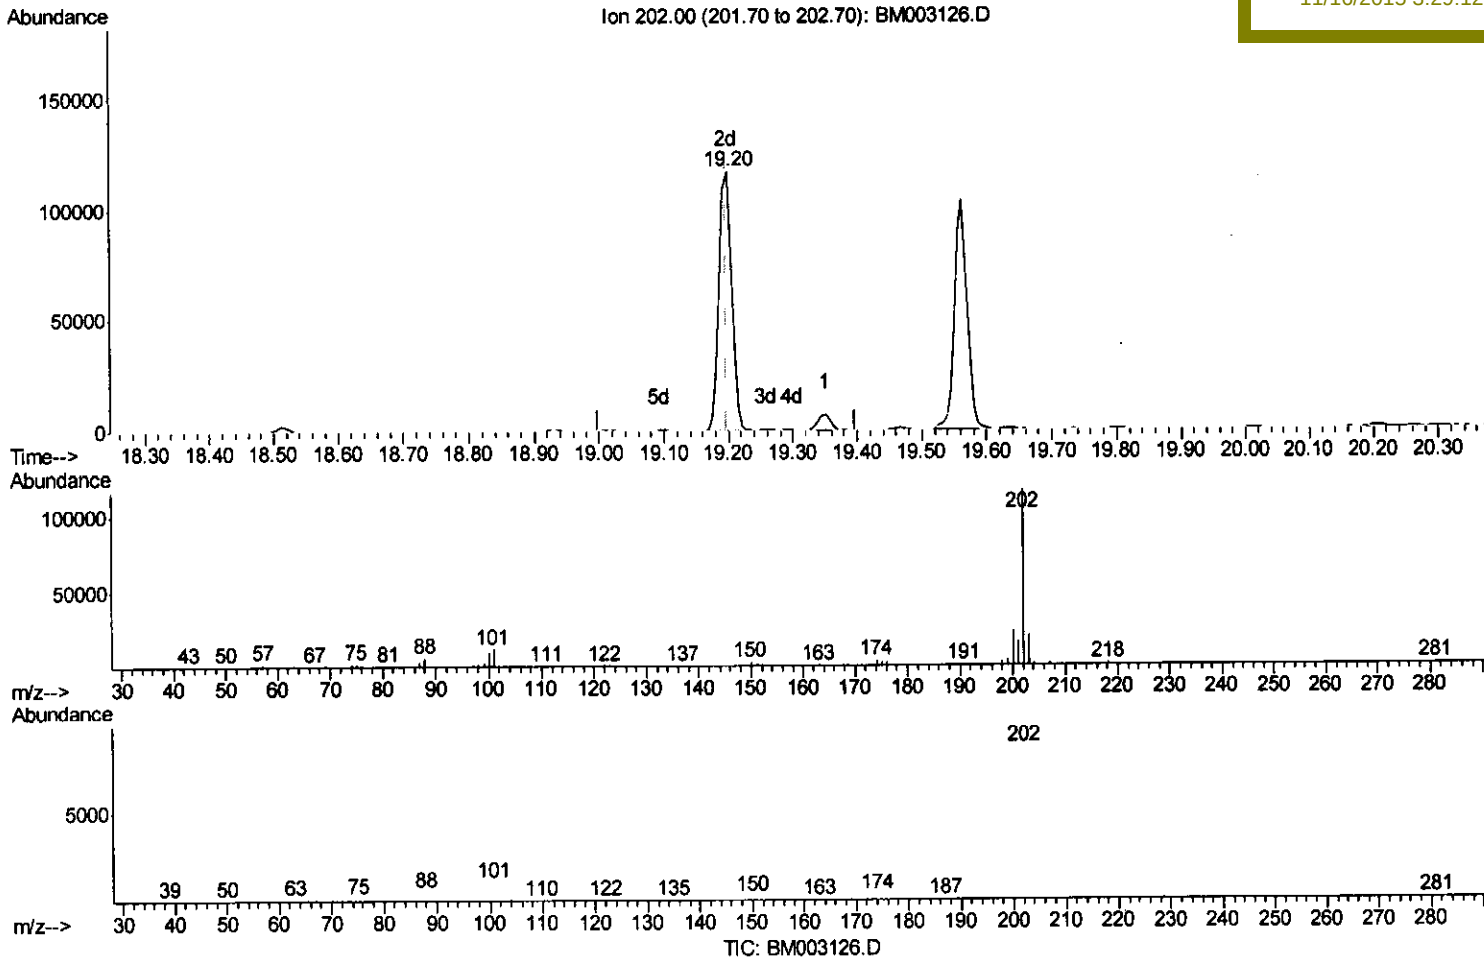

(77) Fluoranthene (C)

19.198min (+0.000) 4.44ng/ul m

response 157372

Ion	Exp%	Act%
202.00	100	100
101.00	13.00	10.38#
100.00	9.70	8.15
0.00	0.00	0.00

U.M
 11/17/15

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111515\
 Data File : BM003126.D
 Acq On : 15 Nov 2015 11:23
 Operator : UM/IZ
 Sample : G4401-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC784

Quant Time: Nov 16 13:25:43 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 02:34:54 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:29:12 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	110416	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	503101	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	287942	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.13	188	619236	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	632208	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	616899	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	10494	4.48	ng/uL	0.00
5) Phenol-d5	6.90	99	219524	25.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	126012	24.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	186545	25.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	187371	26.62	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	87590	28.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	96478	31.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	179109	25.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	263257	29.18	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	625930	28.90	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	686146	25.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	99272	27.19	ng/ul	0.00
58) Fluorene-d10	15.39	176	507197	27.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	76001	26.50	ng/ul	0.00
71) Anthracene-d10	17.23	188	776604	28.29	ng/ul	0.00
79) Pyrene-d10	19.53	212	819800	26.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	862178	29.41	ng/ul	0.00

Target Compounds						Qvalue
6) Phenol	6.93	94	12441	1.38	ng/ul#	91
45) Dimethylphthalate	13.85	163	503379	22.80	ng/ul	99
70) Phenanthrene	17.17	178	48627	1.39	ng/ul	98
77) Fluoranthene	19.20	202	157372m	4.44	ng/ul	
80) Pyrene	19.56	202	140222	3.39	ng/ul#	91
83) Benzo(a)anthracene	21.32	228	90847	2.62	ng/ul	95
84) Bis(2-ethylhexyl)phthalate	21.24	149	30900	1.62	ng/ul	99
85) Chrysene	21.36	228	78287	2.28	ng/ul	94
88) Benzo(b)fluoranthene	22.91	252	82172m	2.31	ng/ul	
89) Benzo(k)fluoranthene	22.95	252	40831m	1.23	ng/ul	
91) Benzo(a)pyrene	23.49	252	73795	2.19	ng/ul	96
92) Indeno(1,2,3-cd)pyrene	25.87	276	37466	1.01	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
 11/17/15