

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
 Data File : BM007885.D
 Acq On : 15 Nov 2016 10:42
 Operator : UM/SJ
 Sample : PB94685BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK85

Quant Time: Nov 16 01:22:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 01:19:46 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	860	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	2780	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1636	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	236134	0.40	ng/ul	0.09
16) Chrysene-d12	21.32	240	3095	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	220378	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1312	0.40	ng/ul	0.01
14) Fluoranthene-d10	19.15	212	2714	0.01	ng/ul	0.00
Target Compounds						
9) Fluorene	15.36	166	459	0.07	ng/ul#	30
17) Pyrene	19.51	202	438	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
Data File : BM007885.D
Acq On : 15 Nov 2016 10:42
Operator : UM/SJ
Sample : PB94685BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK85

Quant Time: Nov 16 01:22:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:19:46 2016
Response via : Initial Calibration

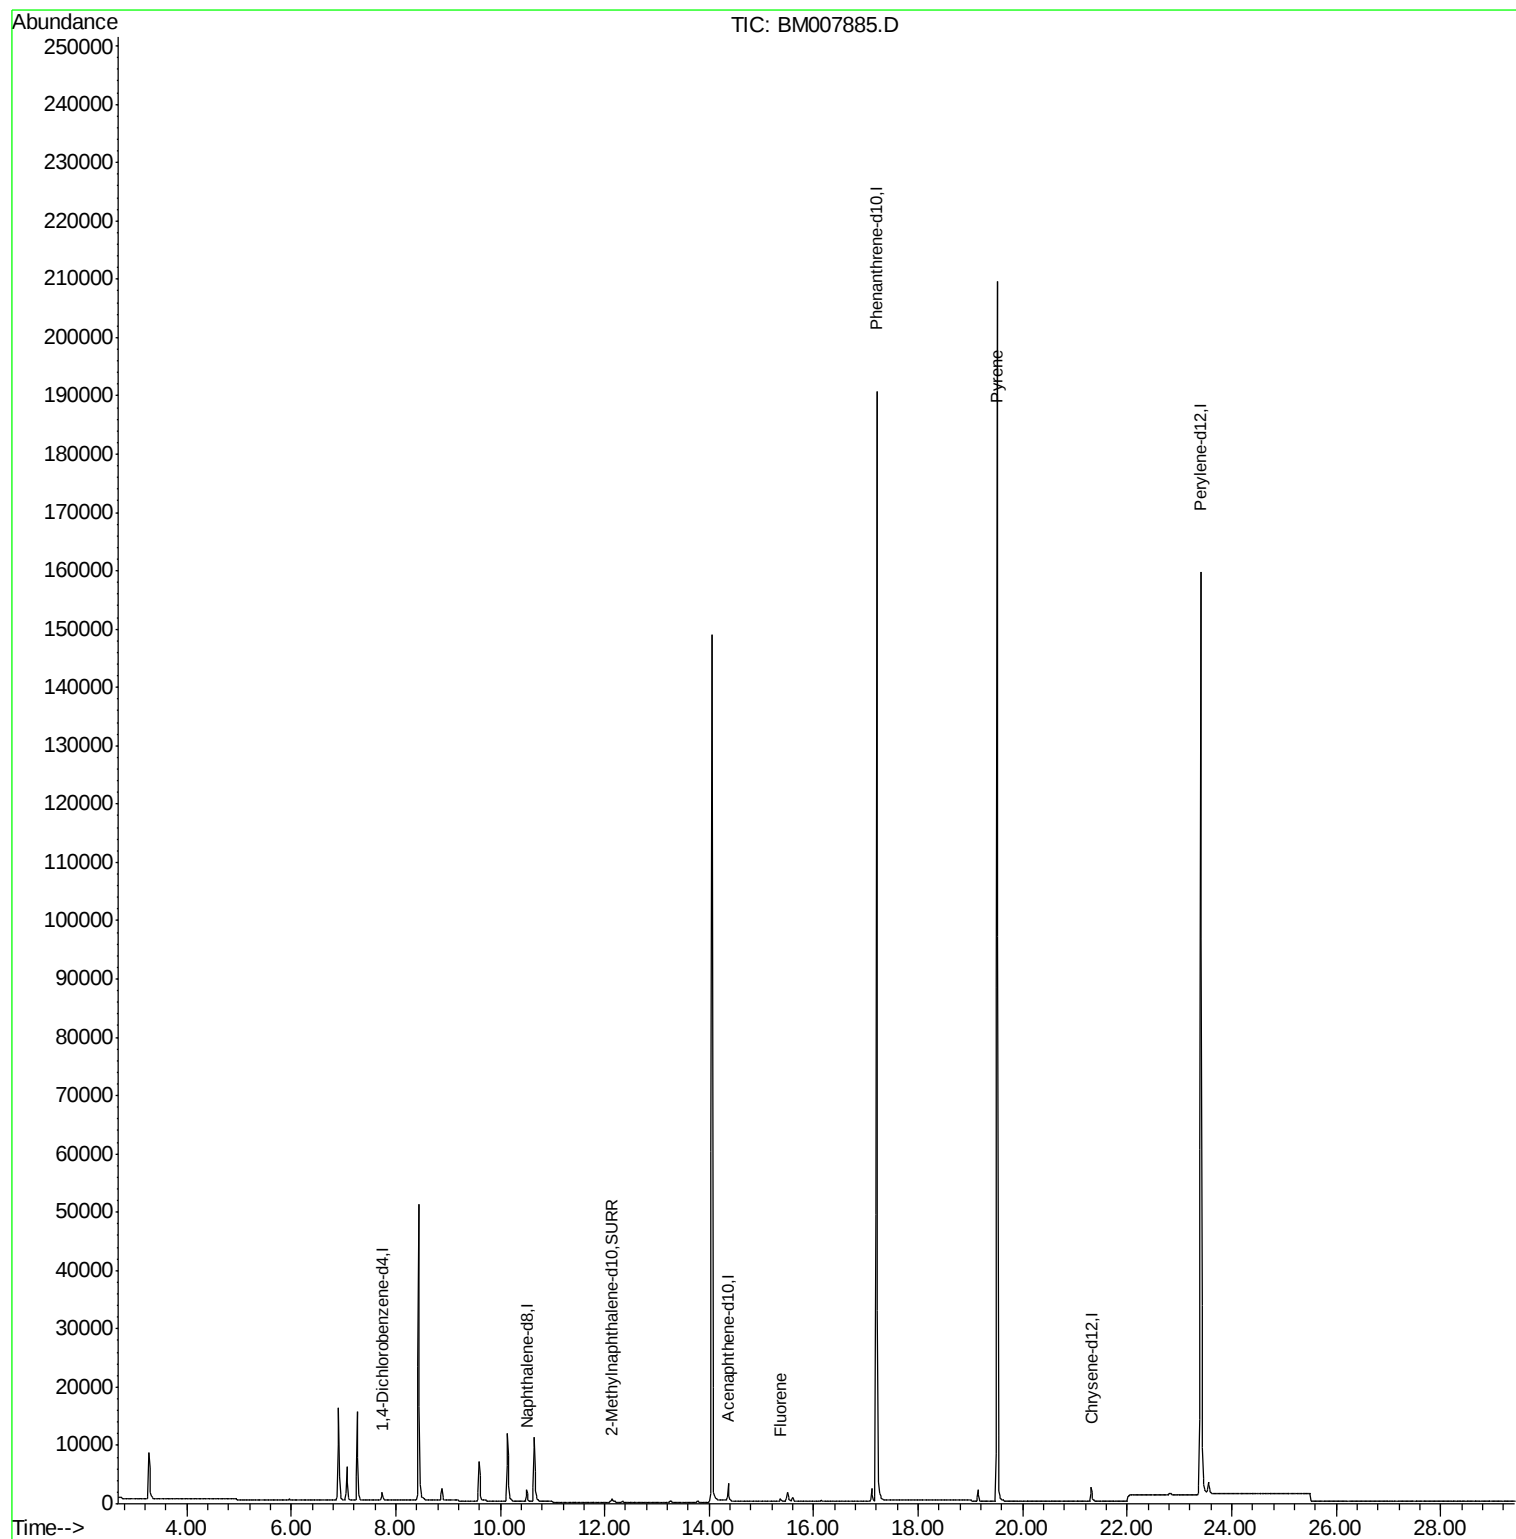

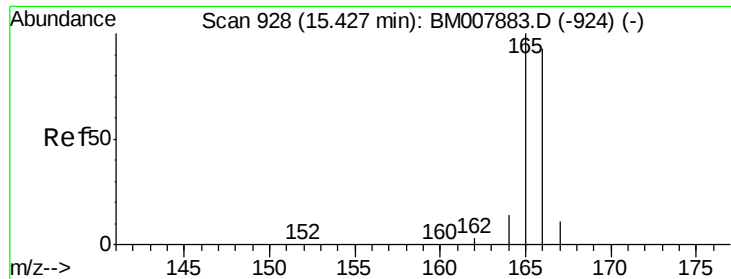

#9

Fluorene

Concen: 0.07 ng/ul

RT: 15.36 min Scan# 924

Delta R.T. -0.07 min

Lab File: BM007885.D

Acq: 15 Nov 2016 10:42

Instrument :

BNA_M

ClientSampleId :

SBLK85


Tgt Ion:166 Resp: 459

Ion Ratio Lower Upper


166 100

165 19.7 73.4 110.2#



167 35.7 14.6 22.0#

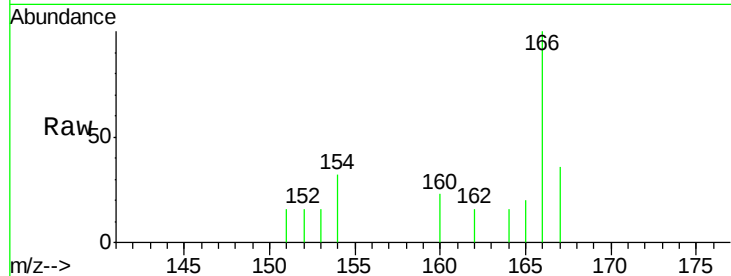

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

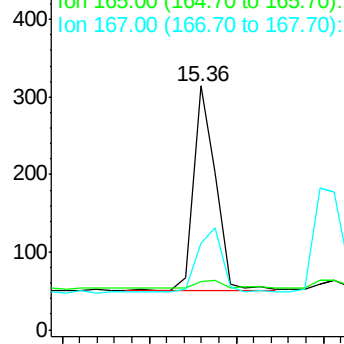

Time--> 15.20 15.30 15.40 15.50

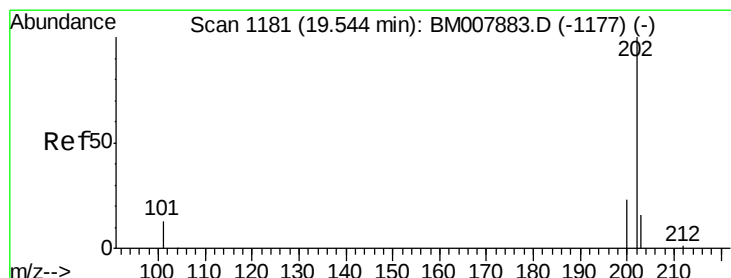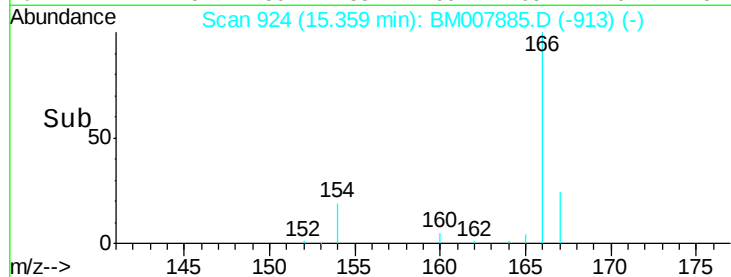

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.51 min Scan# 1178

Delta R.T. -0.03 min

Lab File: BM007885.D

Acq: 15 Nov 2016 10:42


Tgt Ion:202 Resp: 438

Ion Ratio Lower Upper


202 100

200 16.6 18.2 27.4#

203 166.9 15.6 23.4#

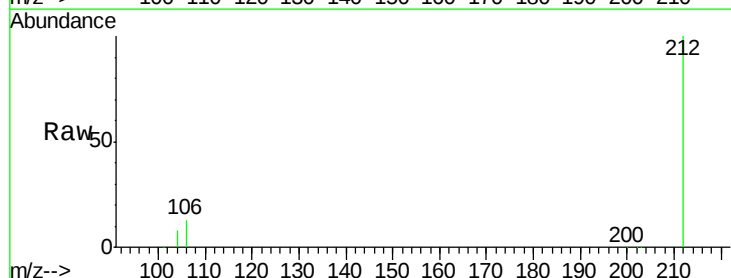

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

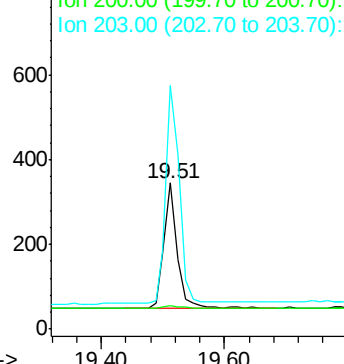

Time--> 19.40 19.60

