

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
 Data File : BM007886.D
 Acq On : 15 Nov 2016 11:18
 Operator : UM/SJ
 Sample : PB94643BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Quant Time: Nov 16 01:22:10 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 01:19:46 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	956	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	3274	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1940	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	268086	0.40	ng/ul	0.09
16) Chrysene-d12	21.32	240	3227	0.40	ng/ul	0.01
20) Perylene-d12	23.41	264	218427	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1540	0.40	ng/ul	0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.36	166	533	0.07	ng/ul#	29
17) Pyrene	19.51	202	502	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
Data File : BM007886.D
Acq On : 15 Nov 2016 11:18
Operator : UM/SJ
Sample : PB94643BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Time: Nov 16 01:22:10 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:19:46 2016
Response via : Initial Calibration




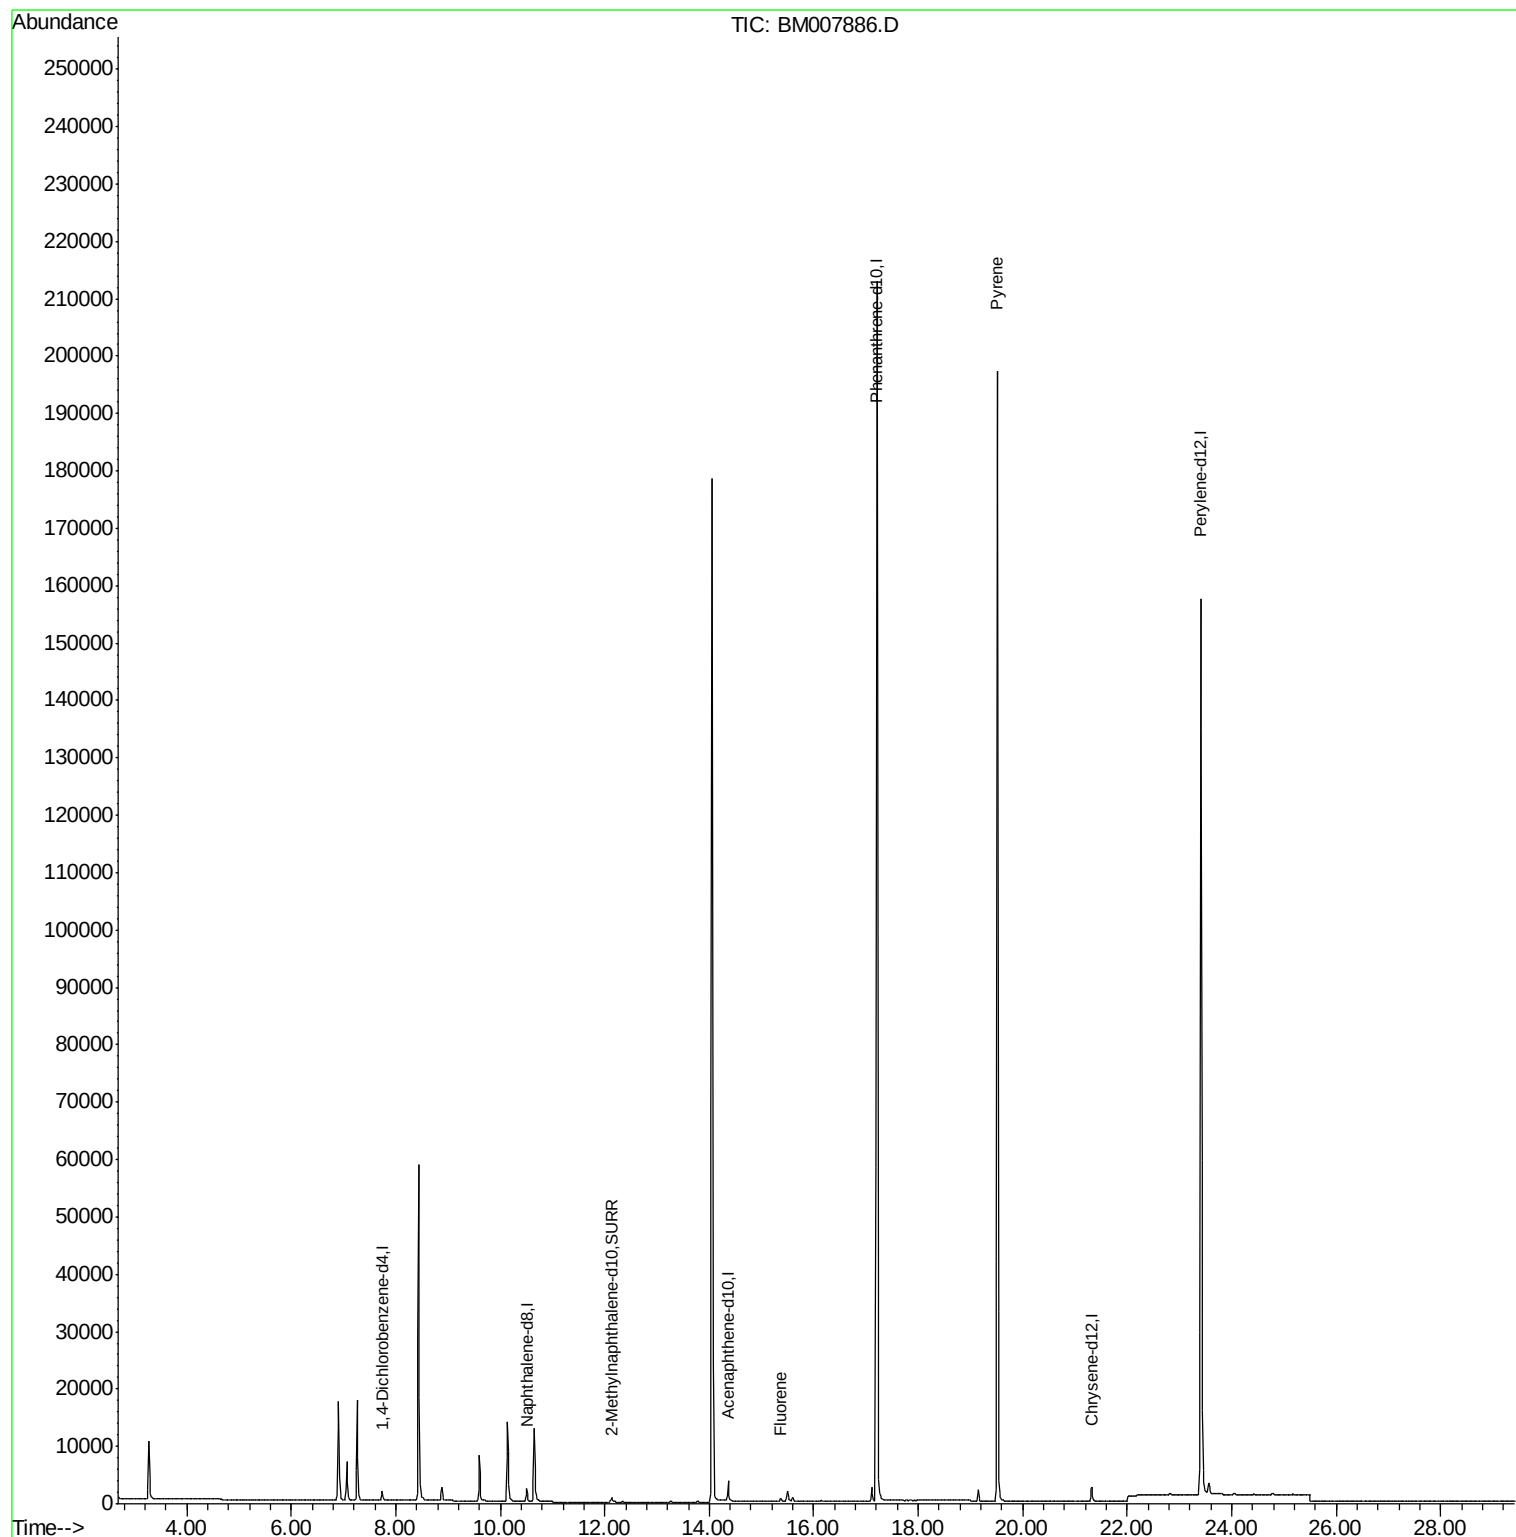


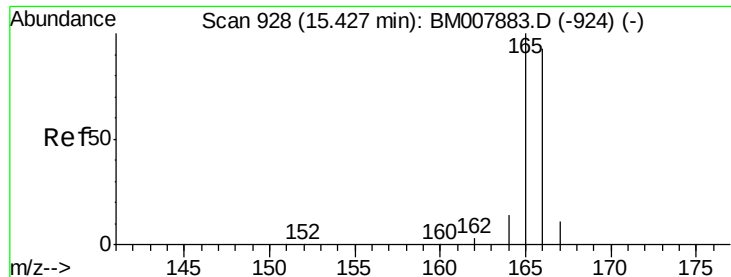

#9
Fluorene
 Concen: 0.07 ng/ul
 RT: 15.36 min Scan# 924
 Delta R.T. -0.07 min
 Lab File: BM007886.D
 Acq: 15 Nov 2016 11:18

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Tgt Ion:166 Resp: 533
 Ion Ratio Lower Upper
 166 100
 165 17.8 73.4 110.2#
 167 34.7 14.6 22.0#

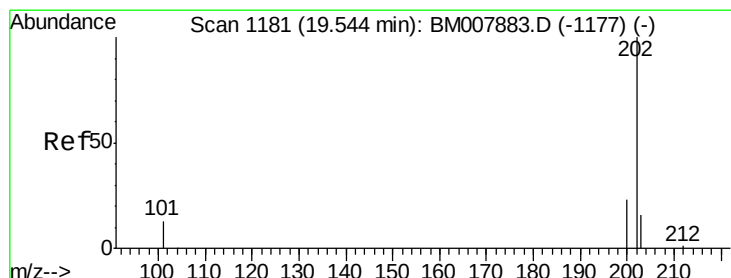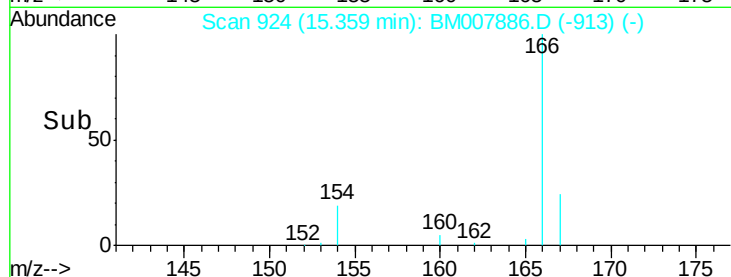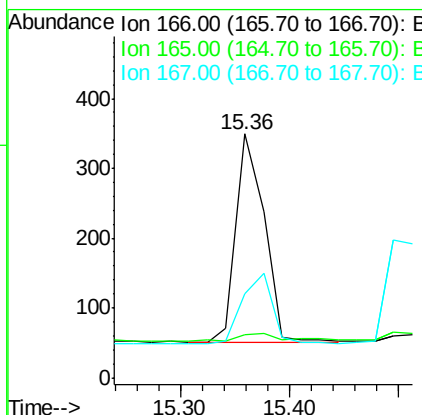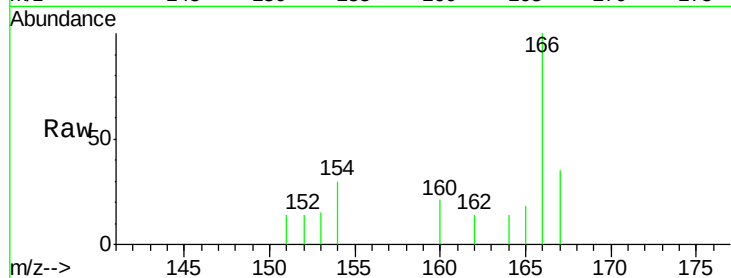

#17
Pyrene
 Concen: 0.05 ng/ul
 RT: 19.51 min Scan# 1178
 Delta R.T. -0.04 min
 Lab File: BM007886.D
 Acq: 15 Nov 2016 11:18

Tgt Ion:202 Resp: 502
 Ion Ratio Lower Upper
 202 100
 200 17.2 18.2 27.4#
 203 136.5 15.6 23.4#

