

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
 Data File : BM007897.D
 Acq On : 15 Nov 2016 17:47
 Operator : UM/SJ
 Sample : H5612-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F2H16

Quant Time: Nov 16 07:45:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 07:43:19 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	965	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	3104	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1718	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	137049	0.40	ng/ul	0.09
16) Chrysene-d12	21.31	240	3211	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	136661	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	813	0.22	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.36	166	307	0.04	ng/ul#	36
17) Pyrene	19.51	202	513	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
Data File : BM007897.D
Acq On : 15 Nov 2016 17:47
Operator : UM/SJ
Sample : H5612-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F2H16

Quant Time: Nov 16 07:45:02 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 07:43:19 2016
Response via : Initial Calibration




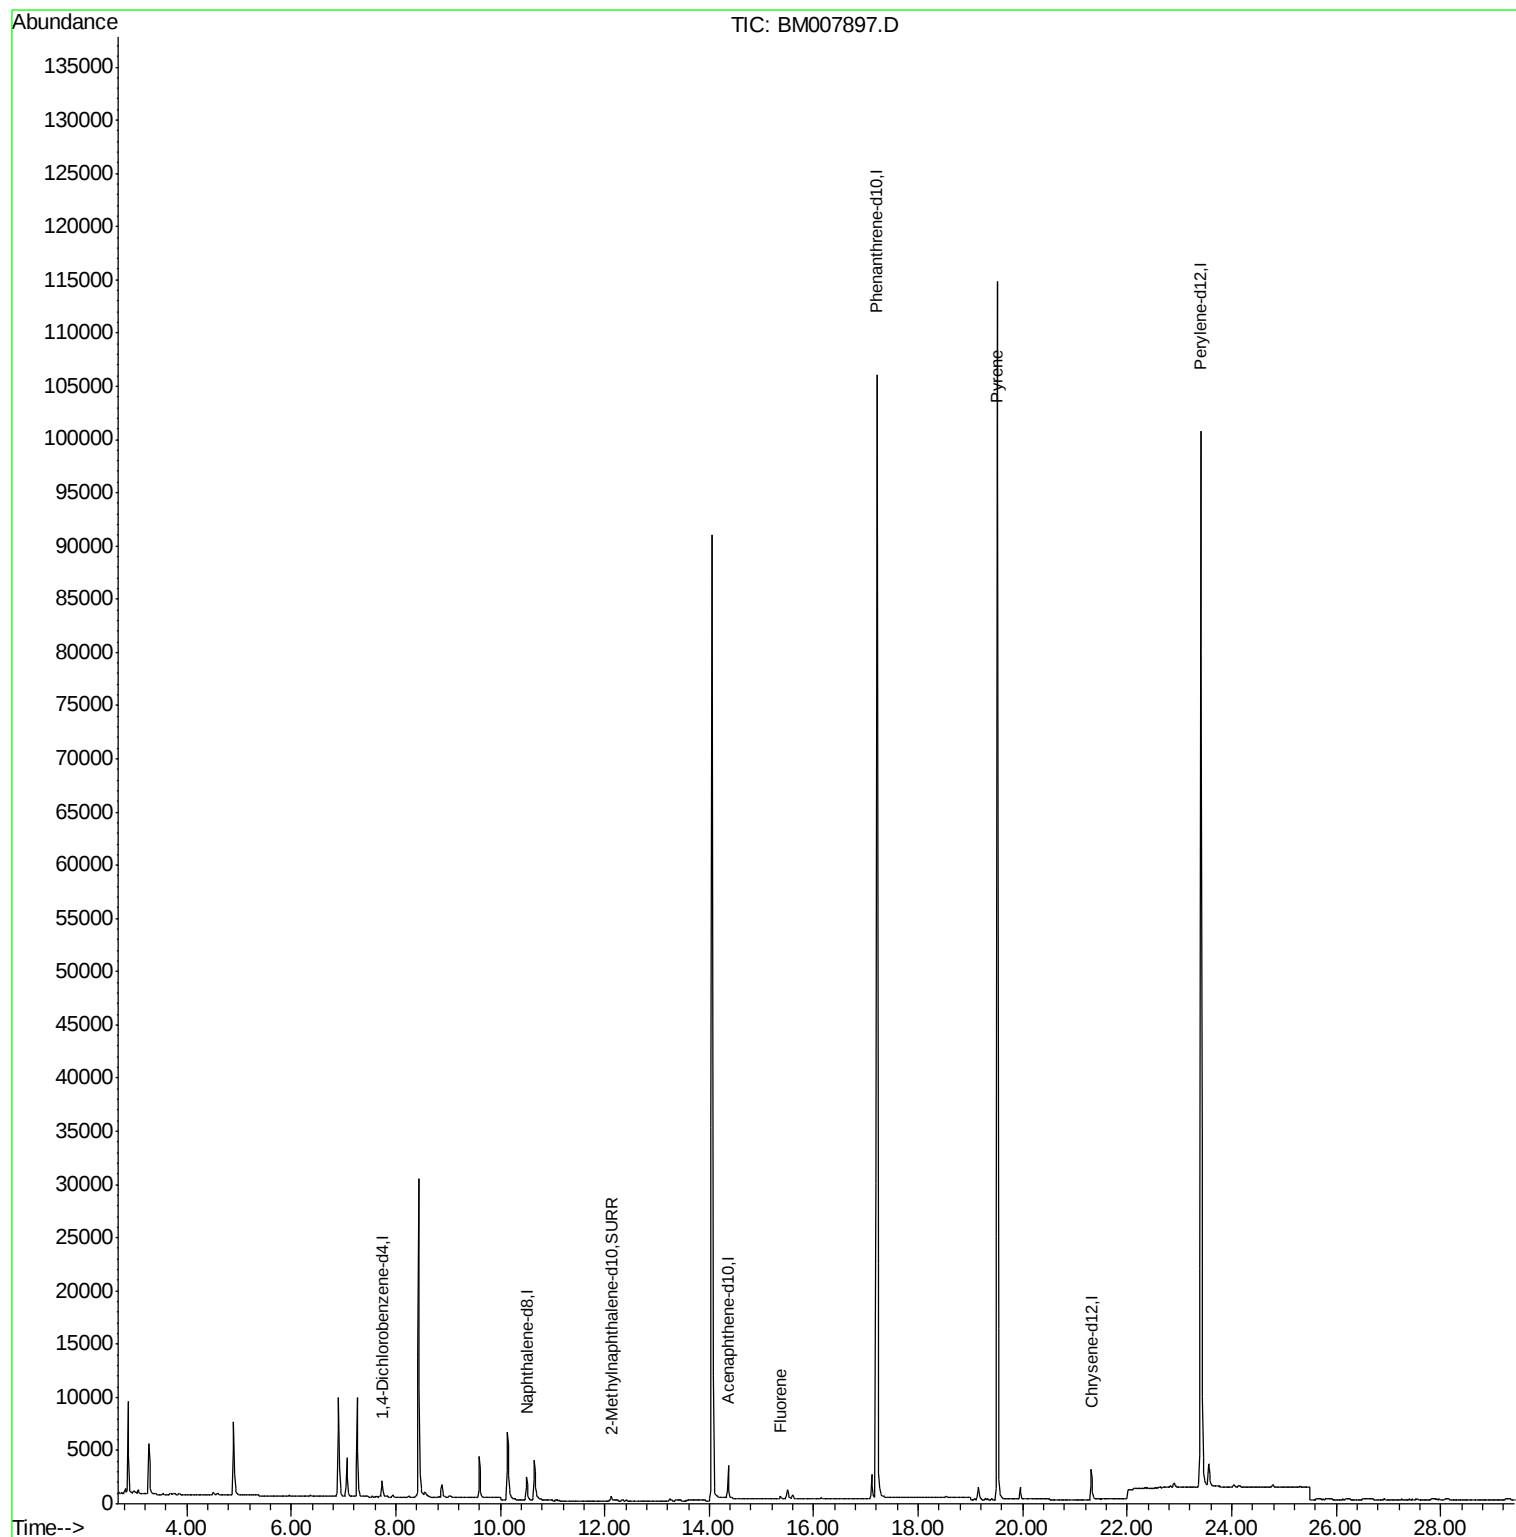


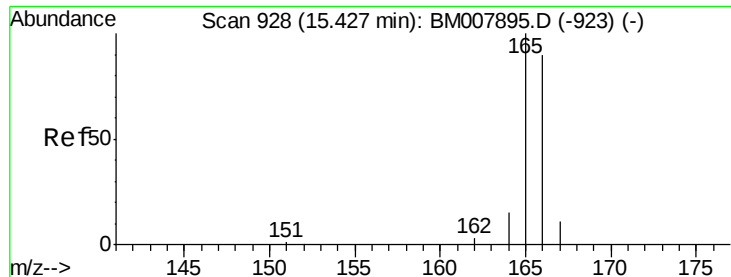

#9
Fluorene
 Concen: 0.04 ng/ul
 RT: 15.36 min Scan# 924
 Delta R.T. -0.07 min
 Lab File: BM007897.D
 Acq: 15 Nov 2016 17:47

Instrument :
 BNA_M
 ClientSampleId :
 F2H16

Tgt Ion:166 Resp: 307
 Ion Ratio Lower Upper
 166 100
 165 28.9 73.4 110.2#
 167 42.7 14.6 22.0#

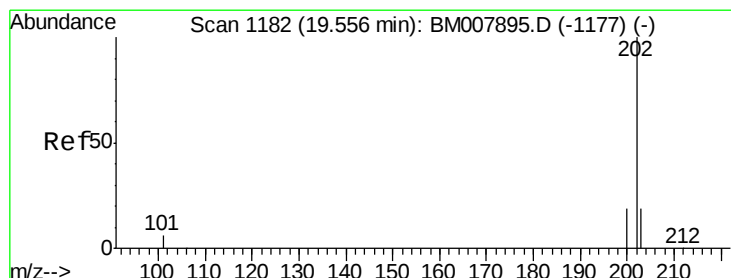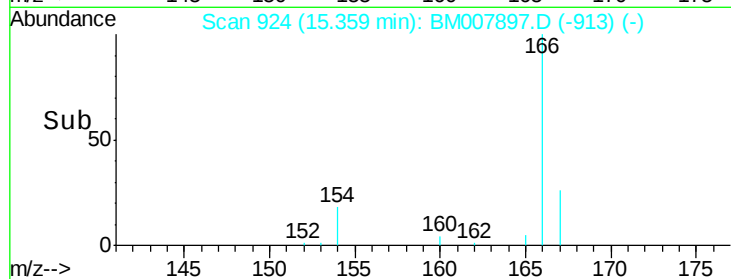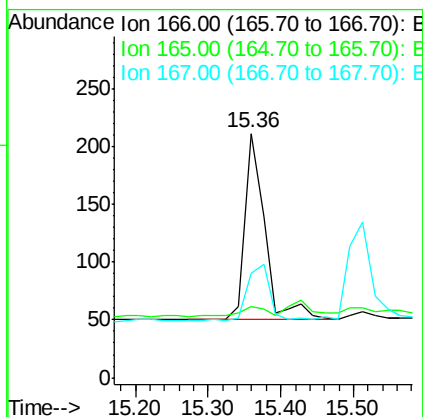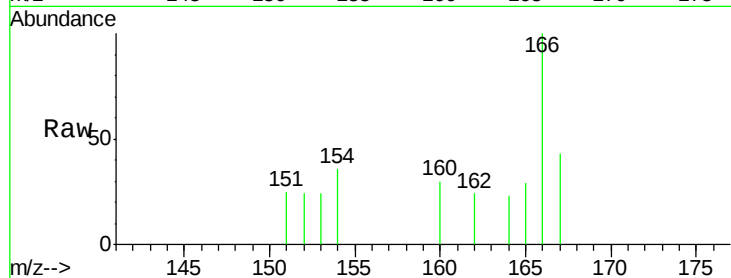

#17
Pyrene
 Concen: 0.05 ng/ul
 RT: 19.51 min Scan# 1178
 Delta R.T. -0.05 min
 Lab File: BM007897.D
 Acq: 15 Nov 2016 17:47

Tgt Ion:202 Resp: 513
 Ion Ratio Lower Upper
 202 100
 200 25.6 18.2 27.4
 203 138.6 15.6 23.4#

