

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
 Data File : BM007905.D
 Acq On : 15 Nov 2016 22:30
 Operator : UM/SJ
 Sample : H5612-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F2H11

Quant Time: Nov 16 07:45:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 07:43:19 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	862	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	2790	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1658	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	198480	0.40	ng/ul	0.09
16) Chrysene-d12	21.31	240	3302	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	204106	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	1097	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.36	166	490	0.07	ng/ul#	33
17) Pyrene	19.51	202	432	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111516\
Data File : BM007905.D
Acq On : 15 Nov 2016 22:30
Operator : UM/SJ
Sample : H5612-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F2H11

Quant Time: Nov 16 07:45:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 07:43:19 2016
Response via : Initial Calibration

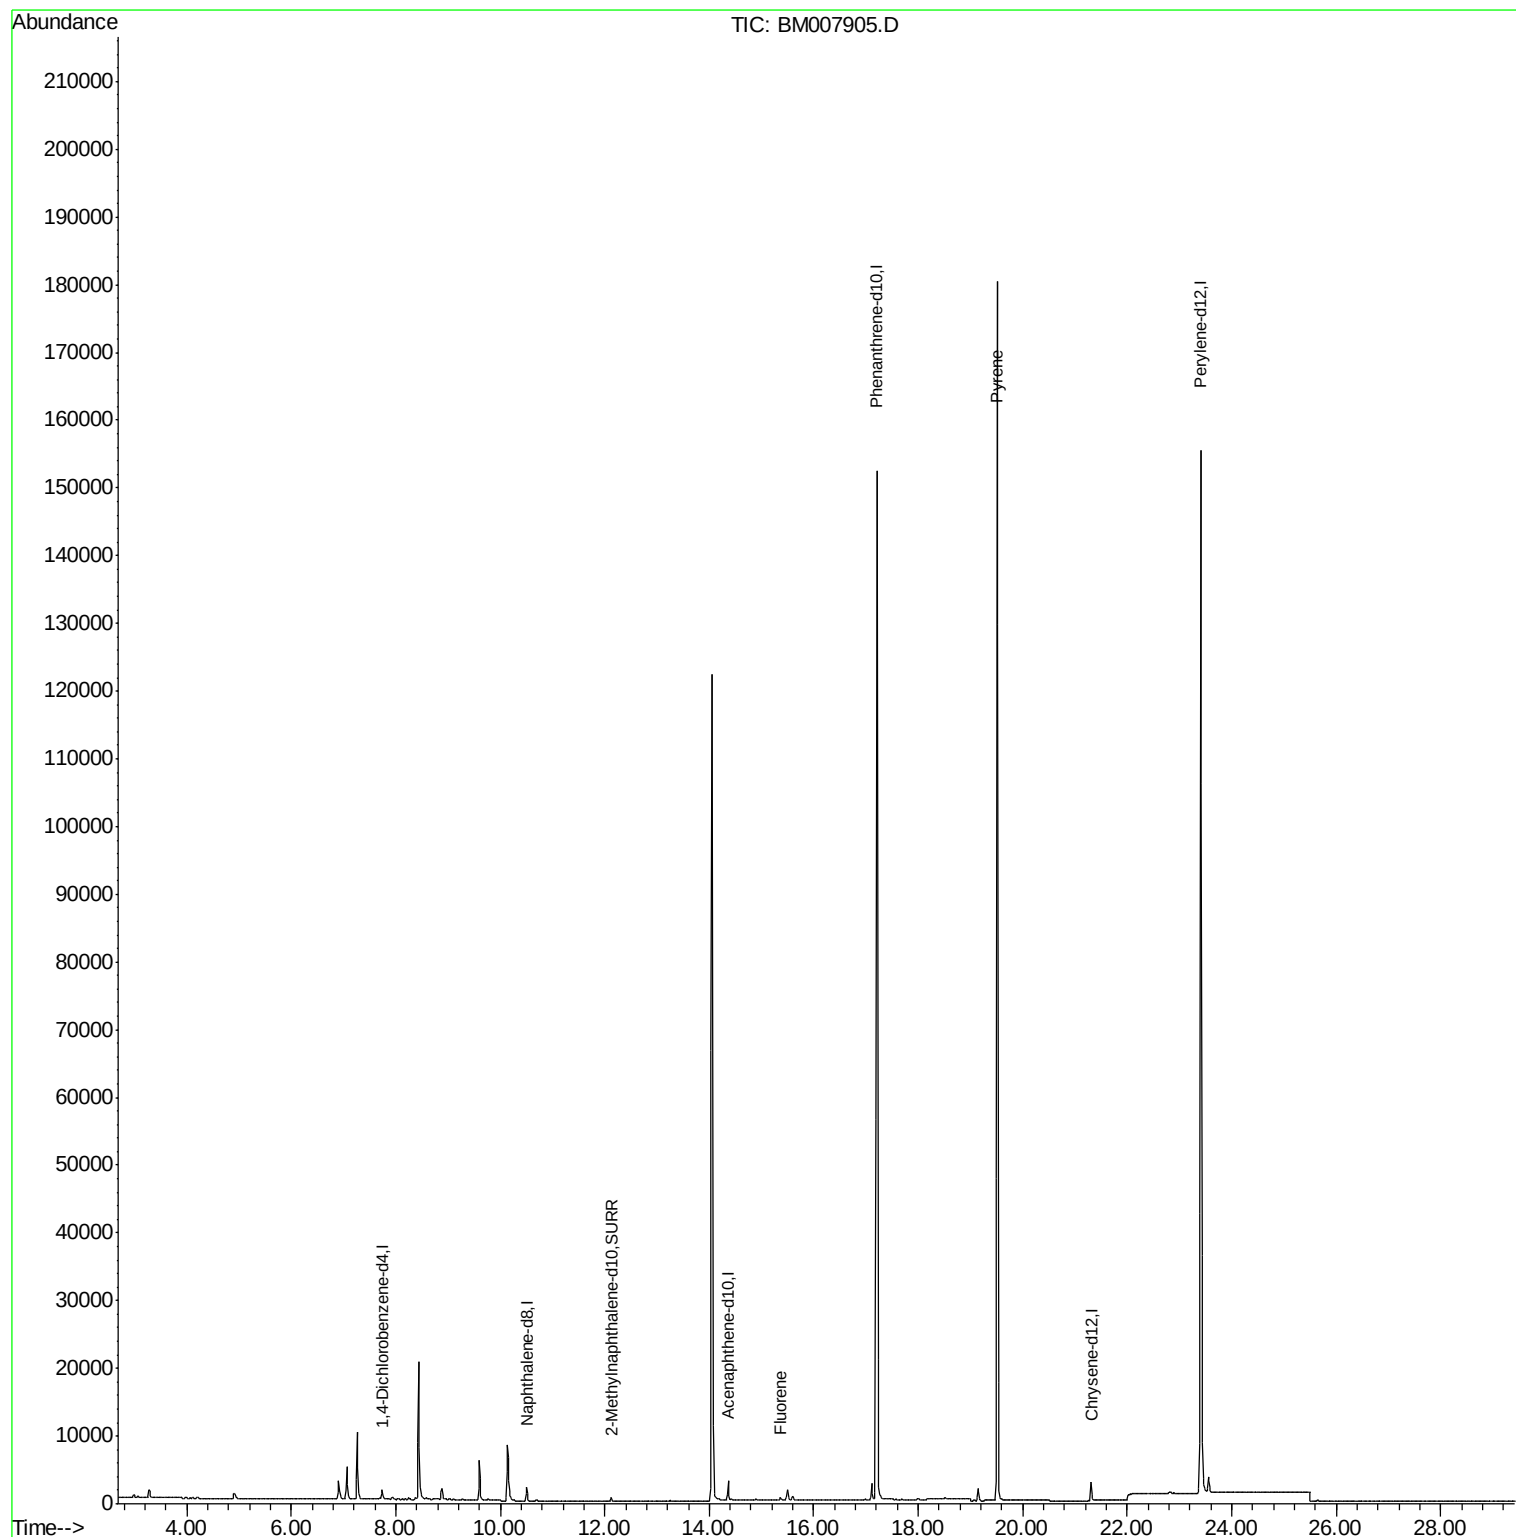

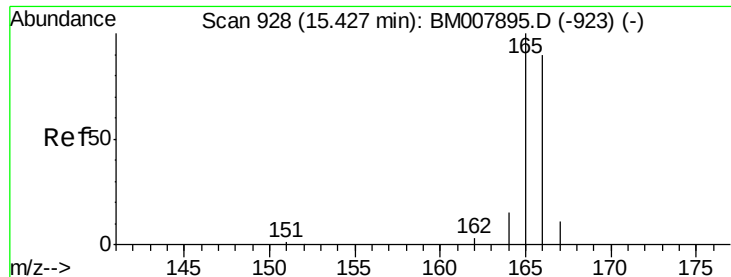

#9

Fluorene

Concen: 0.07 ng/ul

RT: 15.36 min Scan# 924

Delta R.T. -0.07 min

Lab File: BM007905.D

Acq: 15 Nov 2016 22:30

Instrument :

BNA_M

ClientSampleId :

F2H11


Tgt Ion:166 Resp: 490

Ion Ratio Lower Upper

166 100

165 23.6 73.4 110.2#

167 38.7 14.6 22.0#

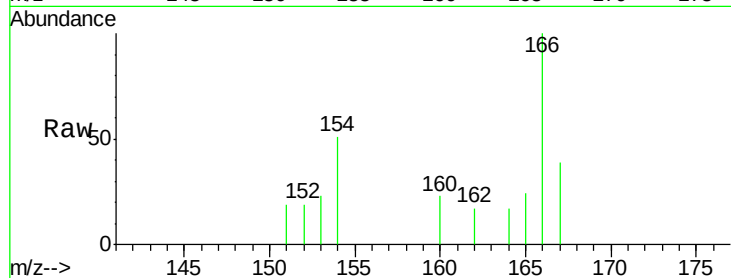

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.36

300



200

100

0

Time-->

15.20 15.40

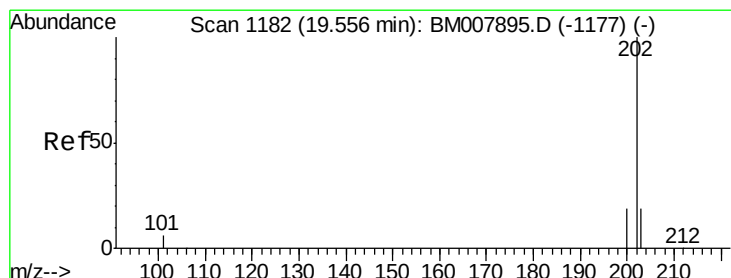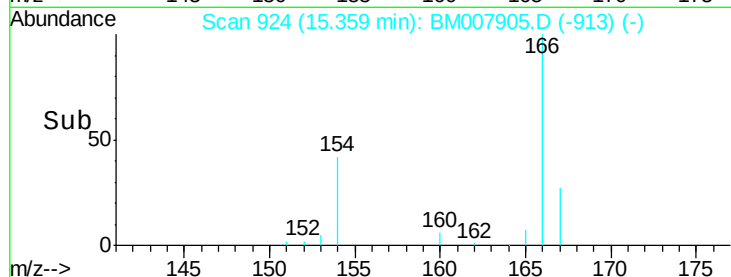

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.51 min Scan# 1178

Delta R.T. -0.05 min

Lab File: BM007905.D

Acq: 15 Nov 2016 22:30


Tgt Ion:202 Resp: 432

Ion Ratio Lower Upper

202 100

200 20.0 18.2 27.4

203 144.9 15.6 23.4#

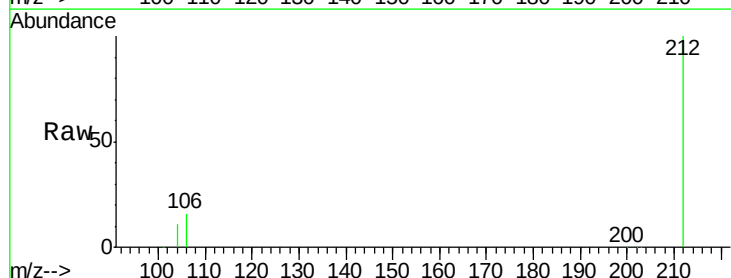

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

19.51

600

400

200

0

Time-->

19.40 19.50 19.60

