


Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
 Data File : BM007891.D
 Acq On : 15 Nov 2016 14:15
 Operator : UM/SJ
 Sample : H5626-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 16 07:31:09 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 01:19:46 2016
 Response via : Initial Calibration

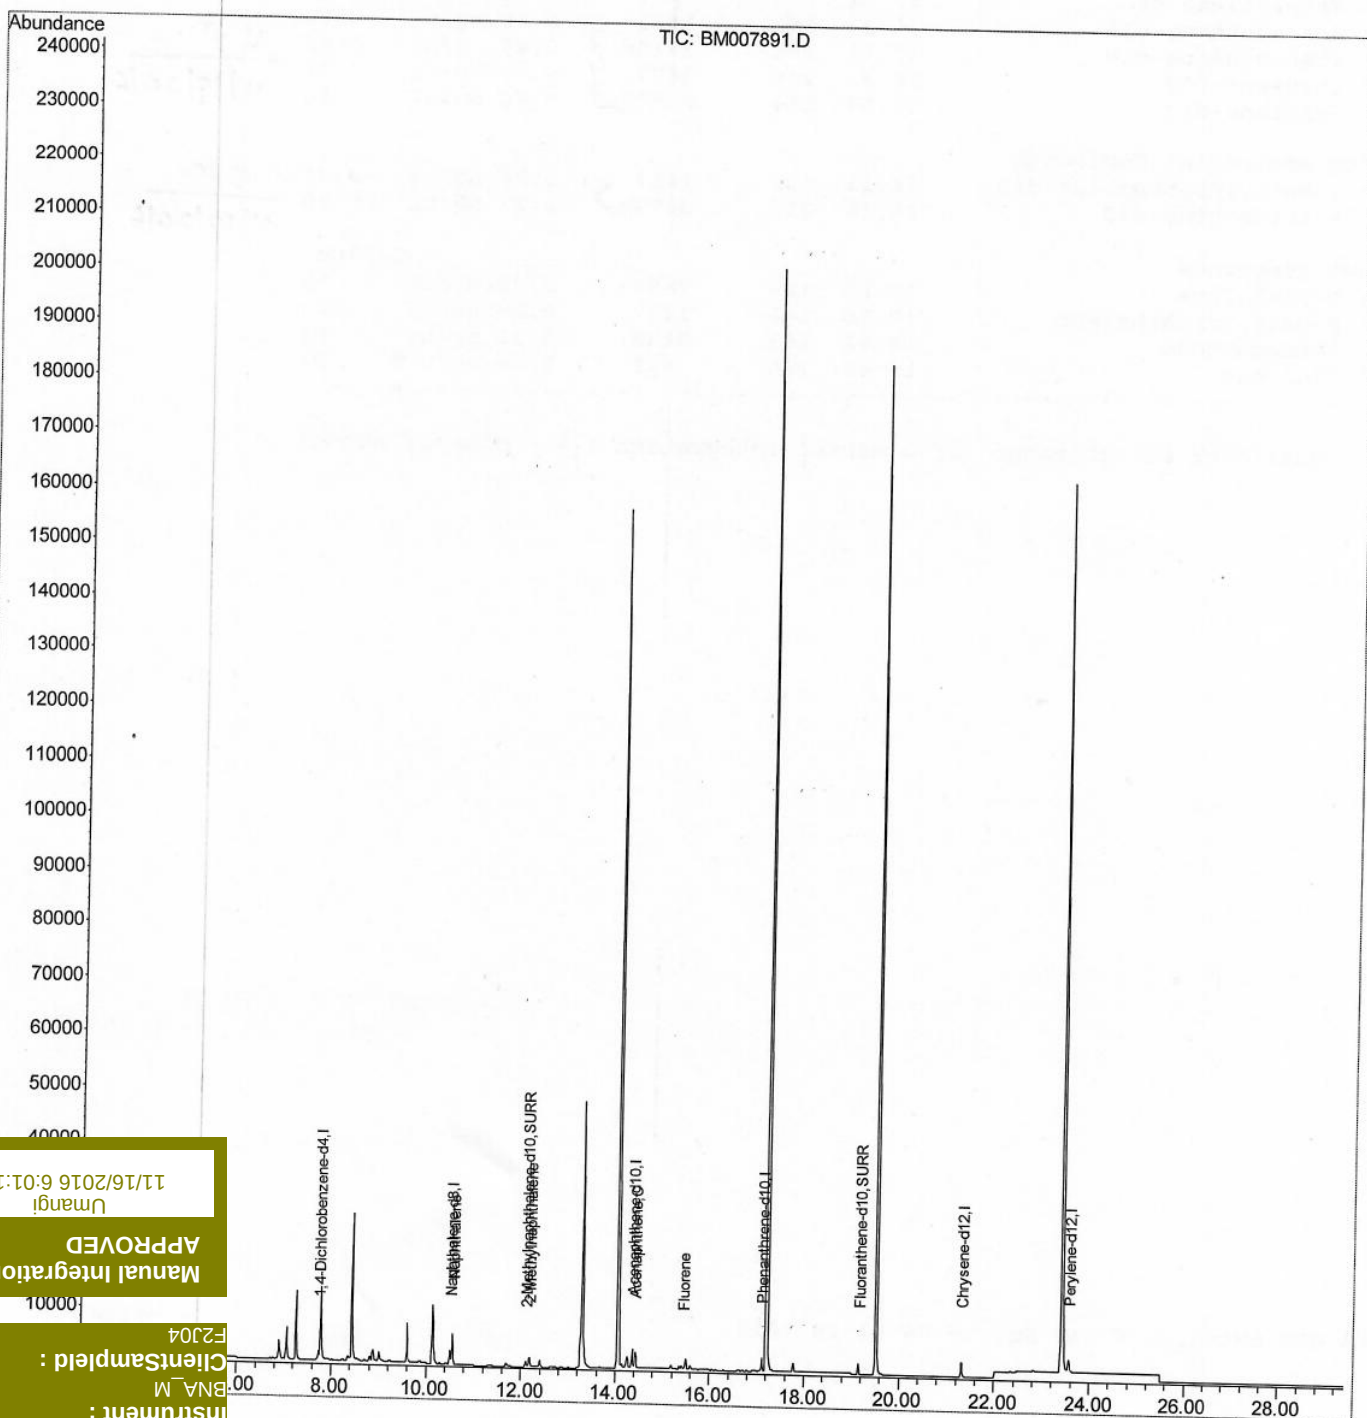

11/16/2016 6:01:17 PM
 Umani

Manual Integrations
 APPROVED


Instrument :
 Client Sample :
 F2304

SOM-EPA-SIM-BM102516.M Sat Nov 19 04:43:27 2016

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
 Data File : BM007891.D
 Acq On : 15 Nov 2016 14:15
 Operator : UM/SJ
 Sample : H5626-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 19 04:45:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration

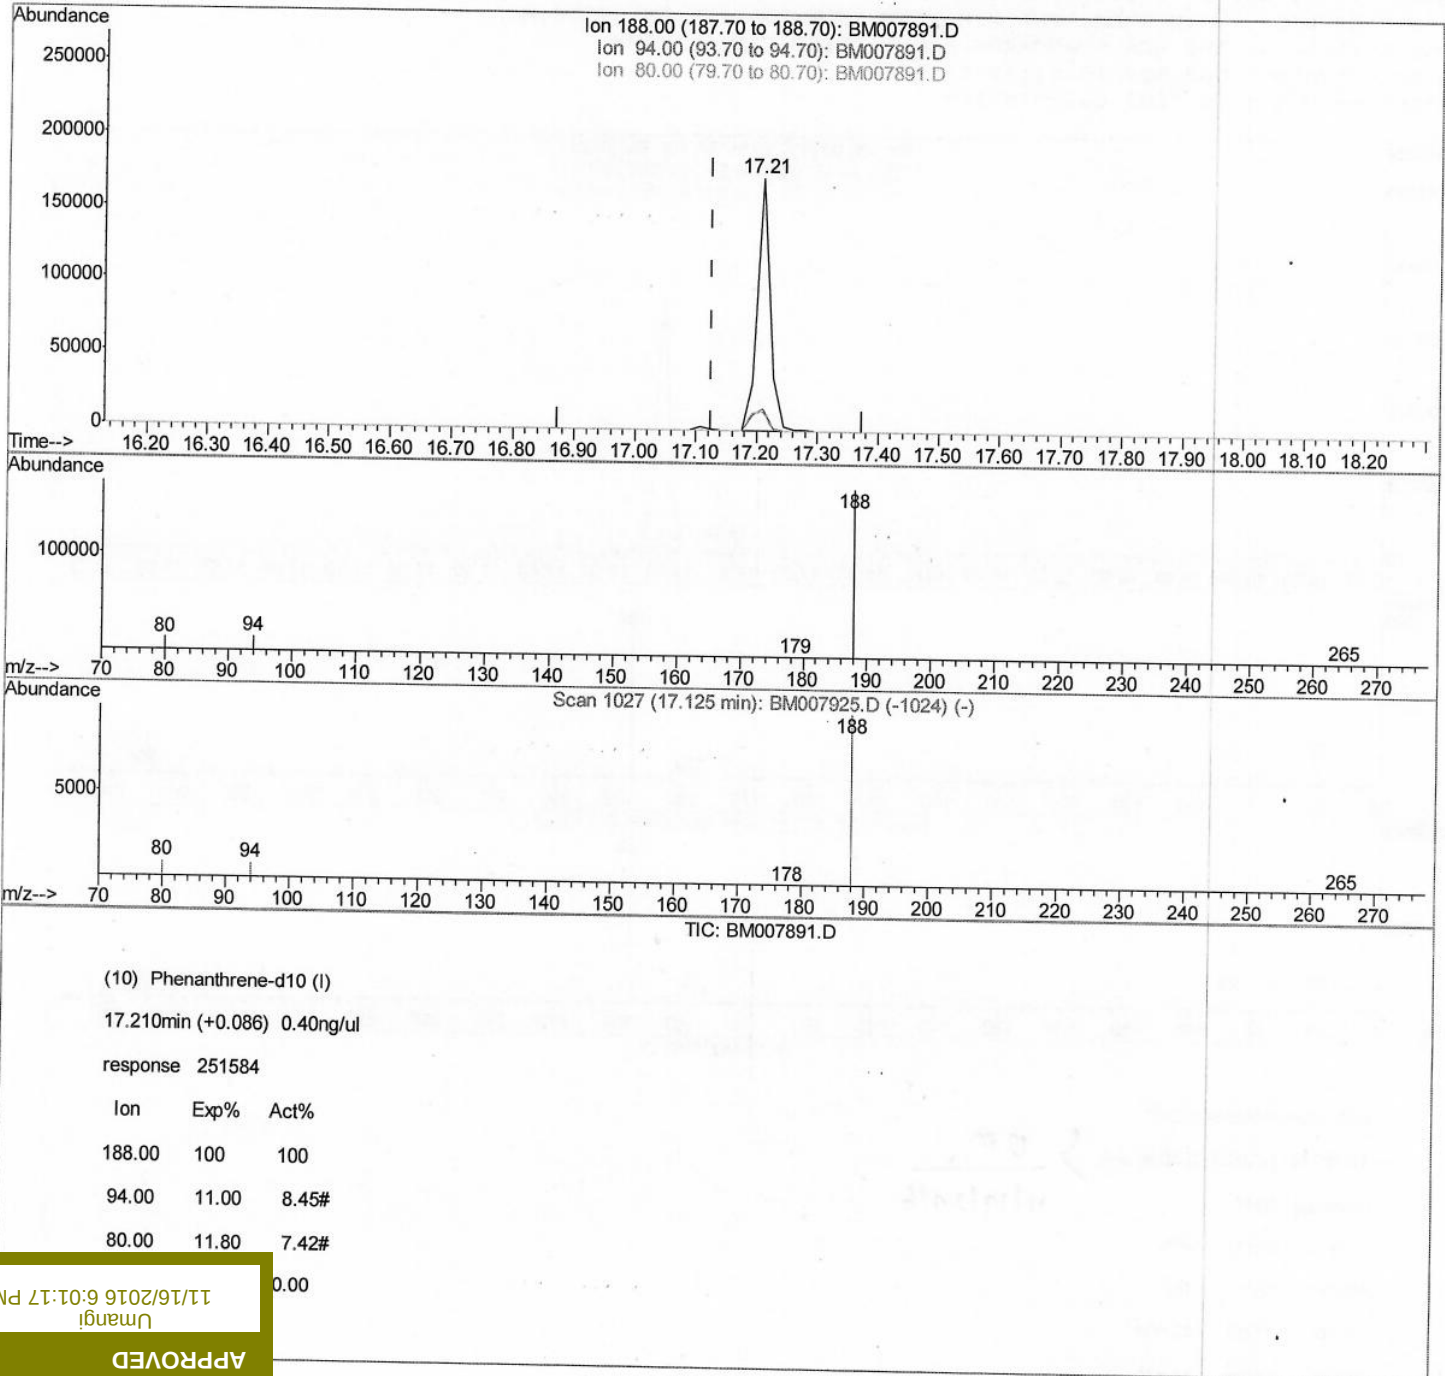




SOM-EPA-SIM-BM102516.M Sat Nov 19 04:44:18 2016

Instrument :
 BNA_M
 ClientSampled :
 F2J04

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
 Data File : BM007891.D
 Acq On : 15 Nov 2016 14:15
 Operator : UM/SJ
 Sample : H5626-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 19 04:45:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration

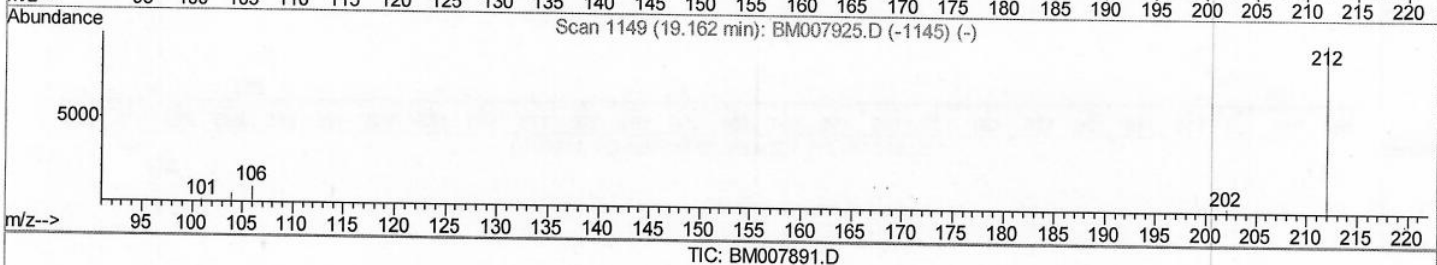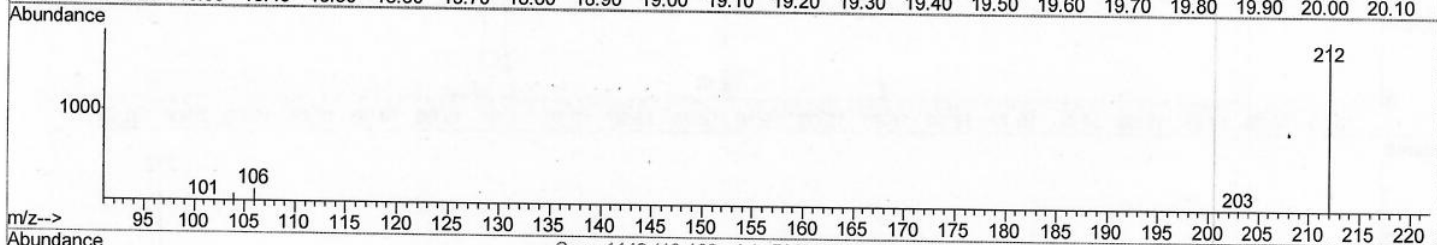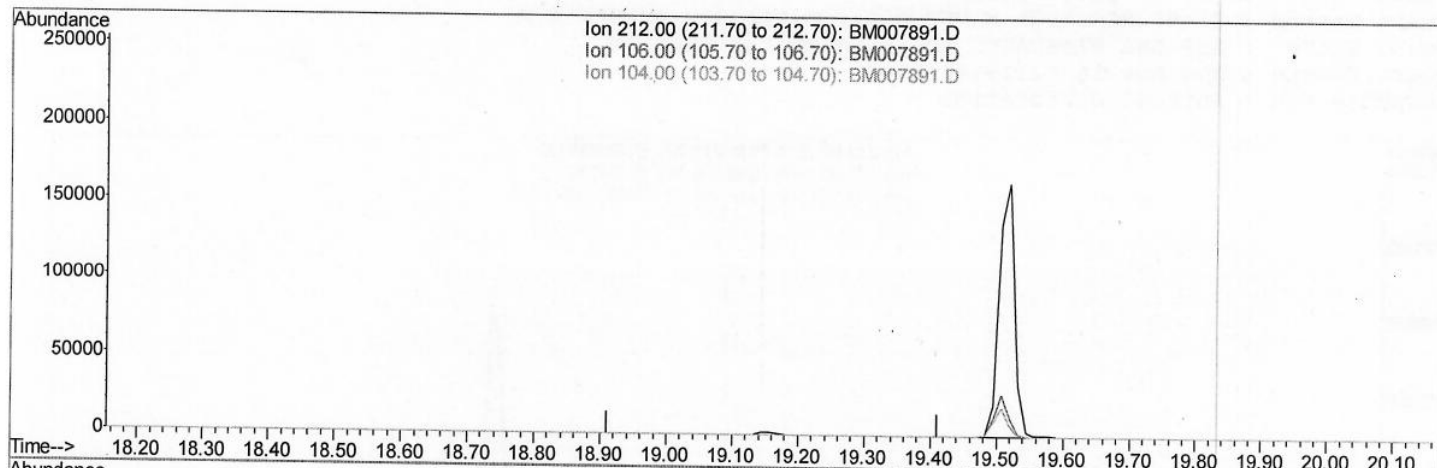

(14) Fluoranthene-d10 (SURR)

19.162min (-19.162) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
		0.00

11/16/2016 6:01:17 PM
 Umani

APPROVED
 Manual Integrations




SOM-EPA-SIM-BM102516.M Sat Nov 19 04:44:23 2016

Instrument : BNA_M
 Client: Sampled : F2J04

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
 Data File : BM007891.D
 Acq On : 15 Nov 2016 14:15
 Operator : UM/SJ
 Sample : H5626-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 19 04:45:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration

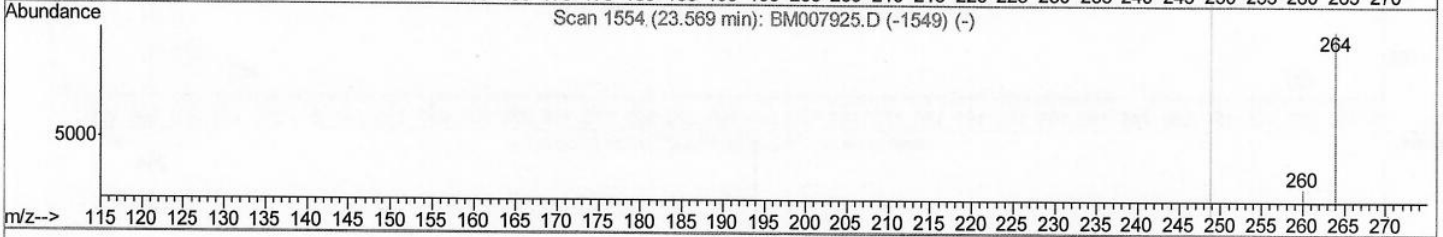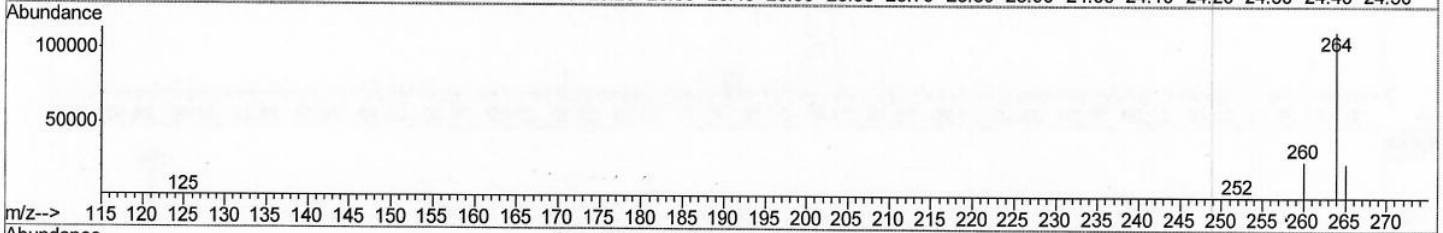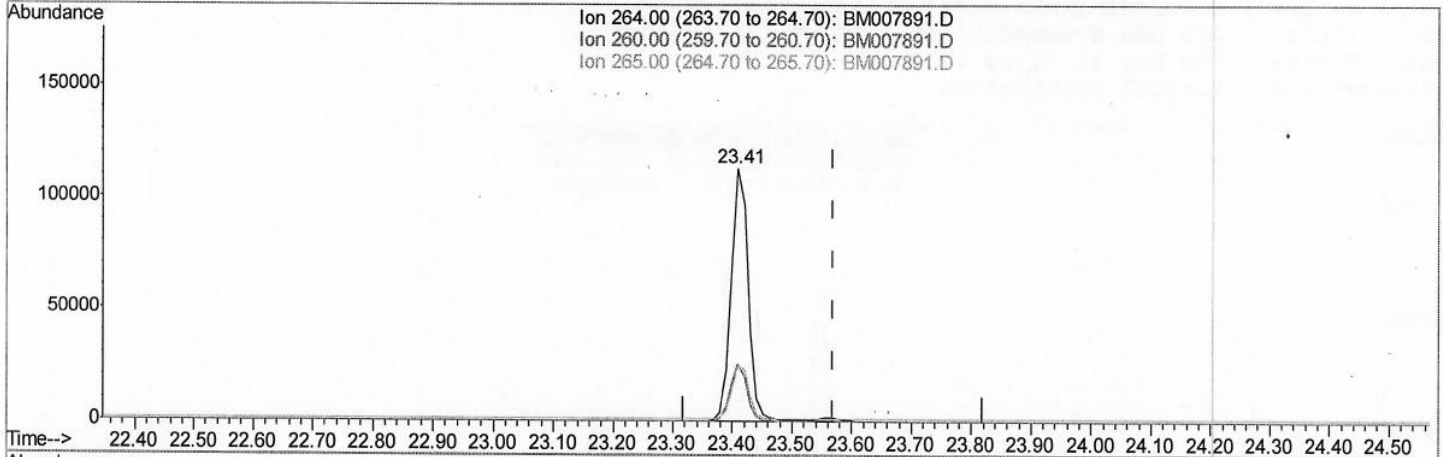

TIC: BM007891.D

(20) Perylene-d12 (I)
 23.410min (-0.160) 0.40ng/ul
 response 225909

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.33#
265.00	103.50	21.16#
		0.00

11/16/2016 6:01:17 PM

Umanji

APPROVED
 Manual Integrations


SOM-EPA-SIM-BM102516.M Sat Nov 19 04:44:27 2016

Instrument :
 BNA_M
 ClientSampled :
 F2J04

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
 Data File : BM007891.D
 Acq On : 15 Nov 2016 14:15
 Operator : UM/SJ
 Sample : H5626-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 16 07:31:09 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 01:19:46 2016
 Response via : Initial Calibration

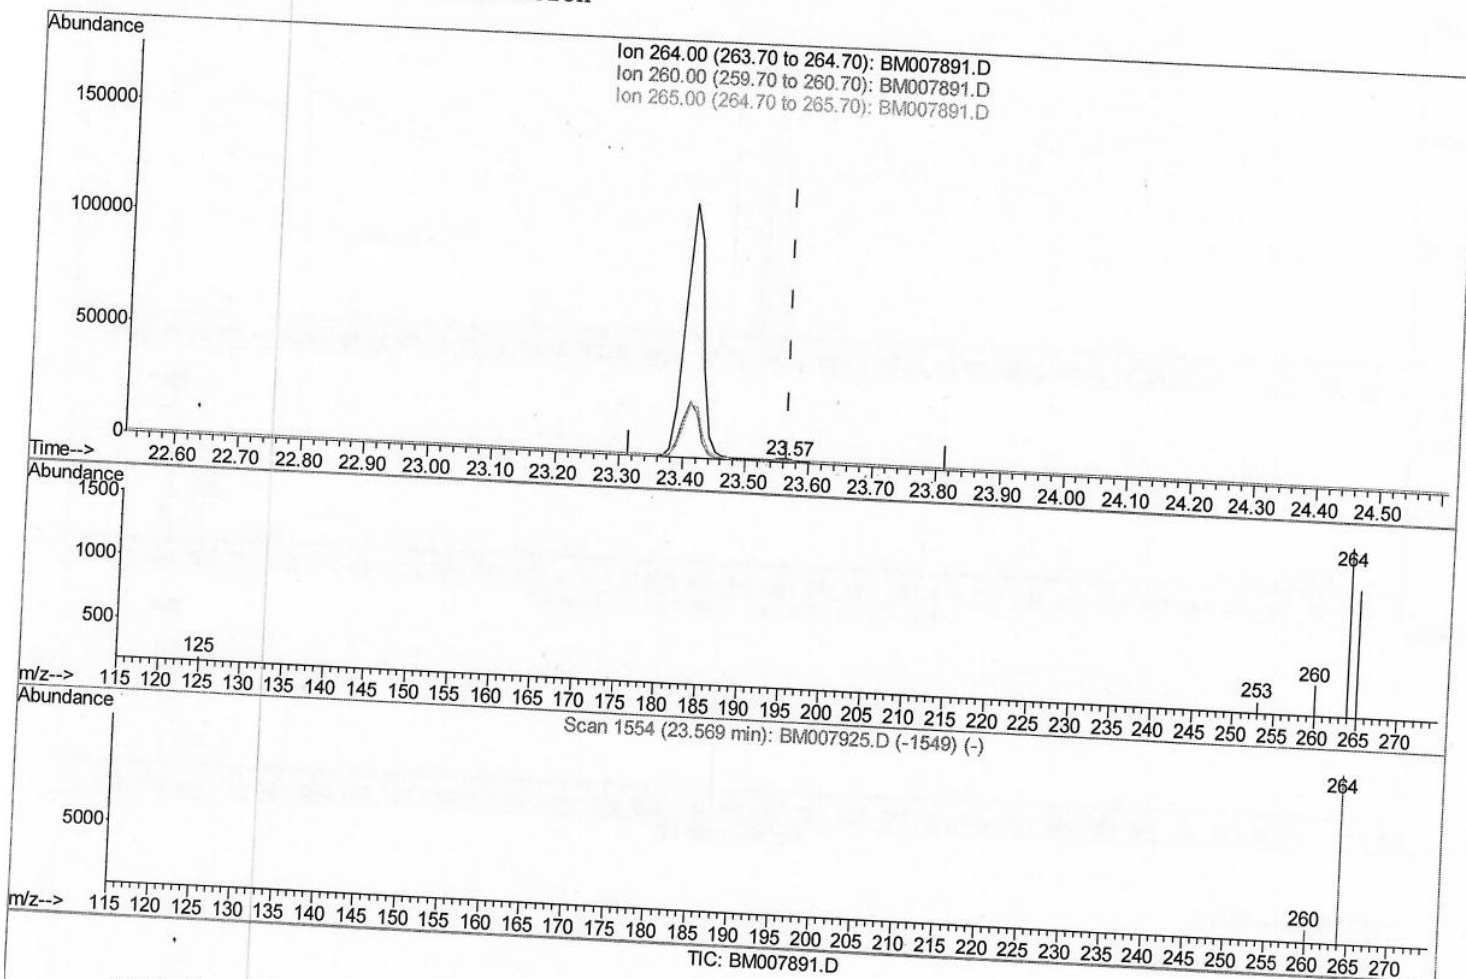

(20) Perylene-d12 (I)

23.566min (0.000) 0.40ng/ul m

response 2599

Ion Exp% Act%

264.00 100 64.07#

11/16/2016 6:01:17 PM
 Umani

APPROVED
 Manual Integrations


F2304
 ClientSampled :
 BNA_M
 Instrument :

Sat Nov 19 04:43:19 2016

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
 Data File : BM007891.D
 Acq On : 15 Nov 2016 14:15
 Operator : UM/SJ
 Sample : H5626-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 16 07:31:09 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 01:19:46 2016
 Response via : Initial Calibration

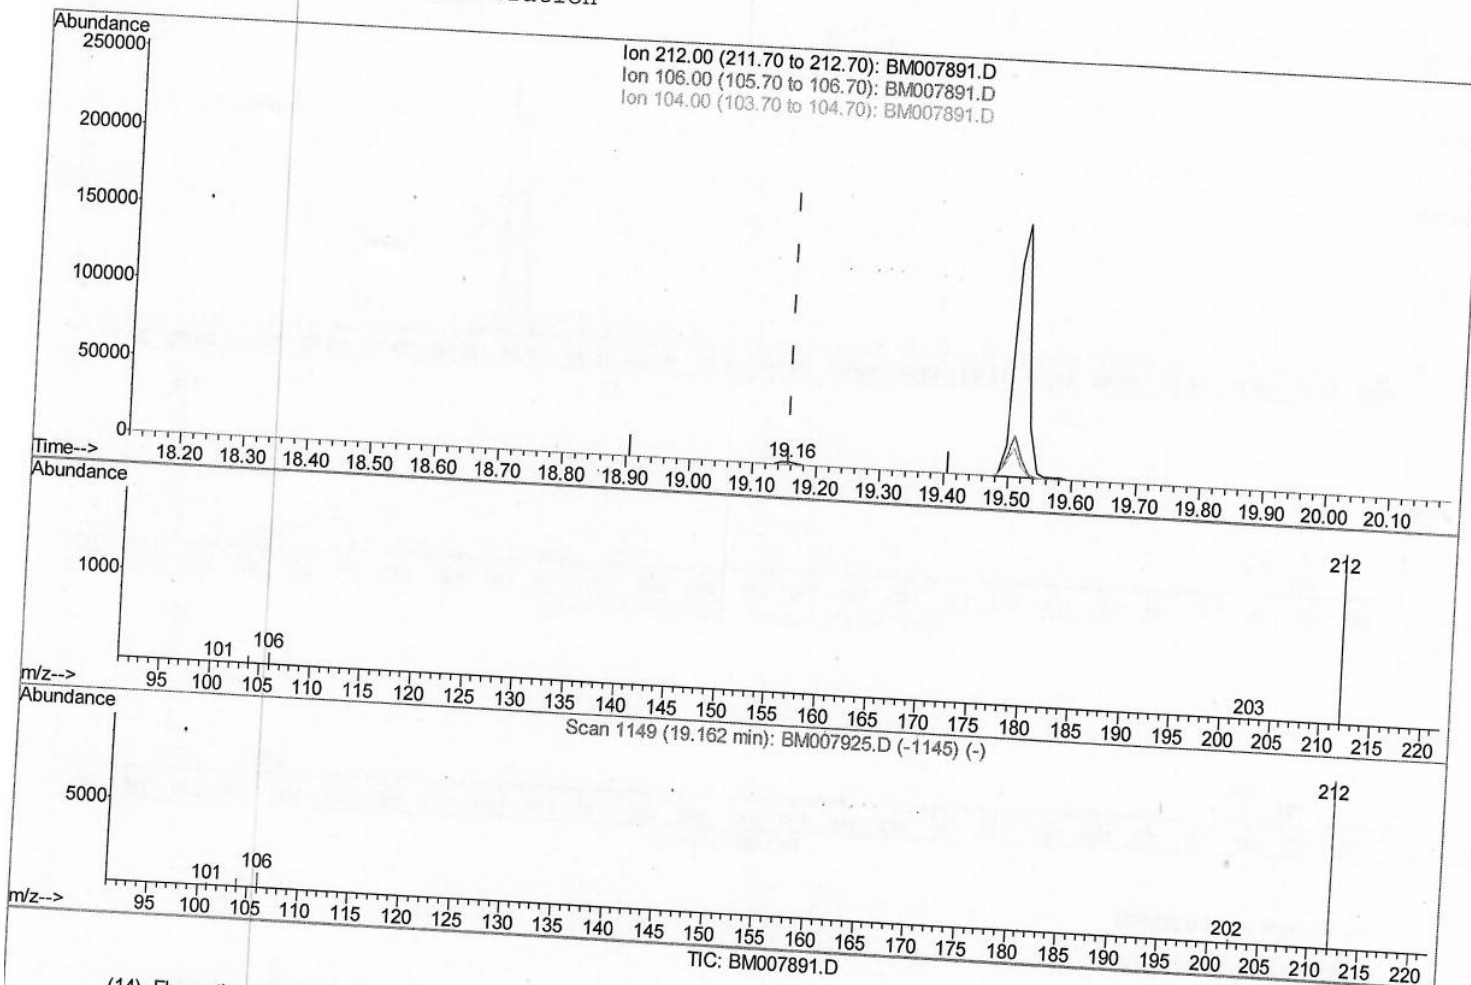

(14) Fluoranthene-d10 (SURR)

19.157min (0.000) 0.37ng/ul m

response 2879

Ion	Exp%	Act%
212.00	100	100

11/16/2016 6:01:17 PM
 Umangi

APPROVED
 Manual Integrations


Client: Sampled :
 BNA_M
 Instrument :
 F2304

Sat Nov 19 04:43:13 2016

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
 Data File : BM007891.D
 Acq On : 15 Nov 2016 14:15
 Operator : UM/SJ
 Sample : H5626-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 16 07:31:09 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 01:19:46 2016
 Response via : Initial Calibration

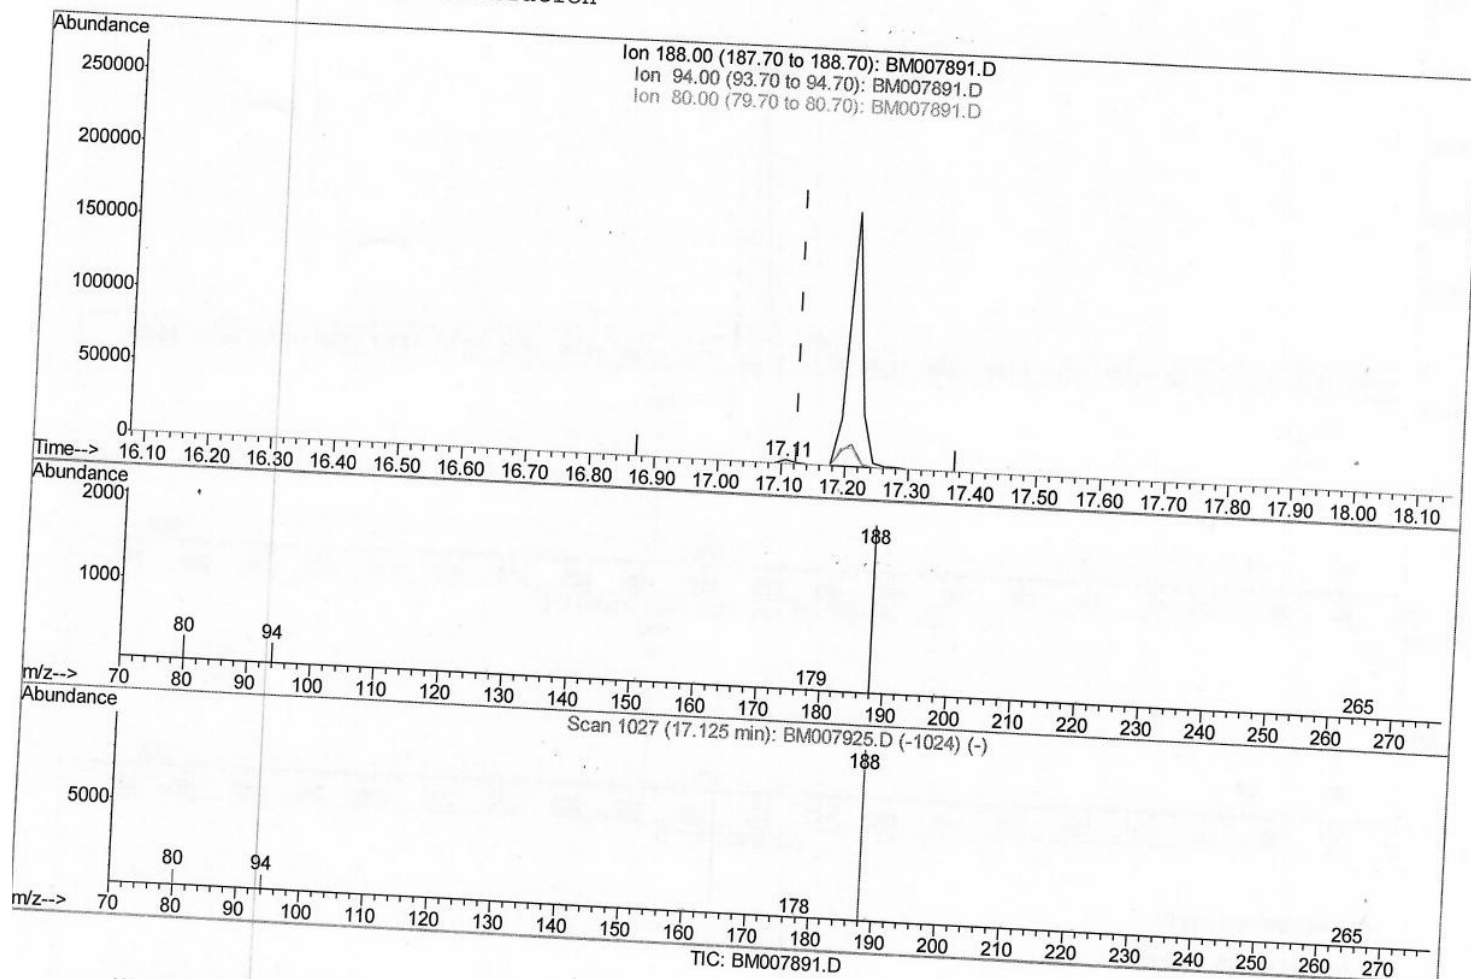

(10) Phenanthrene-d10 (I)

17.107min (-0.017) 0.40ng/ul m

response 3415

Ion Exp% Act%

188.00 100

0.10
 11/19/2016

11/16/2016 6:01:17 PM

Manual Integrations
 APPROVED

ClientSampled :
 BNA_M

Instrument :

Sat Nov 19 04:43:01 2016

Data Path : Z:\HPCHEM1\BNA_M\Data\BM111516\
Data File : BM007891.D
Acq On : 15 Nov 2016 14:15
Operator : UM/SJ
Sample : H5626-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 16 07:31:09 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:19:46 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	1009	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	3313	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1920	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	3415m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.32	240	3477	0.40	ng/ul	0.01
20) Perylene-d12	23.57	264	2599m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	1411	0.36	ng/ul	-0.01
14) Fluoranthene-d10	19.16	212	2879m	0.37	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.56	128	7859	0.92	ng/ul	95
5) 2-Methylnaphthalene	12.18	142	1357	0.25	ng/ul	100
8) Acenaphthene	14.42	153	2136	0.31	ng/ul	90
9) Fluorene	15.43	166	488	0.06	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M.
11/19/2016

U.M.
11/19/2016

11/16/2016 6:01:17 PM
Umani

APPROVED
Manual Integrations

BM102516.M Sat Nov 19 04:43:26 2016

Instrument :
BNA_M
ClientSampled :
F2304