


Data Path : Z:\HPCHEM1\BNA M\DATA\BM111615\
Data File : BM003135.D
Acq On : 16 Nov 2015 09:22
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 17 04:41:30 2015

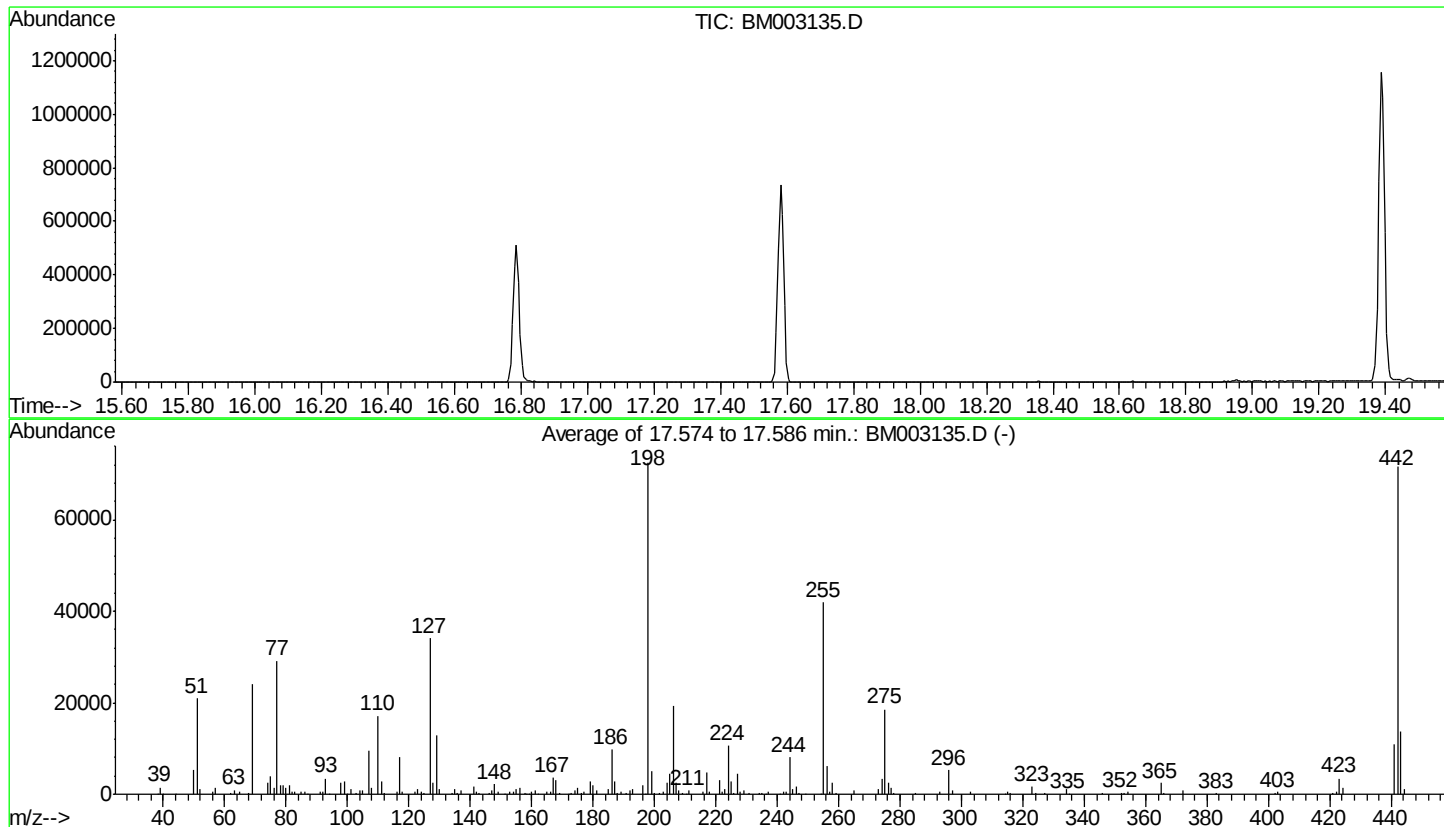

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	20928	PASS
68	69	0.00	2	1.8	425	PASS
69	198	0.00	100	33.1	23970	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	34029	PASS
197	198	0.00	2	0.2	121	PASS
198	198	100	100	100.0	72458	PASS
199	198	5	9	6.8	4937	PASS
275	198	10	60	25.6	18559	PASS
365	198	1	100	3.4	2477	PASS
441	442	0.01	24	15.3	10978	PASS
442	198	50	100	98.9	71634	PASS
443	442	15	24	19.2	13733	PASS