

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007913.D
 Acq On : 16 Nov 2016 10:24
 Operator : UM/SJ
 Sample : PB94742BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK42

Quant Time: Nov 16 16:20:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:16:41 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	782	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	2513	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1442	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	201062	0.40	ng/ul	0.09
16) Chrysene-d12	21.32	240	2579	0.40	ng/ul	0.01
20) Perylene-d12	23.41	264	194760	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1148	0.39	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.51	202	371	0.04	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007913.D
Acq On : 16 Nov 2016 10:24
Operator : UM/SJ
Sample : PB94742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK42

Quant Time: Nov 16 16:20:03 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

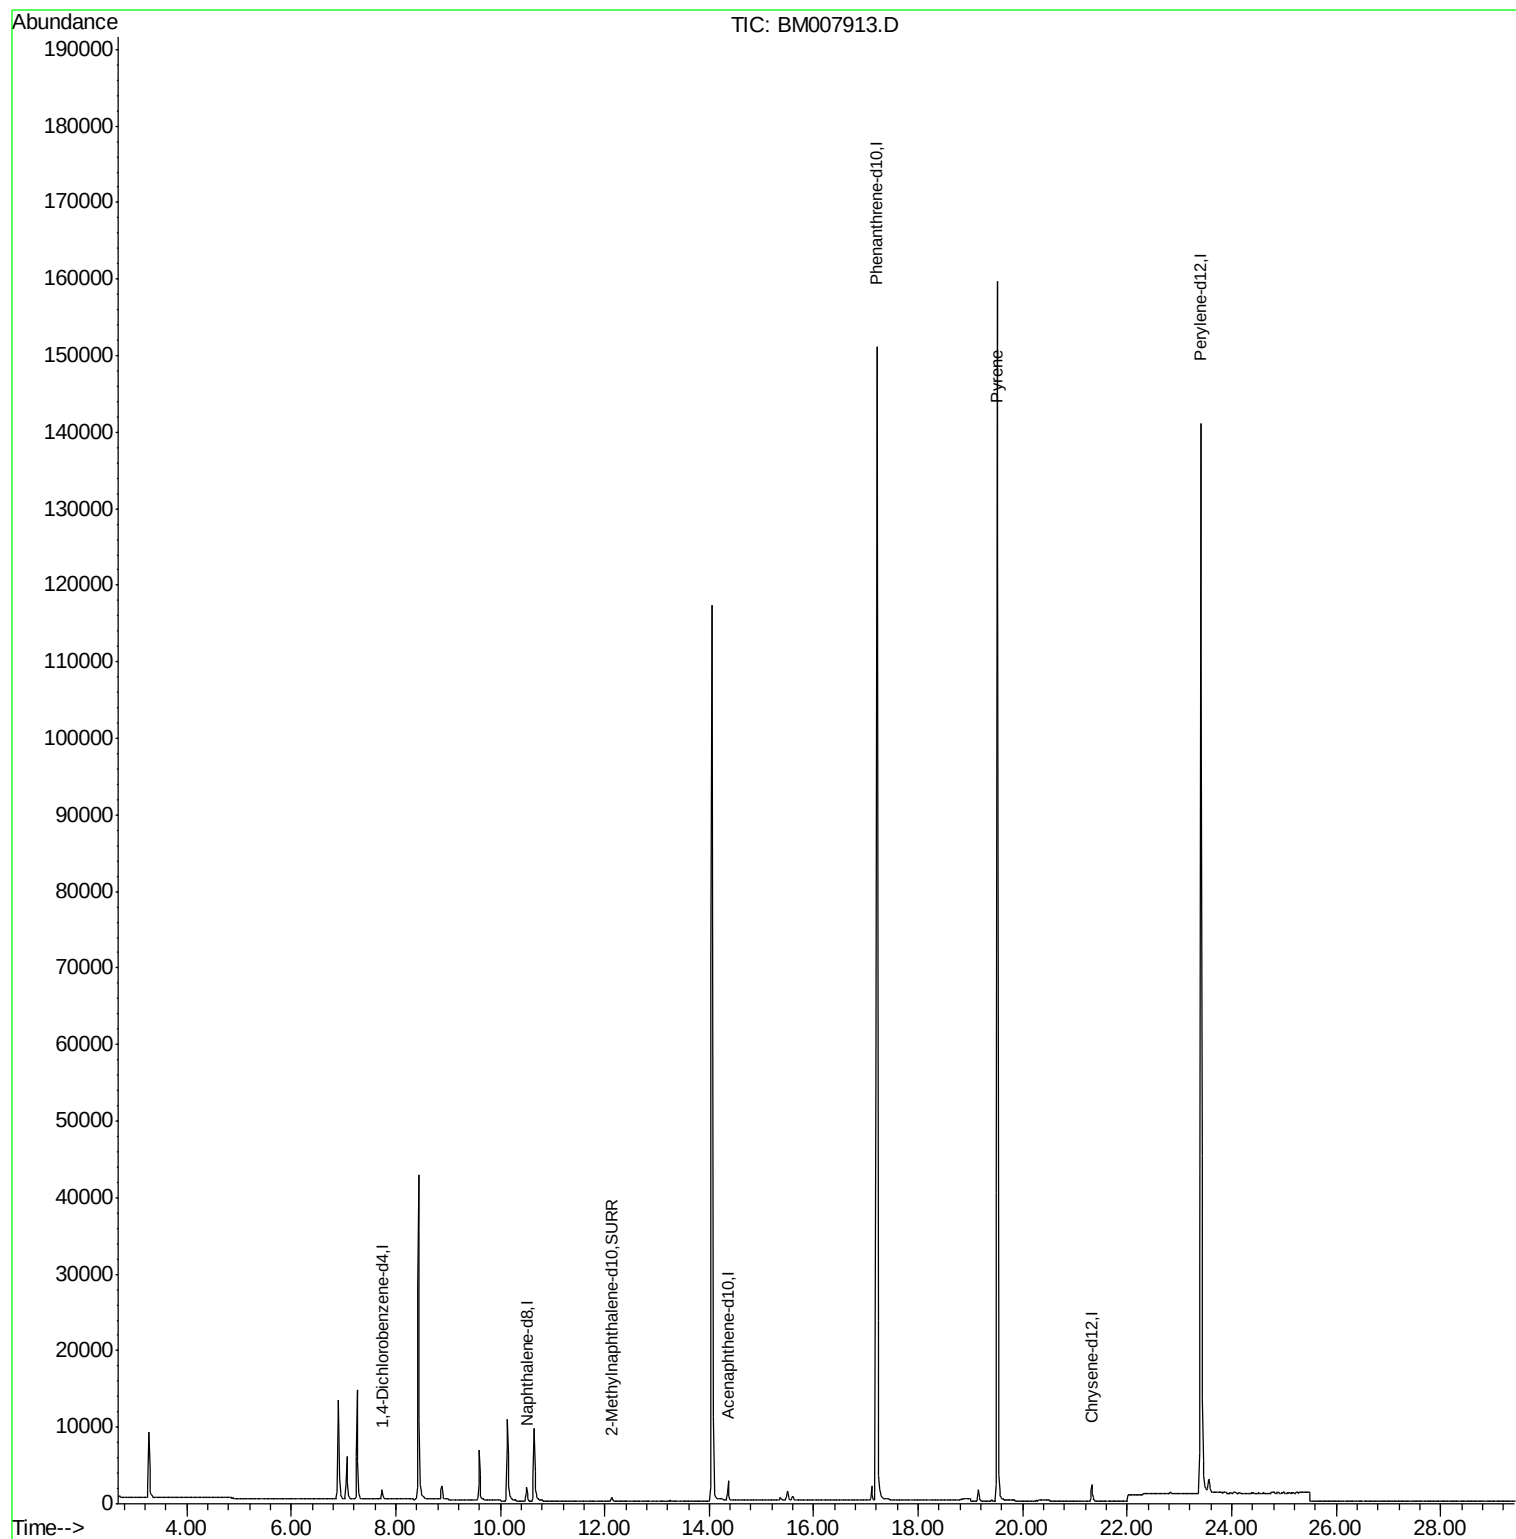

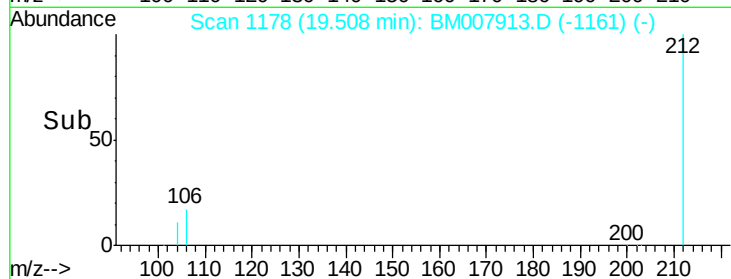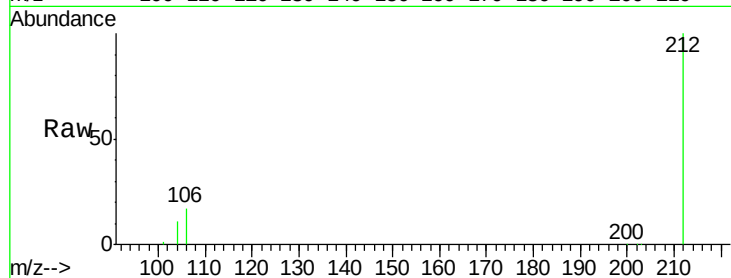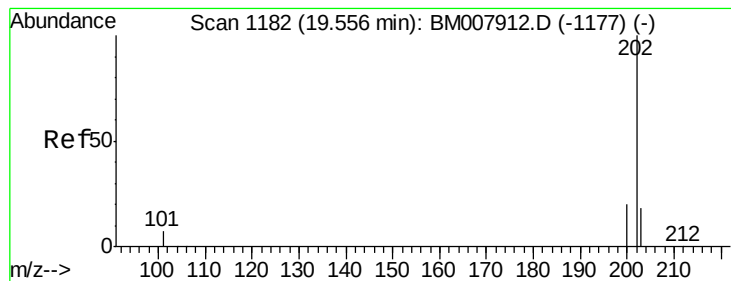

#17
 Pyrene
 Concen: 0.04 ng/ul
 RT: 19.51 min Scan# 1178
 Delta R.T. -0.05 min
 Lab File: BM007913.D
 Acq: 16 Nov 2016 10:24

Instrument :
 BNA_M
 ClientSampleId :
 SBLK42

Tgt Ion	Ratio	Lower	Upper
202	100		
200	19.6	18.2	27.4
203	141.4	15.6	23.4

