

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007926.D
 Acq On : 16 Nov 2016 18:03
 Operator : UM/SJ
 Sample : H5622-07RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WK7RE

Quant Time: Nov 17 04:44:14 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	923	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.51	136	2959	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.37	164	1465	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	146352	0.40	ng/ul	0.09
16) Chrysene-d12	21.33	240	2884	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	75927	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1093	0.31	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.52	202	849	0.09	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007926.D
Acq On : 16 Nov 2016 18:03
Operator : UM/SJ
Sample : H5622-07RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WK7RE

Quant Time: Nov 17 04:44:14 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

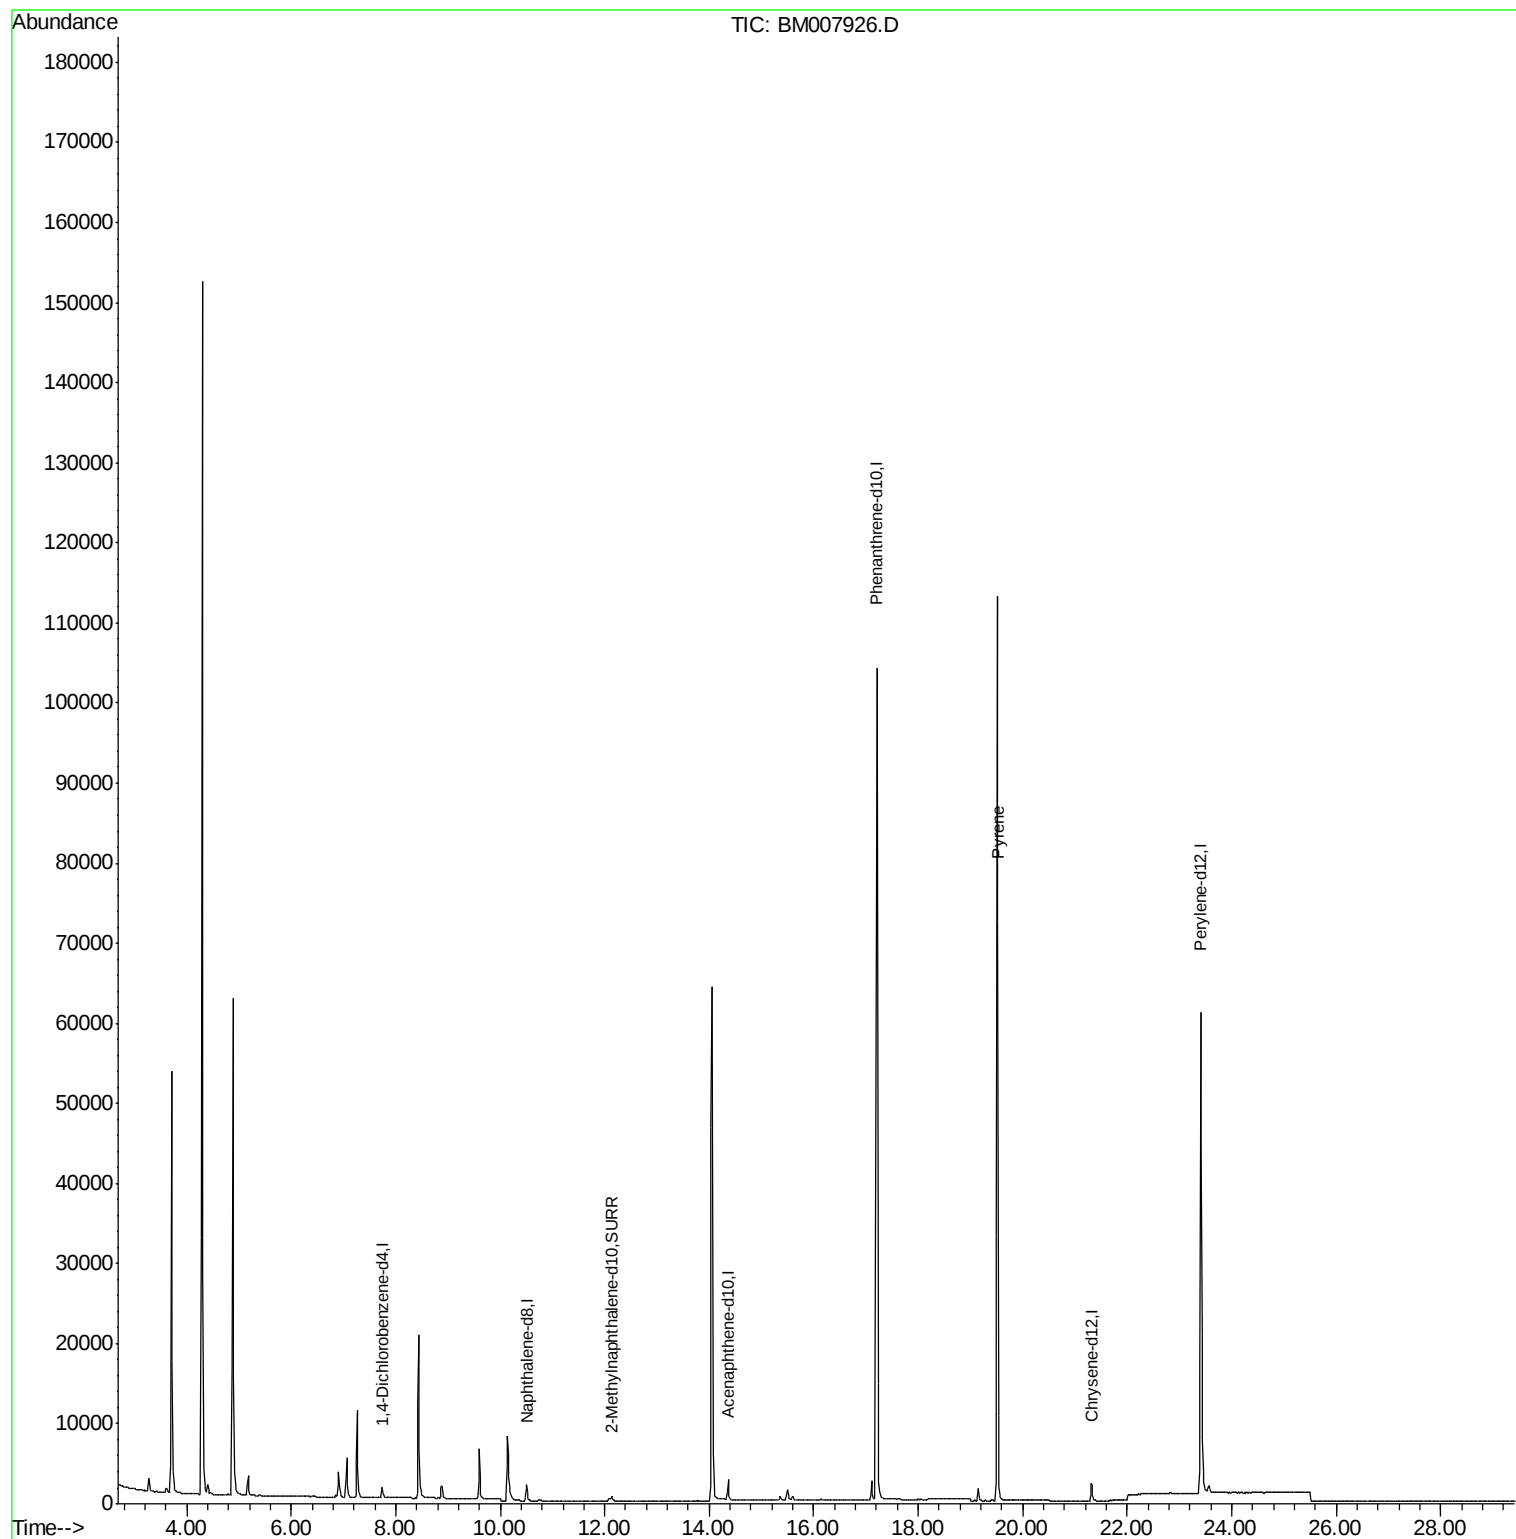

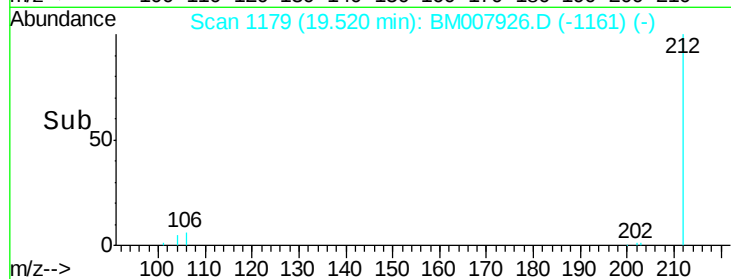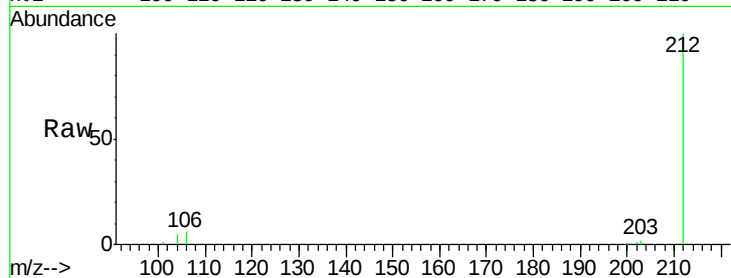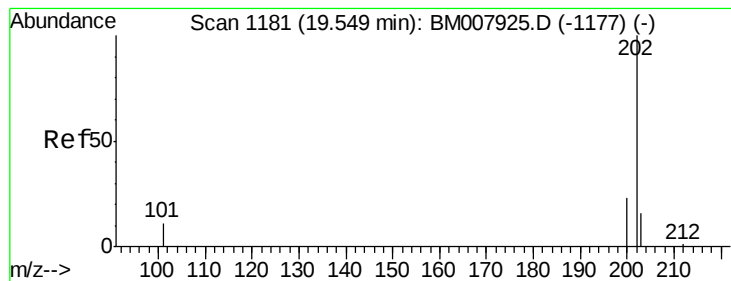

#17

Pyrene

Concen: 0.09 ng/ul

RT: 19.52 min Scan# 1179

Delta R.T. -0.03 min

Lab File: BM007926.D

Acq: 16 Nov 2016 18:03

Instrument :

BNA_M

ClientSampleId :

A4WK7RE

Tgt Ion: 202 Resp: 849

Ion Ratio Lower Upper

202 100

200 18.8 18.2 27.4

203 208.0 15.6 23.4#

