

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007927.D
 Acq On : 16 Nov 2016 18:39
 Operator : UM/SJ
 Sample : PB94744BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK44

Quant Time: Nov 17 04:44:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	884	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.51	136	2849	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.37	164	1663	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	234605	0.40	ng/ul	0.09
16) Chrysene-d12	21.33	240	2919	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	211368	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1251	0.37	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.51	202	455	0.05	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007927.D
Acq On : 16 Nov 2016 18:39
Operator : UM/SJ
Sample : PB94744BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK44

Quant Time: Nov 17 04:44:19 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

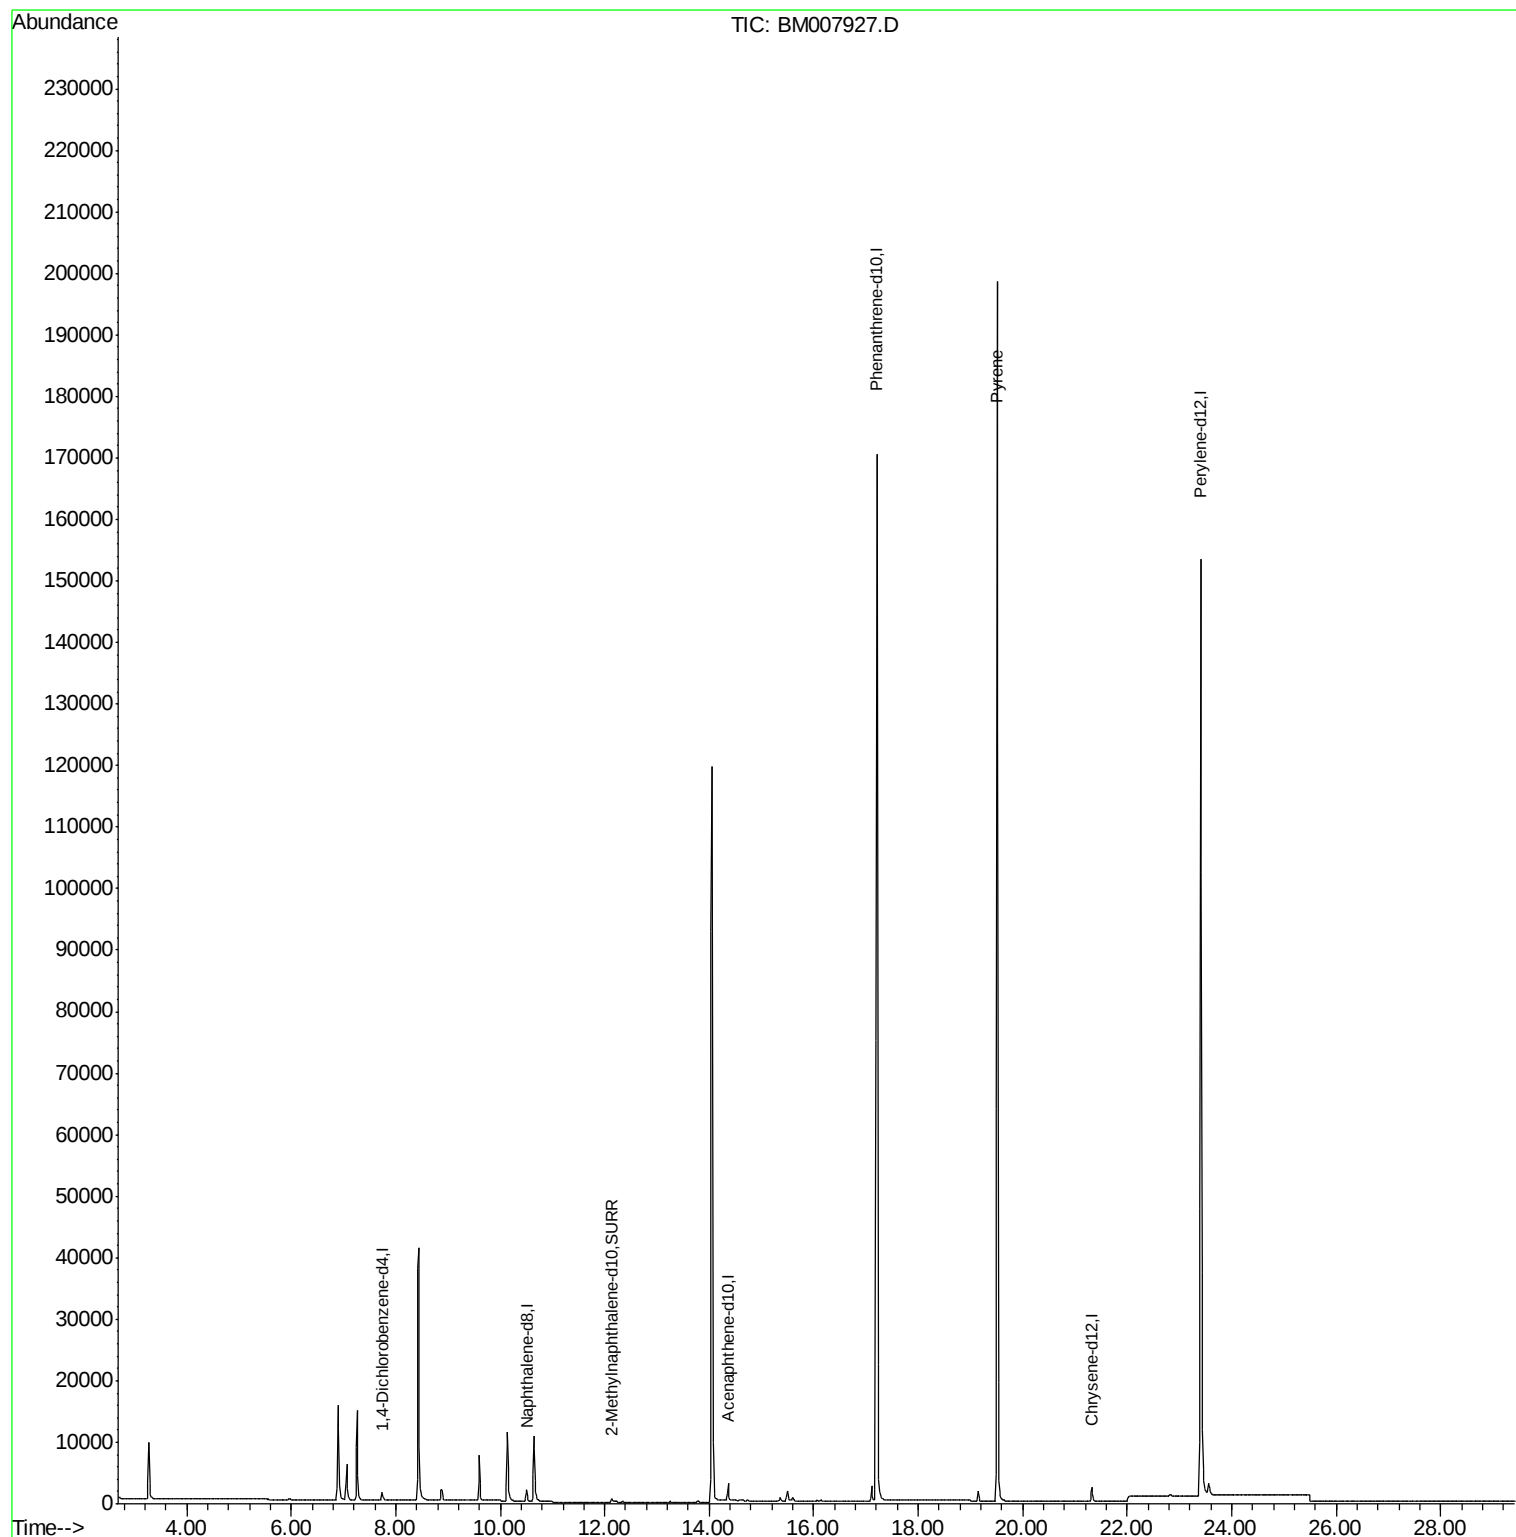

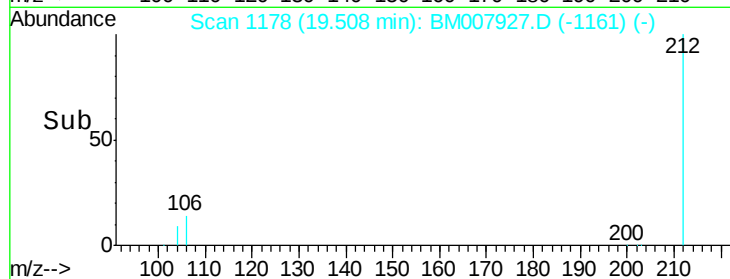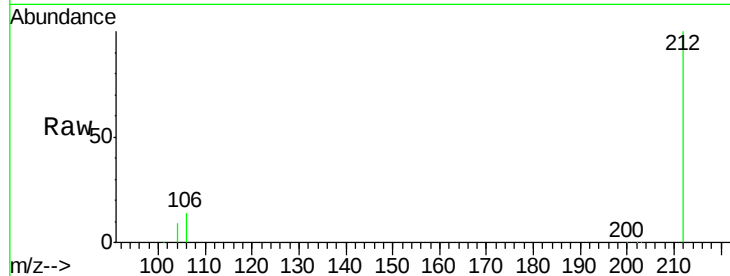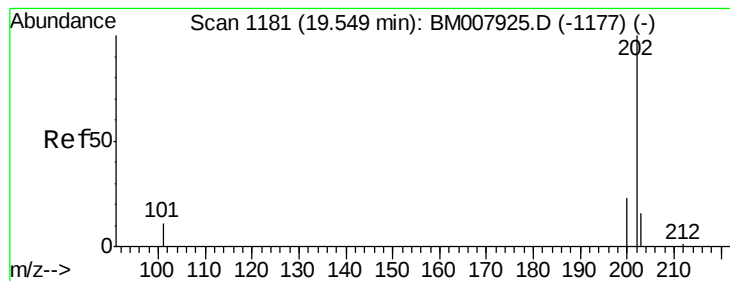

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.51 min Scan# 1178

Delta R.T. -0.04 min

Lab File: BM007927.D

Acq: 16 Nov 2016 18:39

Instrument :

BNA_M

ClientSampleId :

SBLK44

Tgt Ion: 202 Resp: 455

Ion Ratio Lower Upper

202 100

200 16.7 18.2 27.4#

203 153.2 15.6 23.4#

