

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007934.D
 Acq On : 16 Nov 2016 22:47
 Operator : UM/SJ
 Sample : H5622-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WL3

Quant Time: Nov 17 04:44:55 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	865	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.51	136	2765	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.37	164	1644	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	209827	0.40	ng/ul	0.09
16) Chrysene-d12	21.30	240	3228	0.40	ng/ul	-0.01
20) Perylene-d12	23.41	264	207153	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	1195	0.36	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.56	128	154	0.02	ng/ul#	20
17) Pyrene	19.53	202	866	0.08	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007934.D
Acq On : 16 Nov 2016 22:47
Operator : UM/SJ
Sample : H5622-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WL3

Quant Time: Nov 17 04:44:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

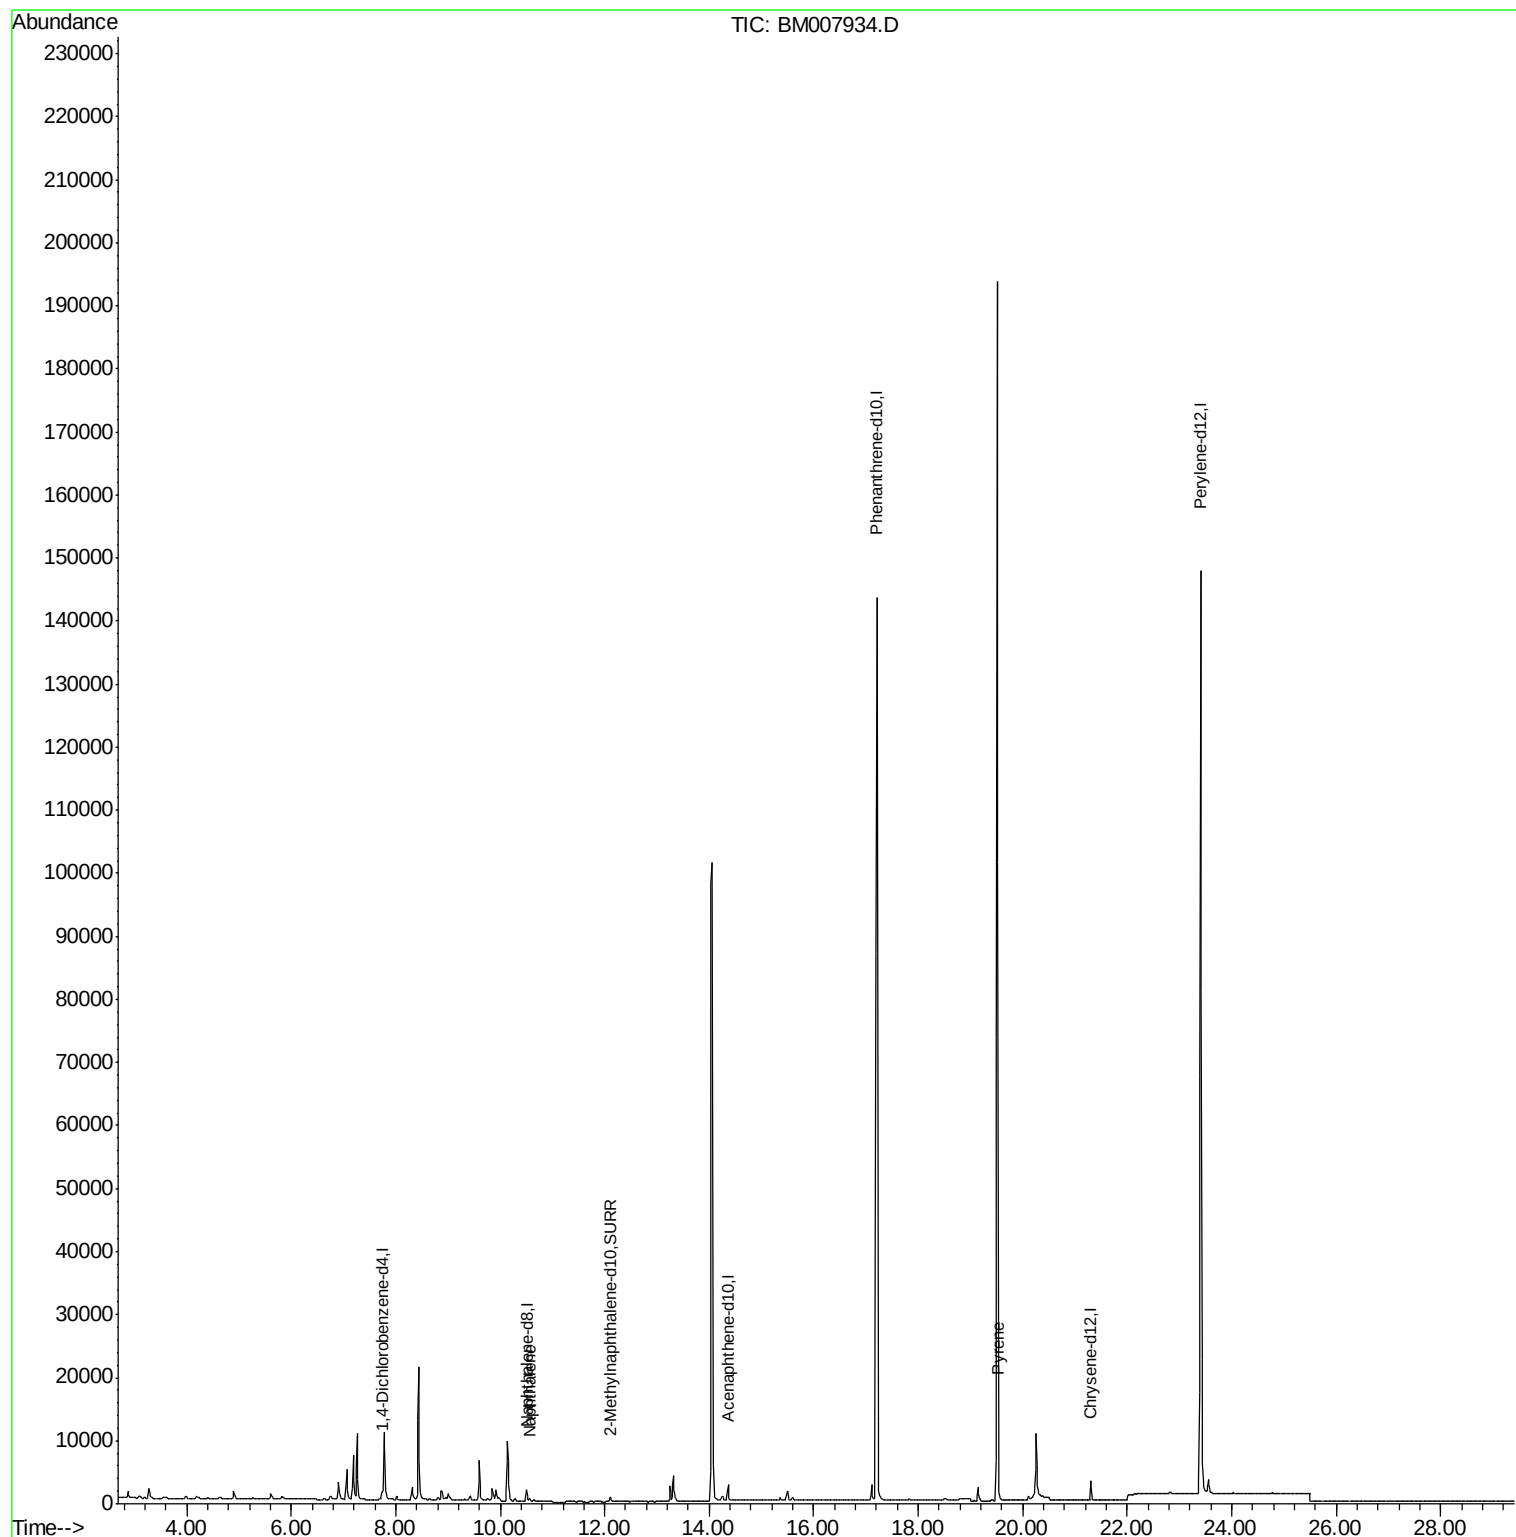

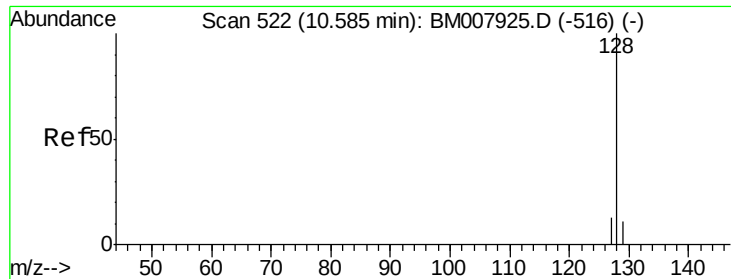

#3

Naphthalene

Concen: 0.02 ng/ul

RT: 10.56 min Scan# 520

Delta R.T. -0.02 min

Lab File: BM007934.D

Acq: 16 Nov 2016 22:47

Instrument :

BNA_M

ClientSampleId :

A4WL3


Tgt Ion:128 Resp: 154

Ion Ratio Lower Upper

128 100

129 49.6 11.3 16.9#




127 47.2 12.8 19.2#

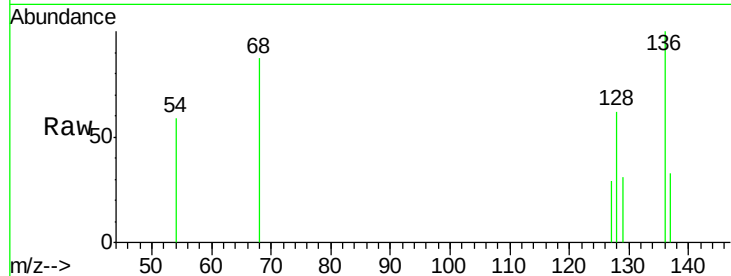

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

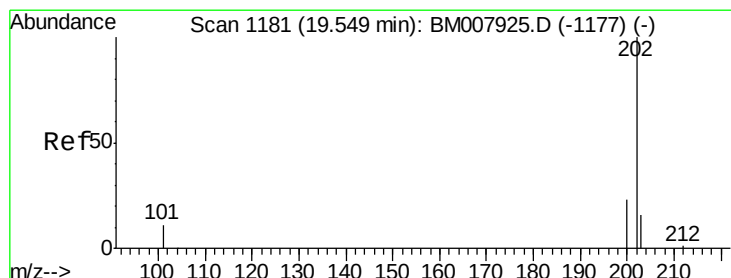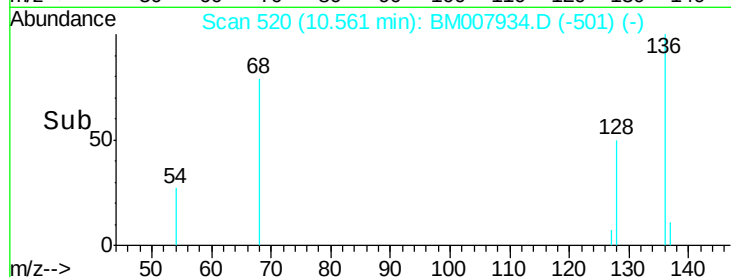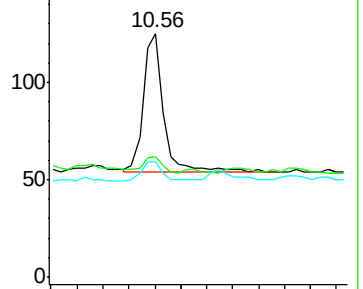

#17

Pyrene

Concen: 0.08 ng/ul

RT: 19.53 min Scan# 1180

Delta R.T. -0.02 min

Lab File: BM007934.D

Acq: 16 Nov 2016 22:47


Tgt Ion:202 Resp: 866

Ion Ratio Lower Upper

202 100

200 35.7 18.2 27.4#

203 47.5 15.6 23.4#

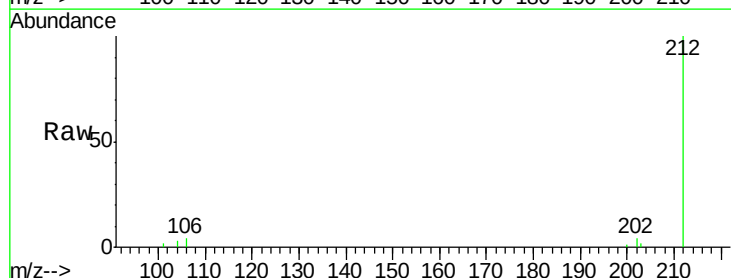

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

