

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007936.D
 Acq On : 16 Nov 2016 23:58
 Operator : UM/SJ
 Sample : H5622-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WL5

Quant Time: Nov 17 04:45:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	875	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.51	136	2844	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.37	164	1671	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	222015	0.40	ng/ul	0.09
16) Chrysene-d12	21.31	240	3197	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	211959	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1097	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.51	202	476	0.04	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007936.D
Acq On : 16 Nov 2016 23:58
Operator : UM/SJ
Sample : H5622-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WL5

Quant Time: Nov 17 04:45:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

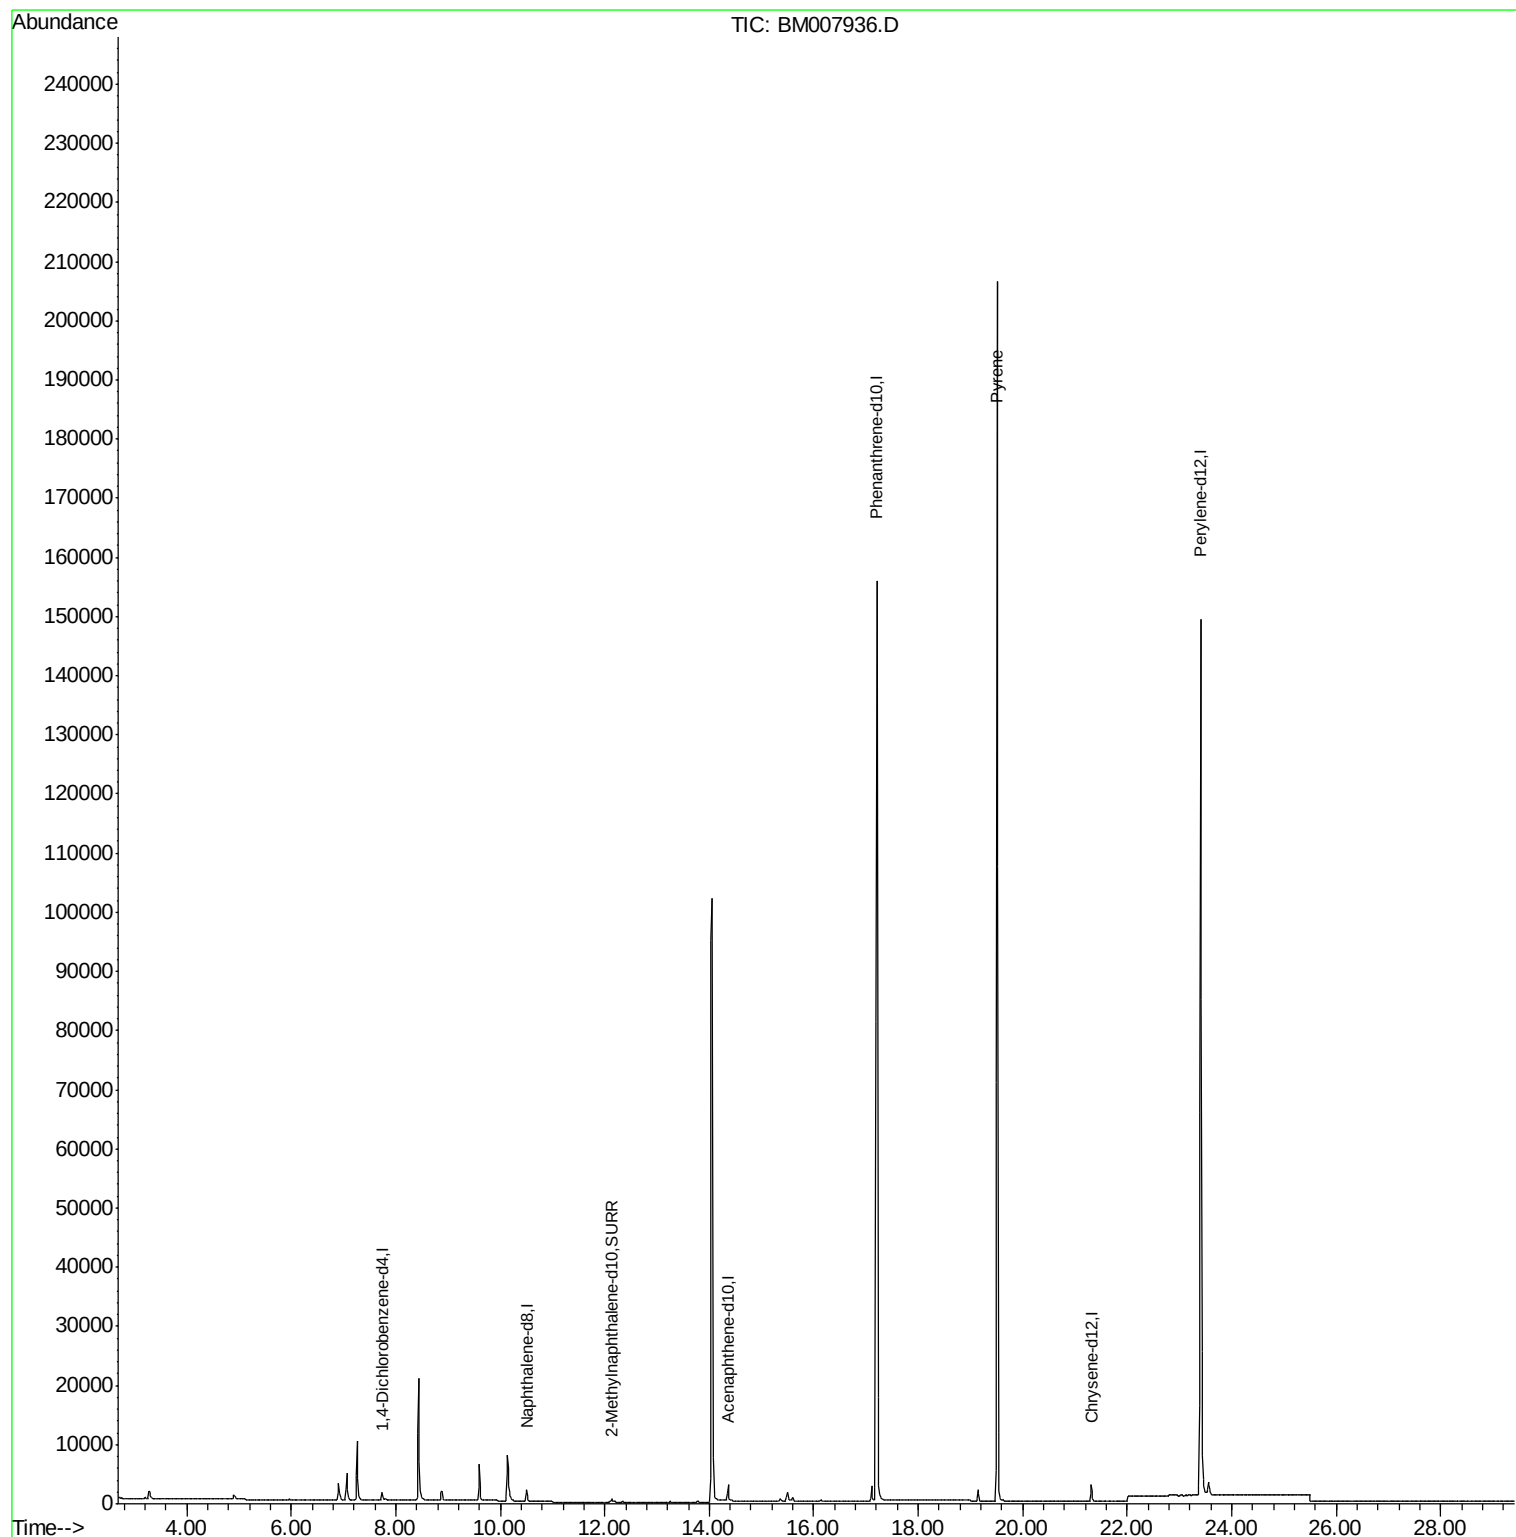

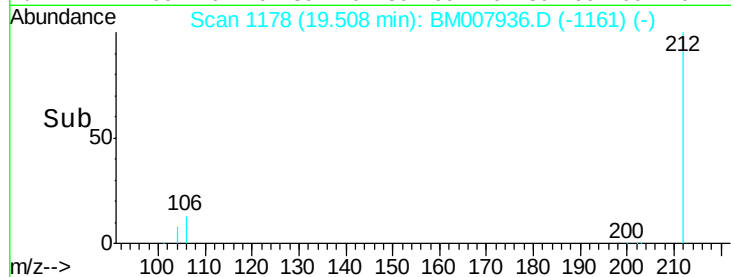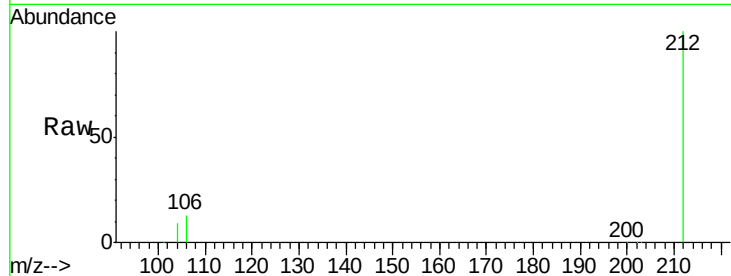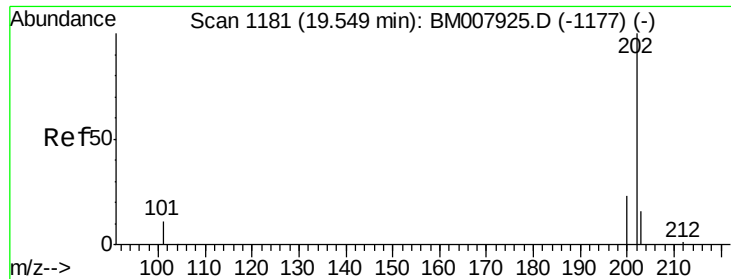

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.51 min Scan# 1178

Delta R.T. -0.04 min

Lab File: BM007936.D

Acq: 16 Nov 2016 23:58

Instrument :

BNA_M

ClientSampleId :

A4WL5

Tgt Ion: 202 Resp: 476

Ion Ratio Lower Upper

202 100

200 17.3 18.2 27.4#

203 162.8 15.6 23.4#

