


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007916.D
Acq On : 16 Nov 2016 12:10
Operator : UM/SJ
Sample : H5622-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WK9

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:54:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

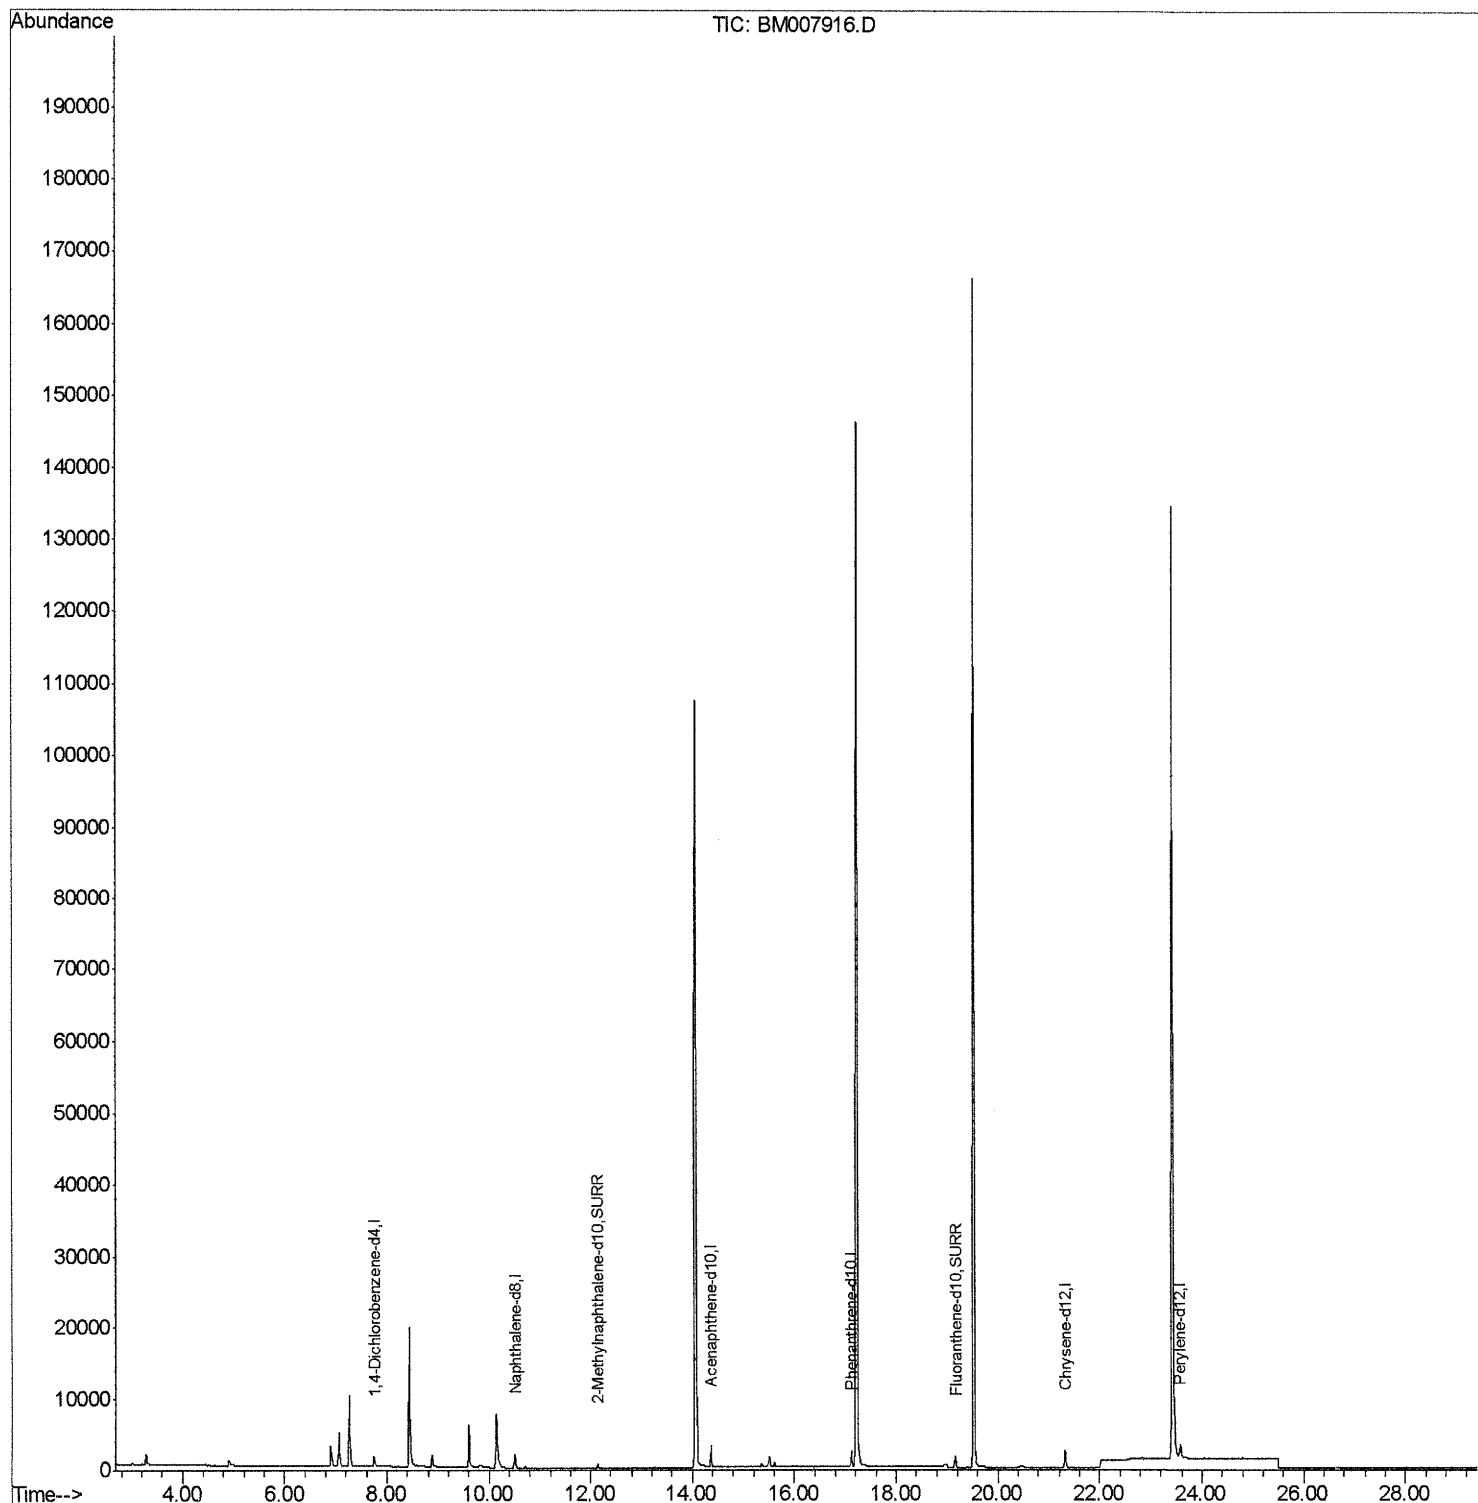




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007916.D
Acq On : 16 Nov 2016 12:10
Operator : UM/SJ
Sample : H5622-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WK9

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:52:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

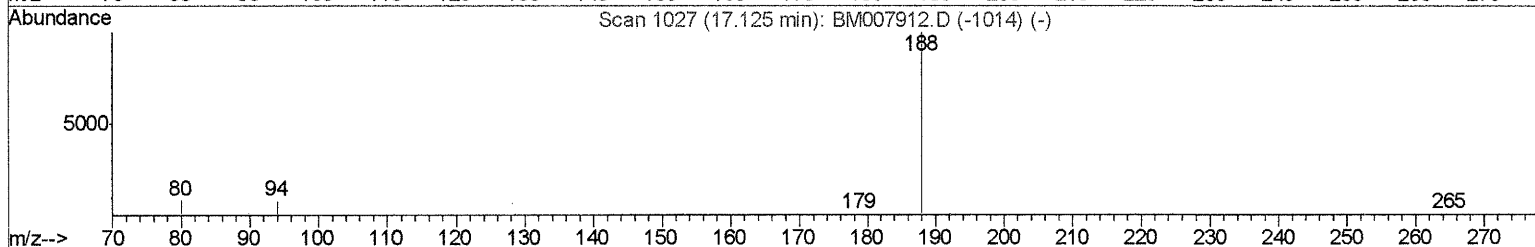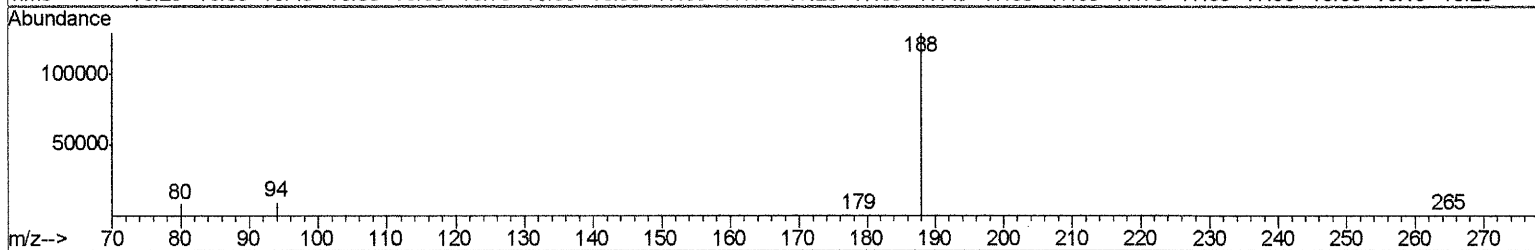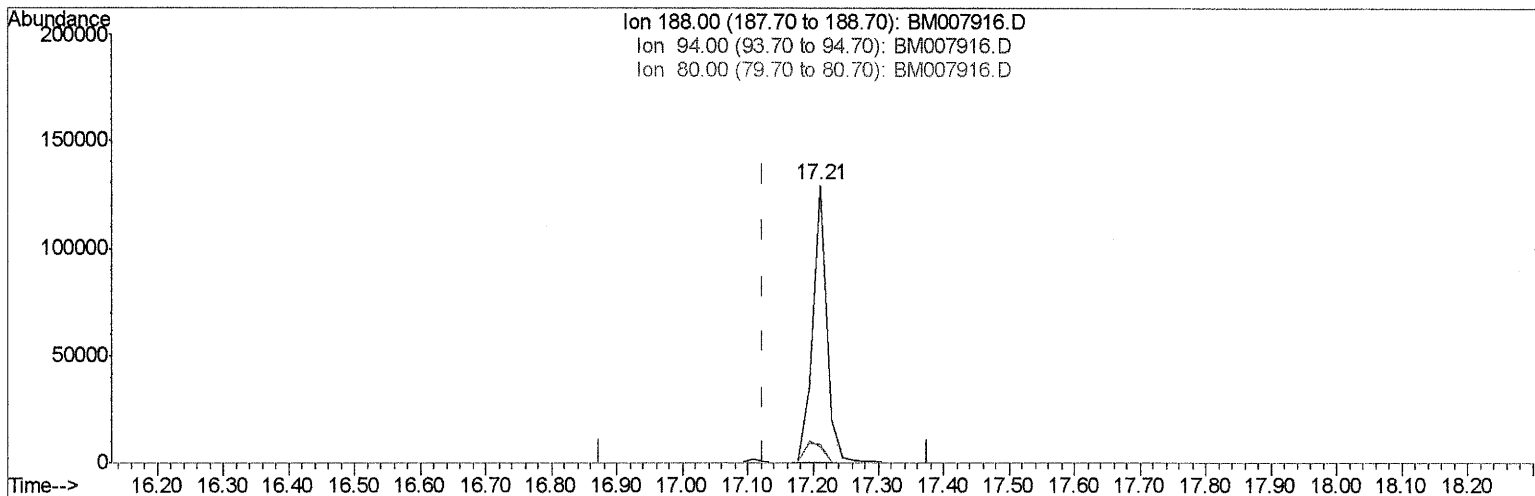

TIC: BM007916.D

(10) Phenanthrene-d10 (I)
17.211min (+0.086) 0.40ng/ul
response 194312

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.91#
80.00	11.80	5.95#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007916.D
Acq On : 16 Nov 2016 12:10
Operator : UM/SJ
Sample : H5622-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A4WK9

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:52:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

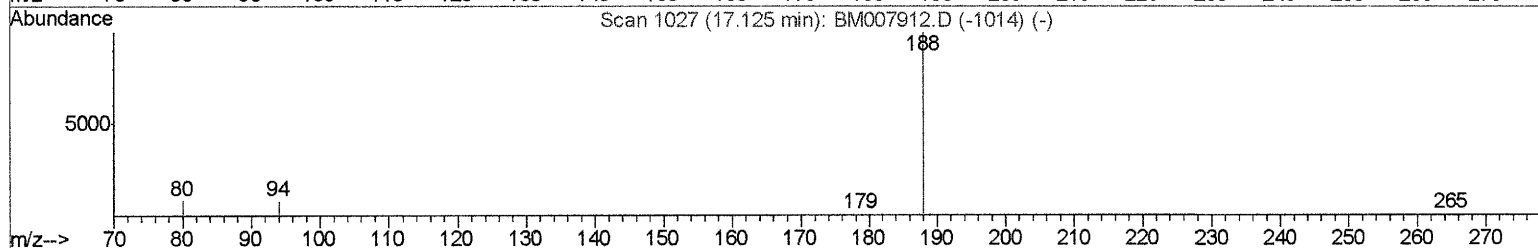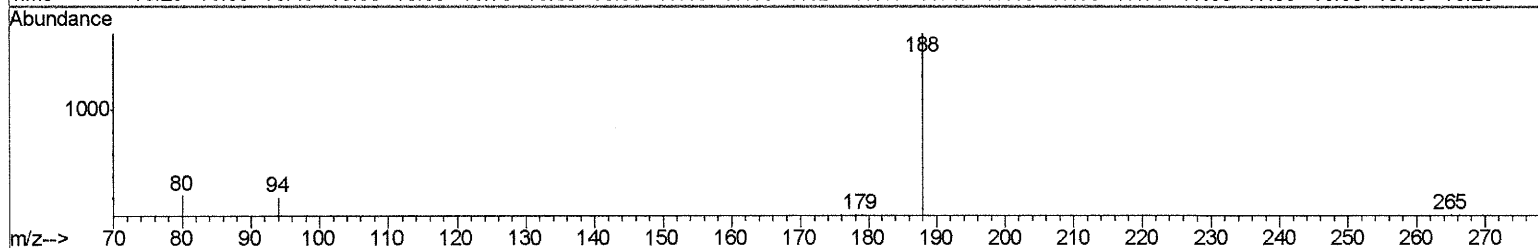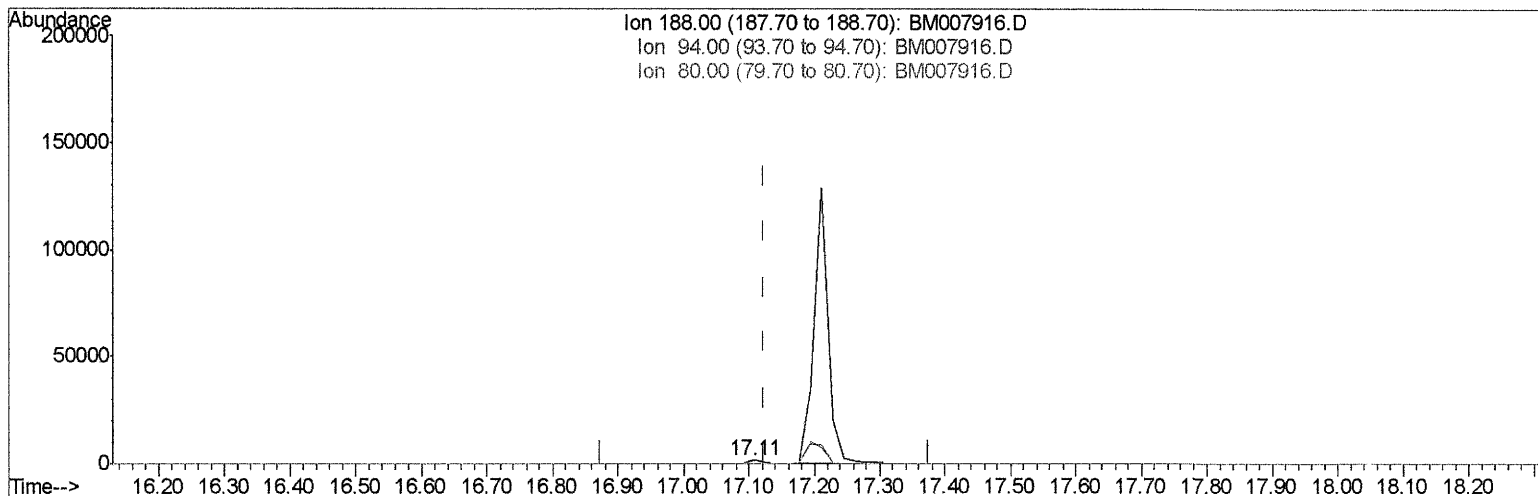

TIC: BM007916.D

(10) Phenanthrene-d10 (I)

17.108min (-0.017) 0.40ng/ul m

response 2934

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.23
80.00	11.80	13.36
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007916.D
Acq On : 16 Nov 2016 12:10
Operator : UM/SJ
Sample : H5622-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WK9

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:53:22 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

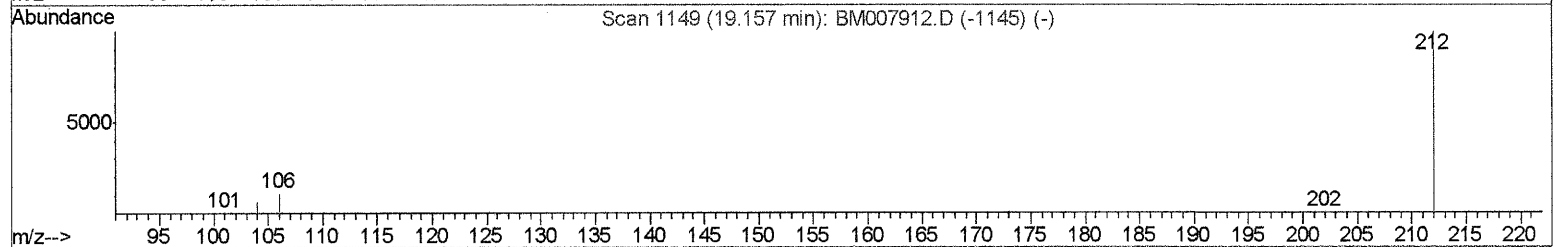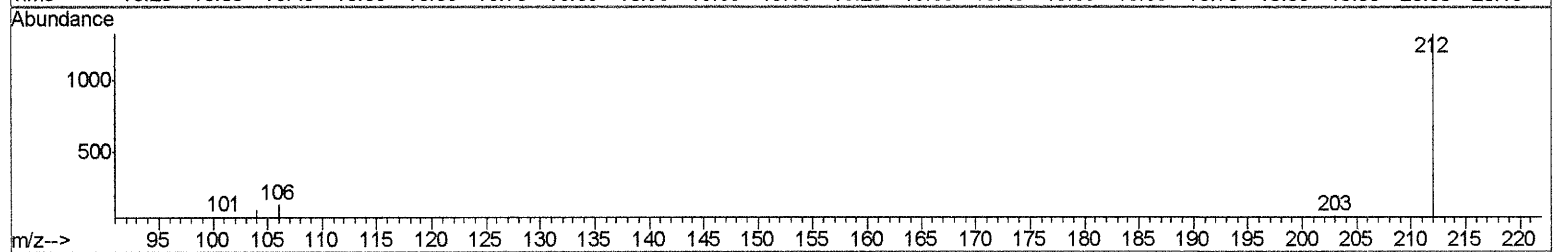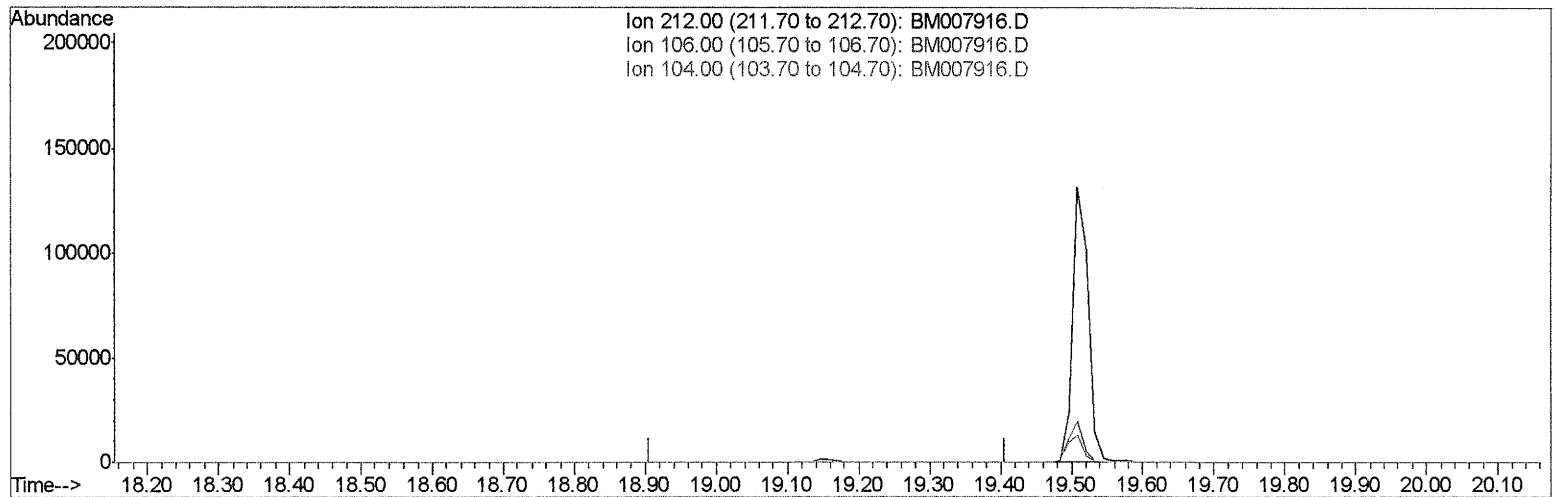

TIC: BM007916.D

(14) Fluoranthene-d10 (SURR)

19.157min (-19.157) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007916.D
 Acq On : 16 Nov 2016 12:10
 Operator : UM/SJ
 Sample : H5622-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WK9

Manual Integrations
 APPROVED

umangi
 11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:53:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:16:41 2016
 Response via : Initial Calibration

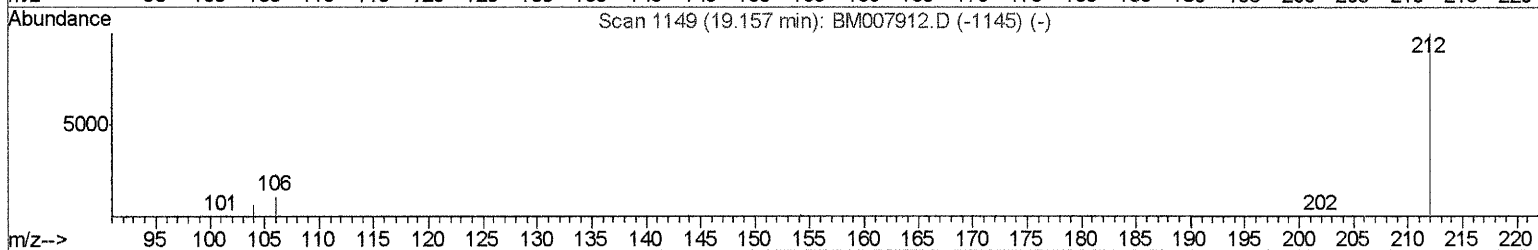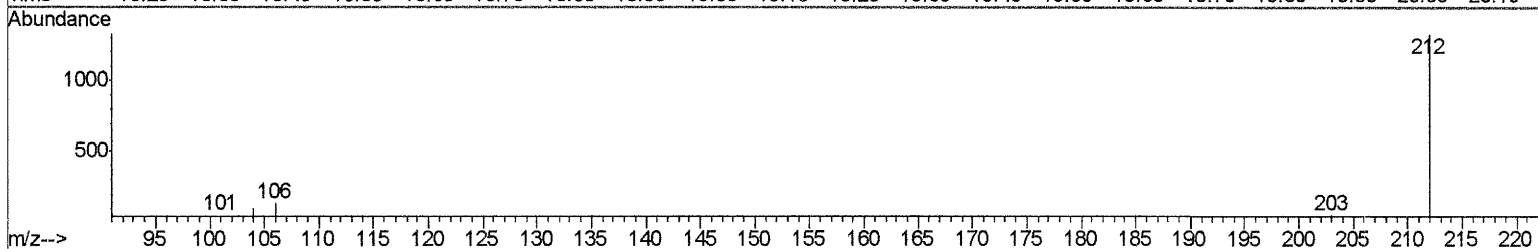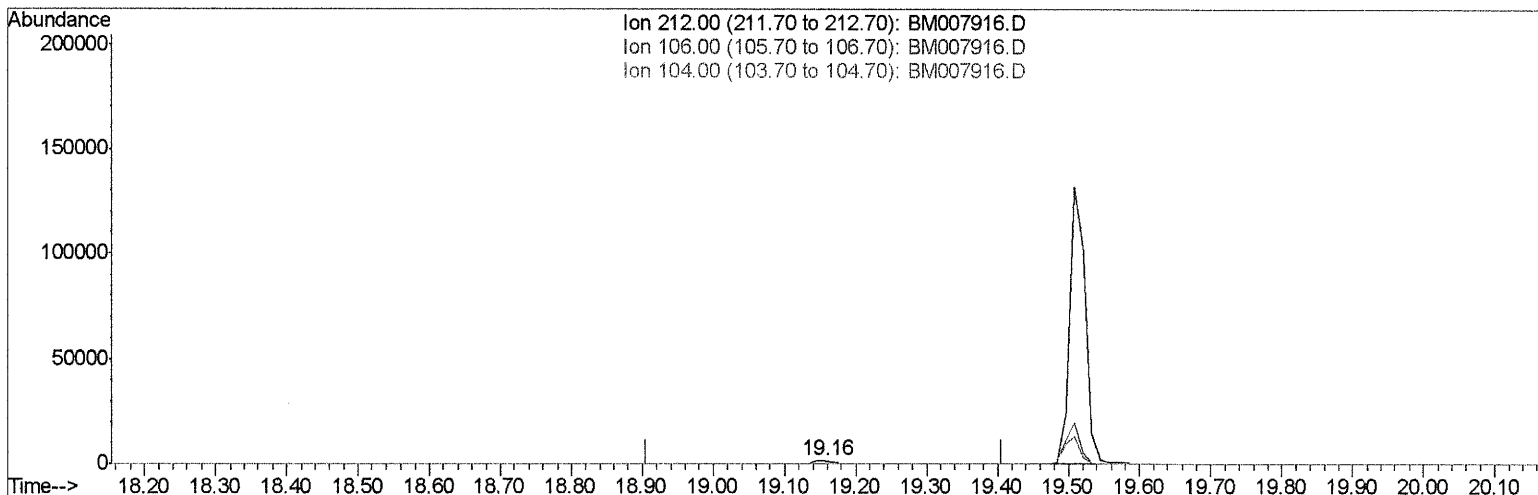

TIC: BM007916.D

(14) Fluoranthene-d10 (SURR)

19.157min (+0.000) 0.37ng/ul m

response 2426

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

um
 11/17/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007916.D
 Acq On : 16 Nov 2016 12:10
 Operator : UM/SJ
 Sample : H5622-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WK9

Manual Integrations
 APPROVED

umangi
 11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:53:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:16:41 2016
 Response via : Initial Calibration

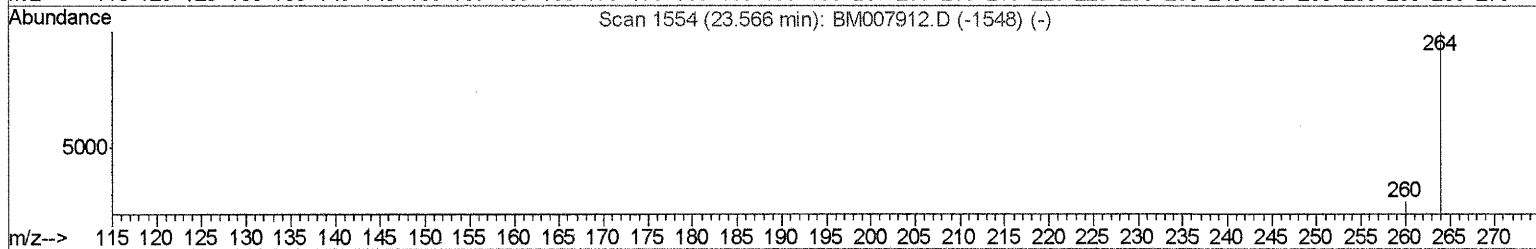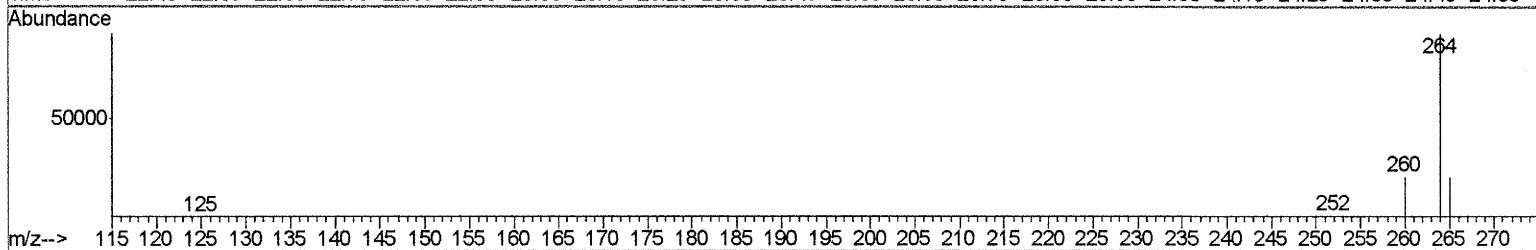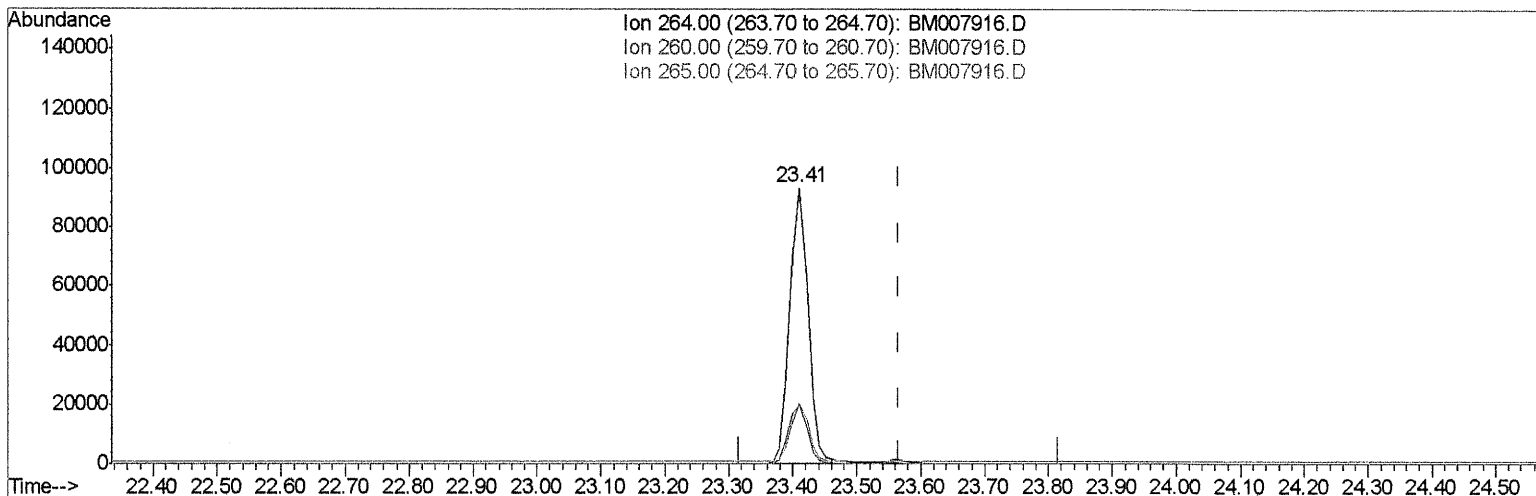

TIC: BM007916.D

(20) Perylene-d12 (I)

23.410min (-0.156) 0.40ng/ul

response 182734

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.57#
265.00	103.50	21.71#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007916.D
 Acq On : 16 Nov 2016 12:10
 Operator : UM/SJ
 Sample : H5622-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4WK9

Manual Integrations
 APPROVED

umangi
 11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:53:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:16:41 2016
 Response via : Initial Calibration

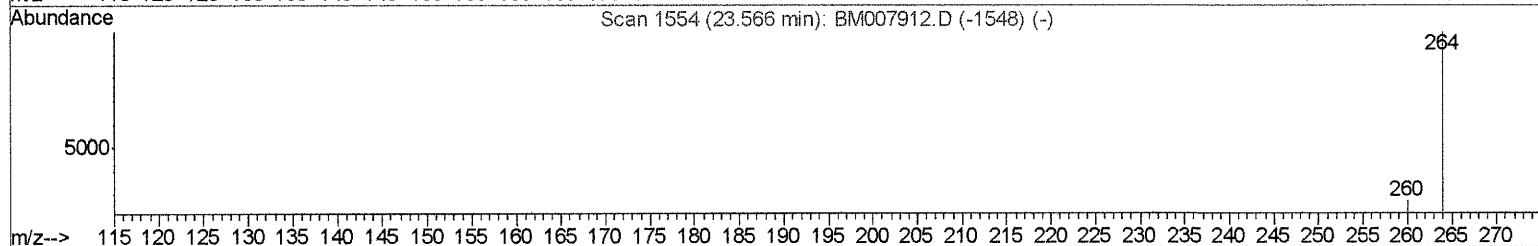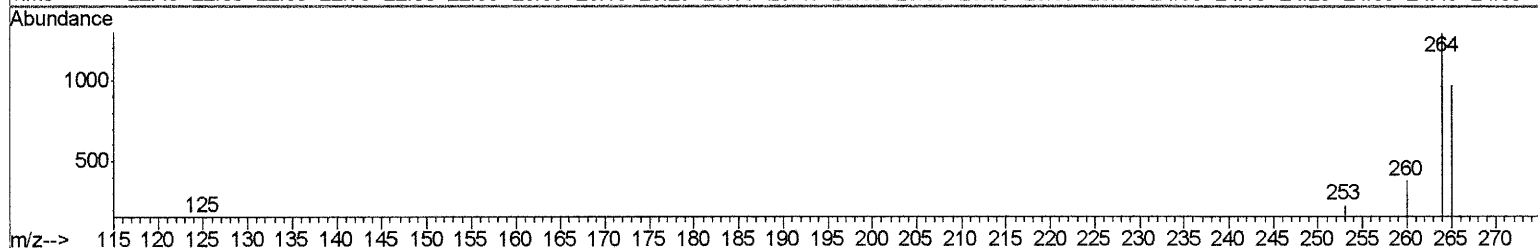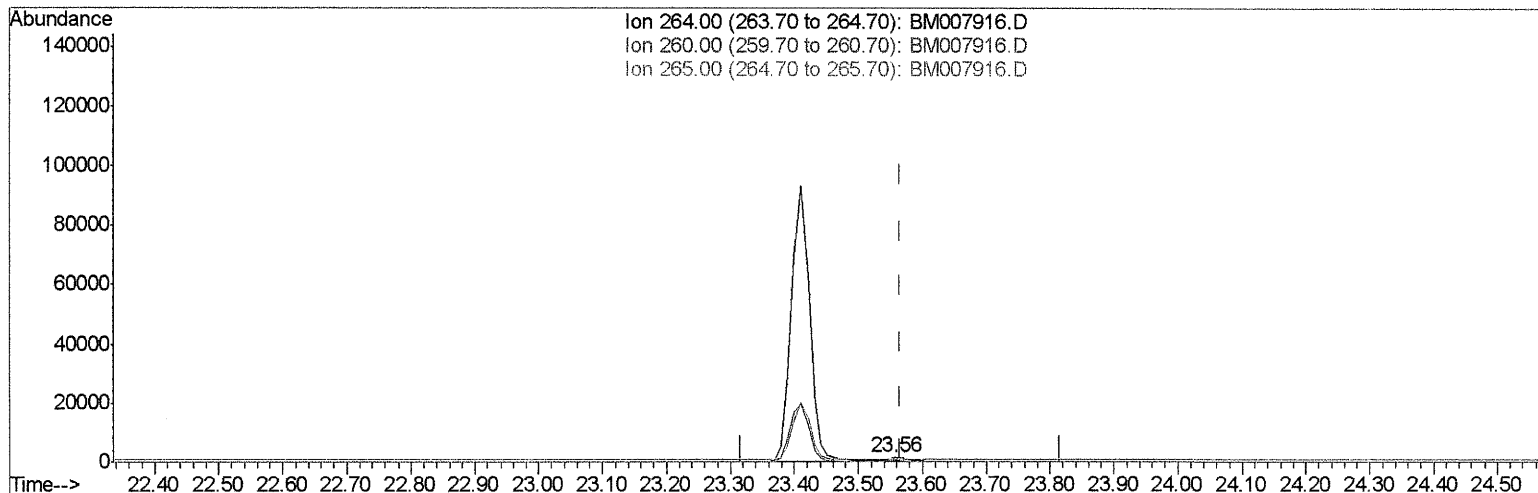

TIC: BM007916.D

(20) Perylene-d12 (I)

23.556min (-0.010) 0.40ng/ul m

UM

response 2510

11/16/16

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	29.01
265.00	103.50	74.77#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007916.D
Acq On : 16 Nov 2016 12:10
Operator : UM/SJ
Sample : H5622-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A4WK9

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:11 PM

Quant Time: Nov 16 16:54:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	808	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	2585	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1447	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	2934m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.31	240	2663	0.40	ng/ul	0.00
20) Perylene-d12	23.56	264	2510m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	992	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.16	212	2426m	0.37	ng/ul	0.00

} um
11/17/16

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed