




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007921.D
Acq On : 16 Nov 2016 15:07
Operator : UM/SJ
Sample : H5626-04DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F2J03DL

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:24 PM

Quant Time: Nov 16 17:18:54 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

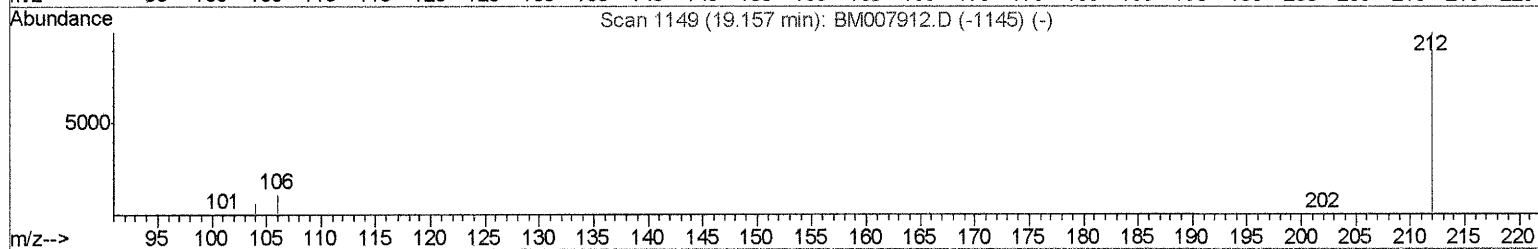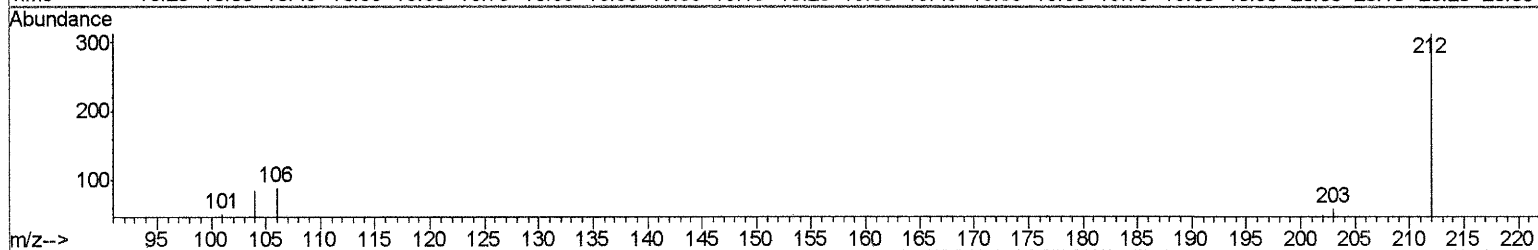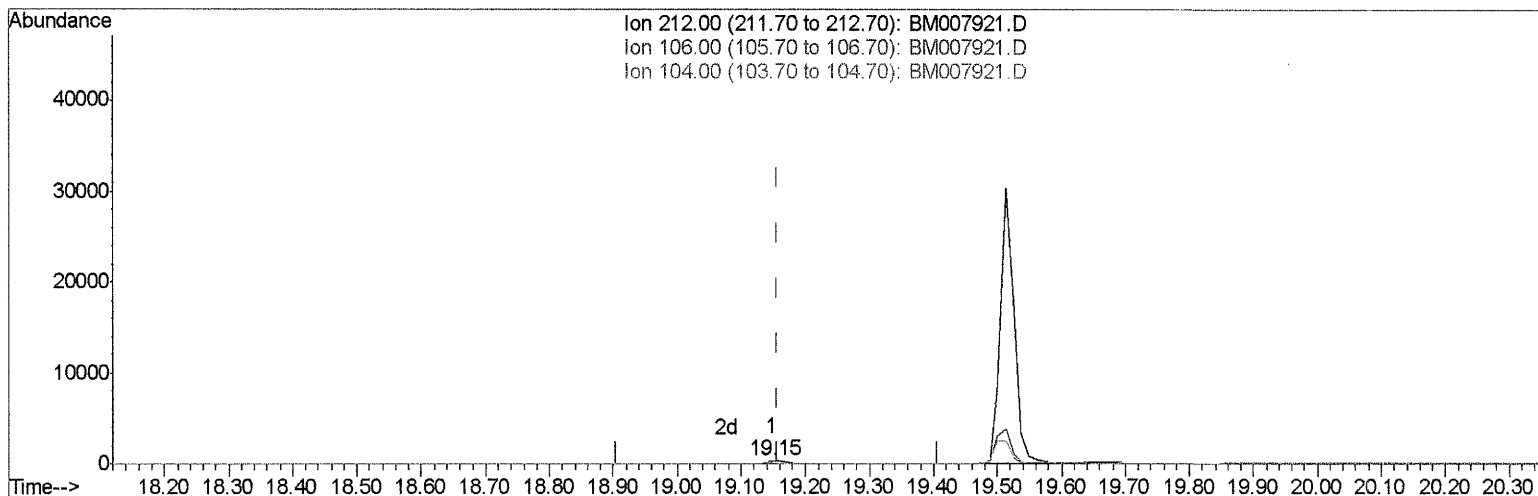

TIC: BM007921.D

(14) Fluoranthene-d10 (SURR)

19.150min (-0.007) 0.12ng/ul

response 738

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	40.24#
104.00	15.60	42.41#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007921.D
 Acq On : 16 Nov 2016 15:07
 Operator : UM/SJ
 Sample : H5626-04DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 F2J03DL

Manual Integrations
 APPROVED

umangi
 11/17/2016 5:55:24 PM

Quant Time: Nov 16 17:18:54 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:16:41 2016
 Response via : Initial Calibration

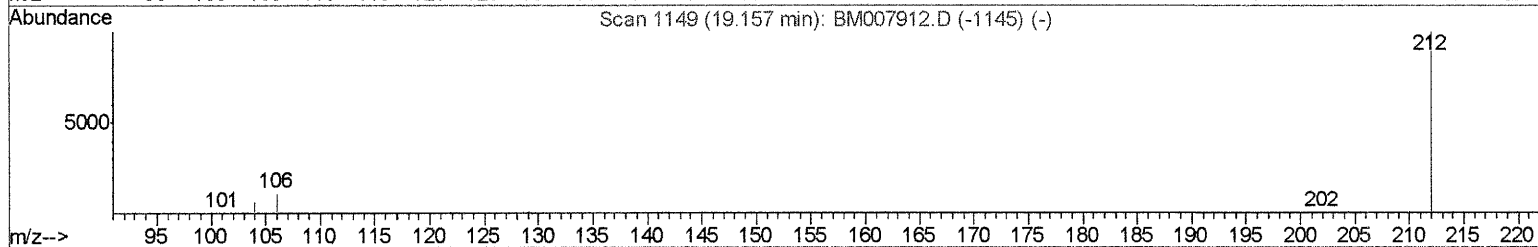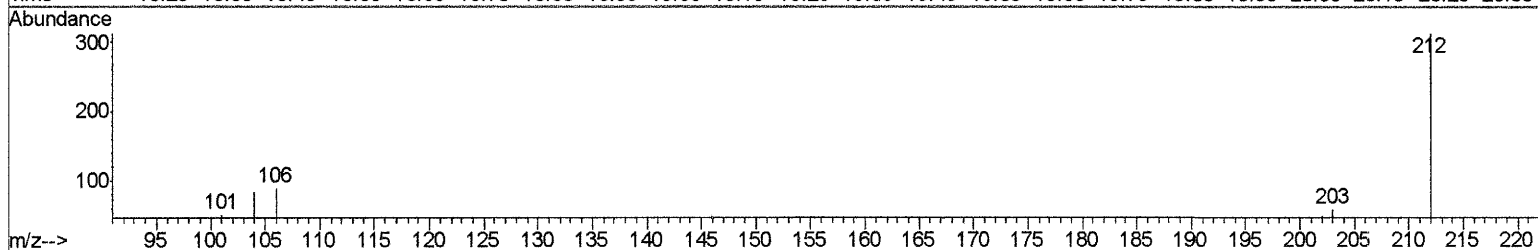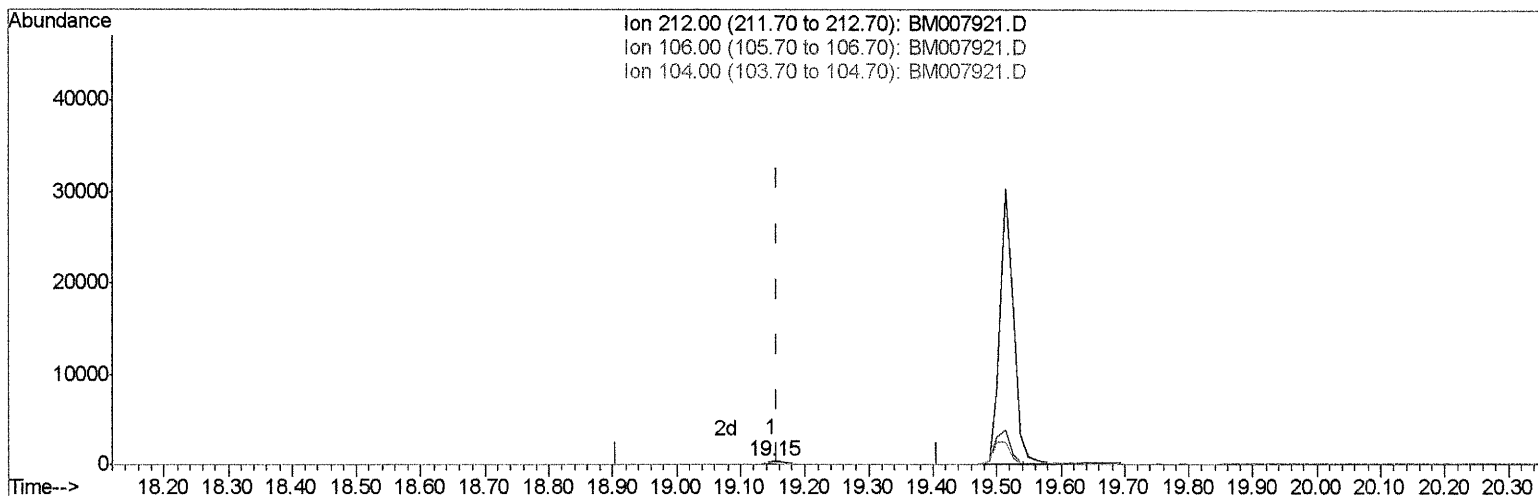

TIC: BM007921.D

(14) Fluoranthene-d10 (SURR)

19.150min (-0.007) 0.08ng/ul m

response 487

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	60.99#
104.00	15.60	64.27#
0.00	0.00	0.00

um
 11/17/16

Quantitation Report

(QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007921.D
 Acq On : 16 Nov 2016 15:07
 Operator : UM/SJ
 Sample : H5626-04DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Nov 21 01:06:13 2016

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Nov 16 16:16:41 2016

Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :

F2J03DL

Manual Integrations
APPROVED

umangi

11/17/2016 5:55:24 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	866	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	2746	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1480	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	2741	0.40	ng/ul	-0.02
16) Chrysene-d12	21.32	240	2786	0.40	ng/ul	0.00
20) Perylene-d12	23.57	264	3289	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	212	0.07	ng/ul	-0.01
14) Fluoranthene-d10	19.15	212	487m	0.08	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.56	128	134827	19.10	ng/ul#	92
5) 2-Methylnaphthalene	12.19	142	2787	0.62	ng/ul	98
8) Acenaphthene	14.42	153	1375	0.26	ng/ul	89
9) Fluorene	15.43	166	915	0.16	ng/ul#	95
11) Pentachlorophenol	16.80	266	108	0.17	ng/ul	96
12) Phenanthrene	17.16	178	825	0.11	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

0.00
 11/17/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007921.D
Acq On : 16 Nov 2016 15:07
Operator : UM/SJ
Sample : H5626-04DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Nov 21 01:06:13 2016

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Nov 16 16:16:41 2016

Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :

F2J03DL

Manual Integrations
APPROVED

umangi

11/17/2016 5:55:24 PM

