


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007934.D
Acq On : 16 Nov 2016 22:47
Operator : UM/SJ
Sample : H5622-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WL3

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:59 PM

Quant Time: Nov 17 06:23:18 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

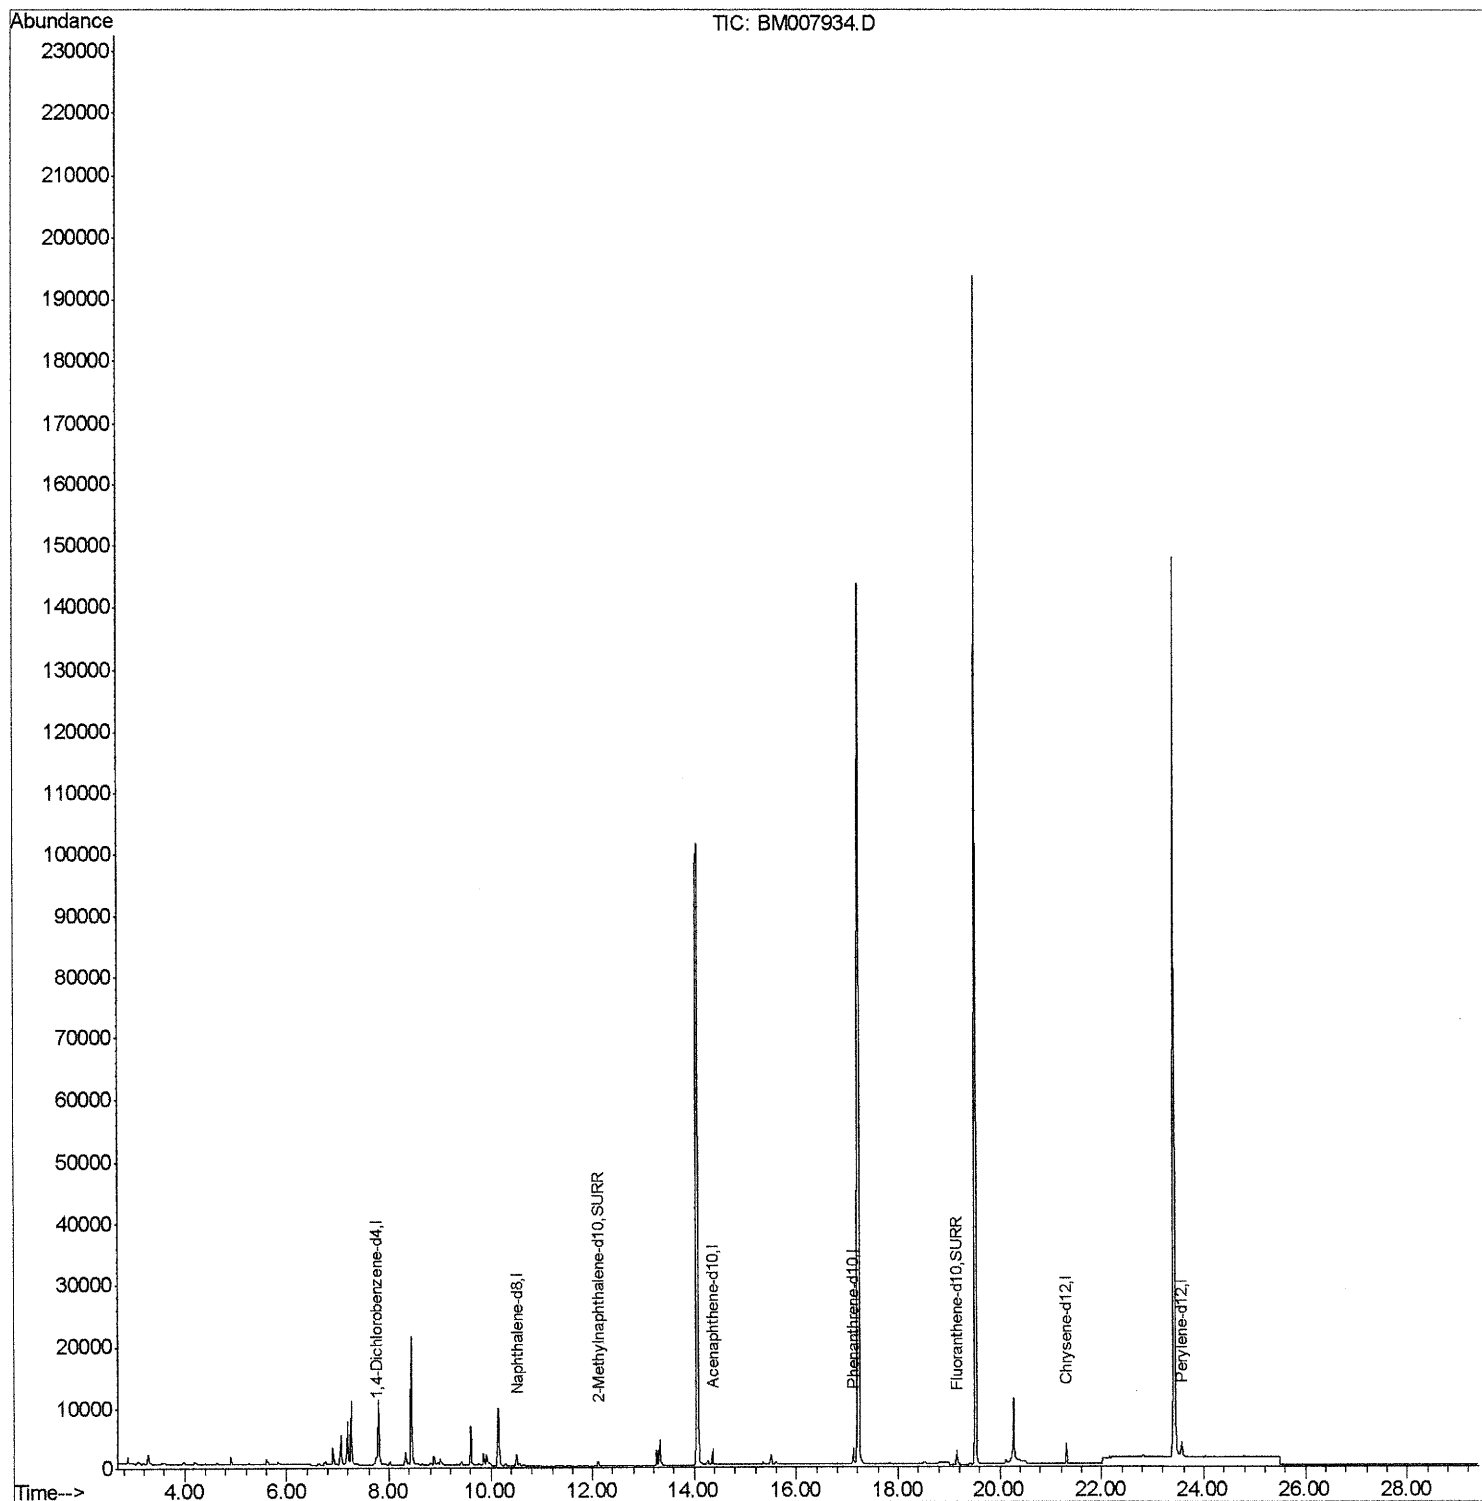




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007934.D
Acq On : 16 Nov 2016 22:47
Operator : UM/SJ
Sample : H5622-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WL3

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:59 PM

Quant Time: Nov 17 04:44:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

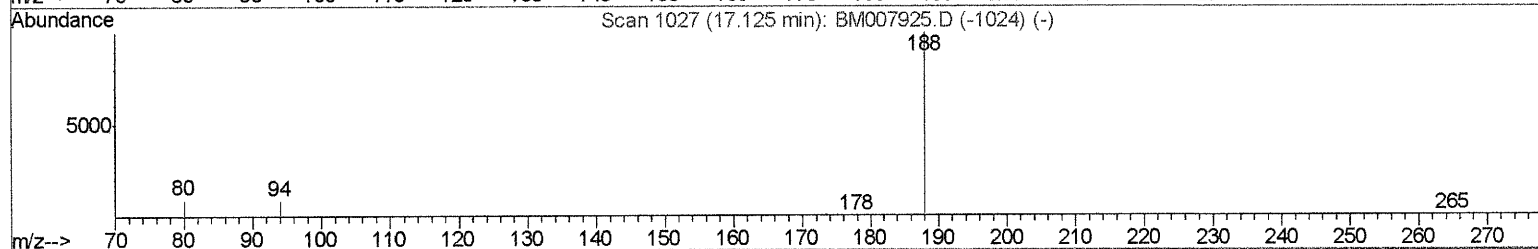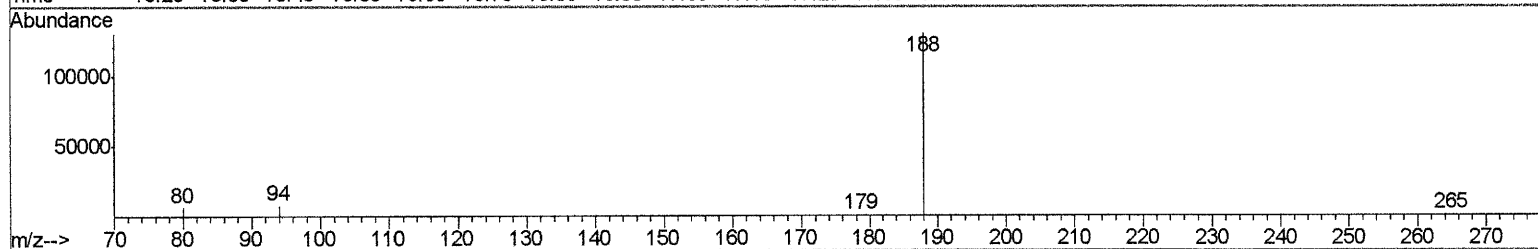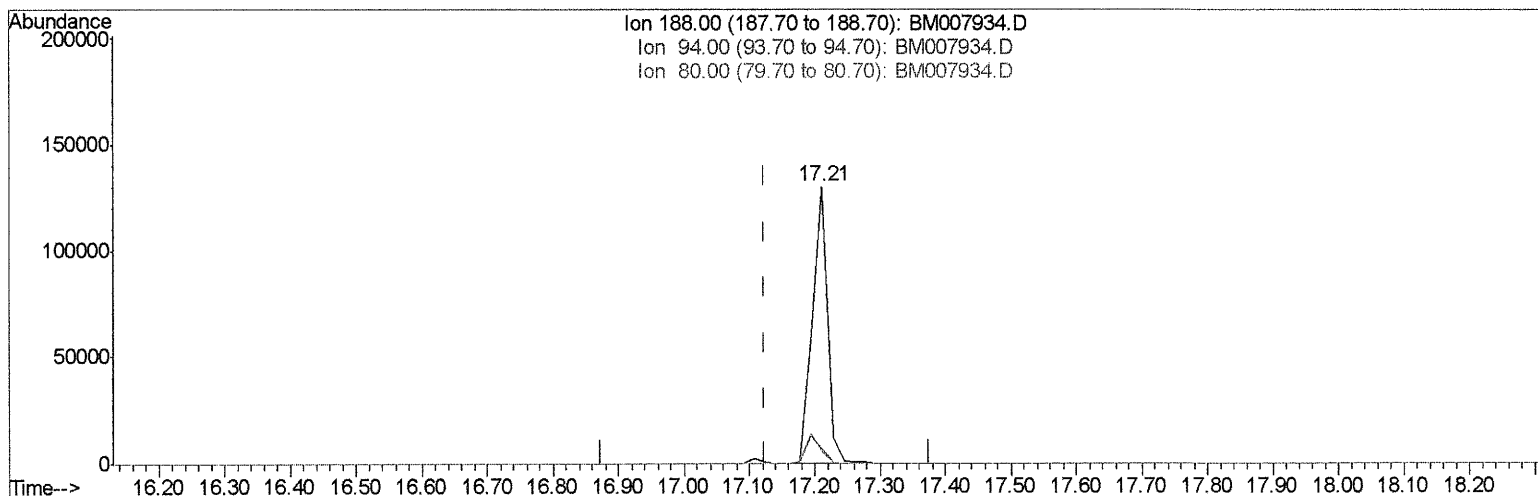

TIC: BM007934.D

(10) Phenanthrene-d10 (I)

17.211min (+0.086) 0.40ng/ul

response 209827

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.64#
80.00	11.80	4.63#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007934.D
Acq On : 16 Nov 2016 22:47
Operator : UM/SJ
Sample : H5622-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WL3

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:59 PM

Quant Time: Nov 17 04:44:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

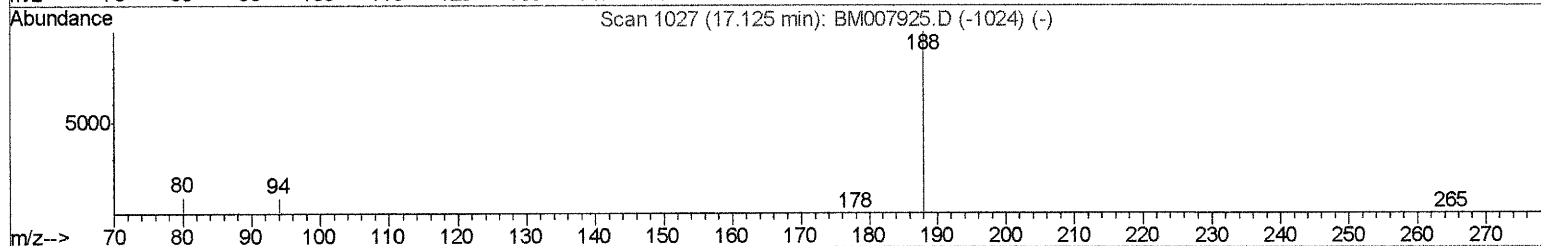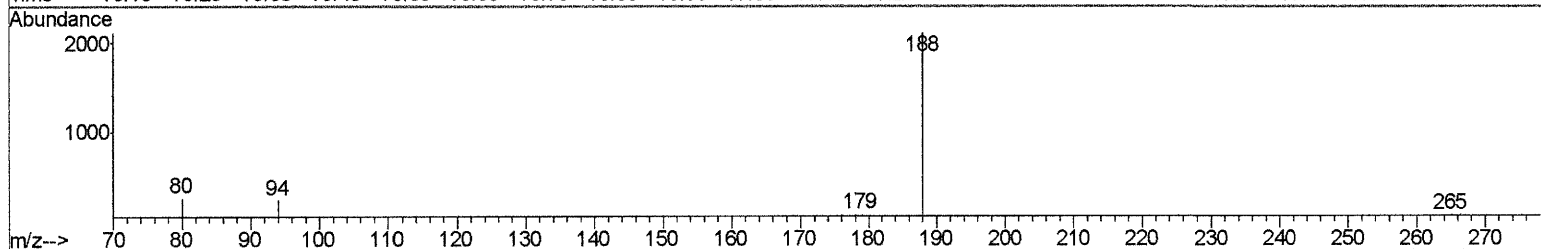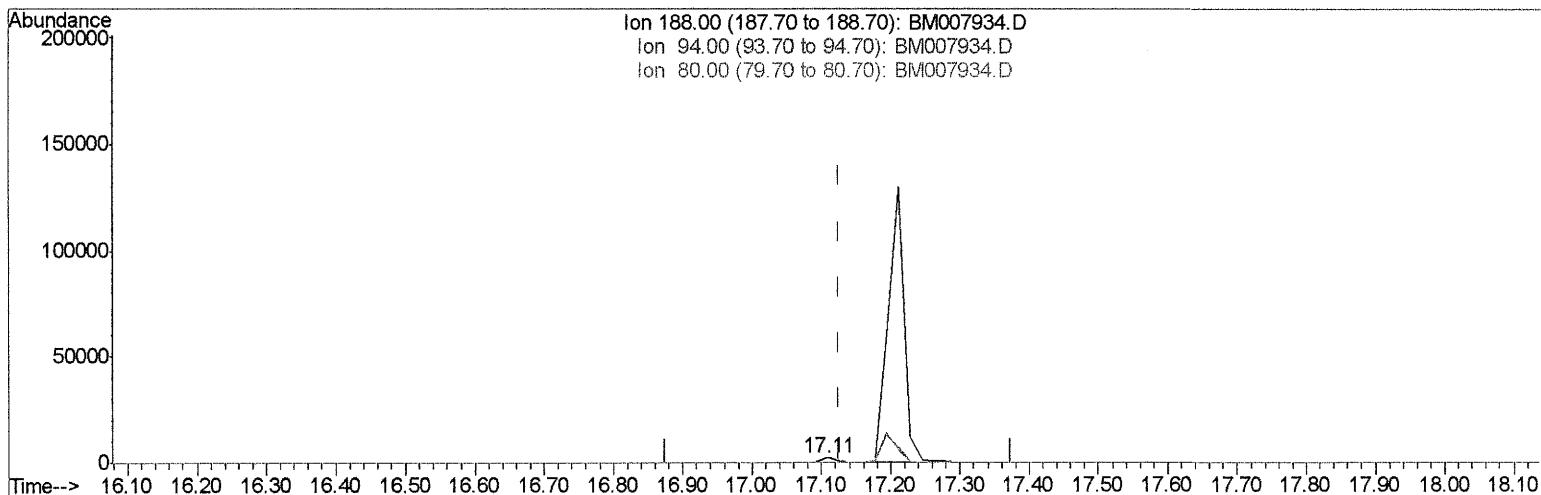

TIC: BM007934.D

(10) Phenanthrene-d10 (I)

17.108min (-0.017) 0.40ng/ul m

response 3198

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.74
80.00	11.80	11.68
0.00	0.00	0.00

UM
11/17/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007934.D
Acq On : 16 Nov 2016 22:47
Operator : UM/SJ
Sample : H5622-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A4WL3

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:59 PM

Quant Time: Nov 17 04:44:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

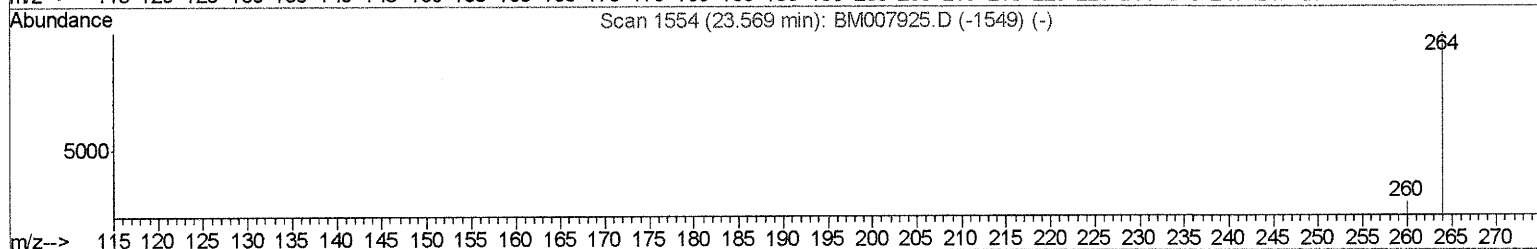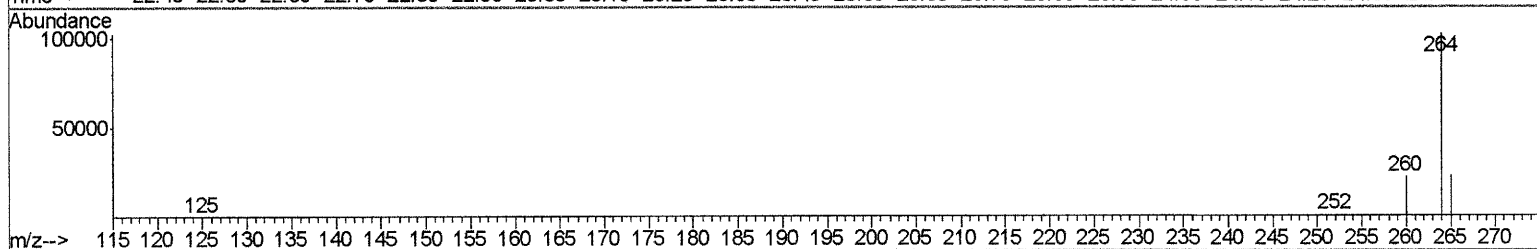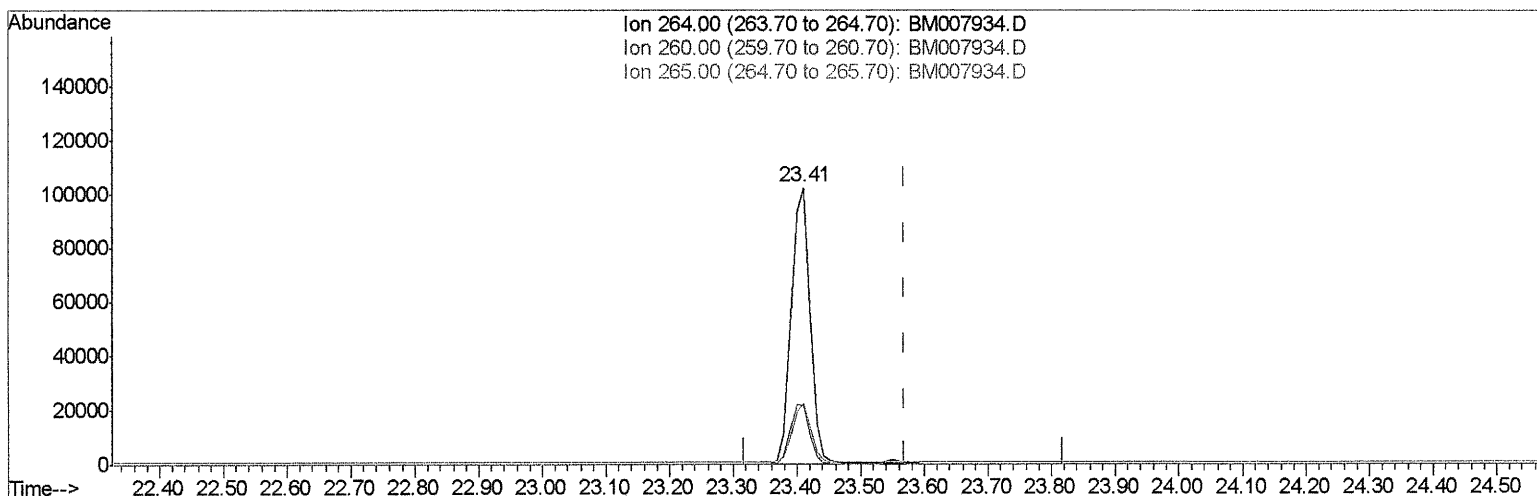

TIC: BM007934.D

(20) Perylene-d12 (I)

23.410min (-0.160) 0.40ng/ul

response 207153

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.21#
265.00	103.50	22.34#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007934.D
 Acq On : 16 Nov 2016 22:47
 Operator : UM/SJ
 Sample : H5622-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 A4WL3

Manual Integrations
 APPROVED

umangi
 11/17/2016 5:55:59 PM

Quant Time: Nov 17 04:44:55 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration

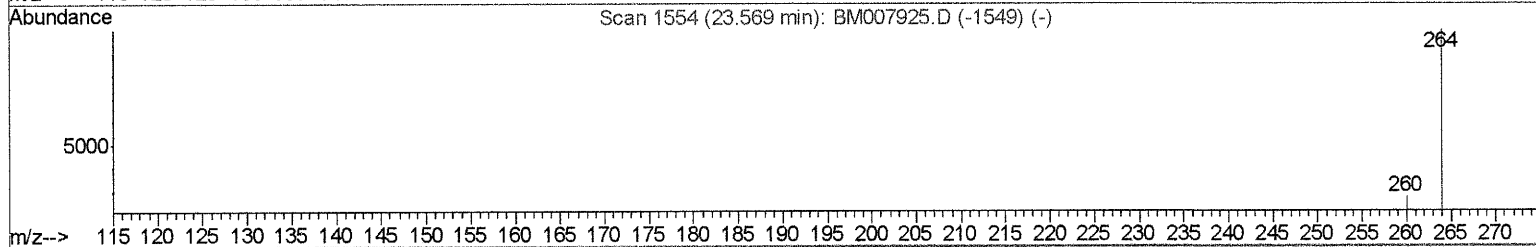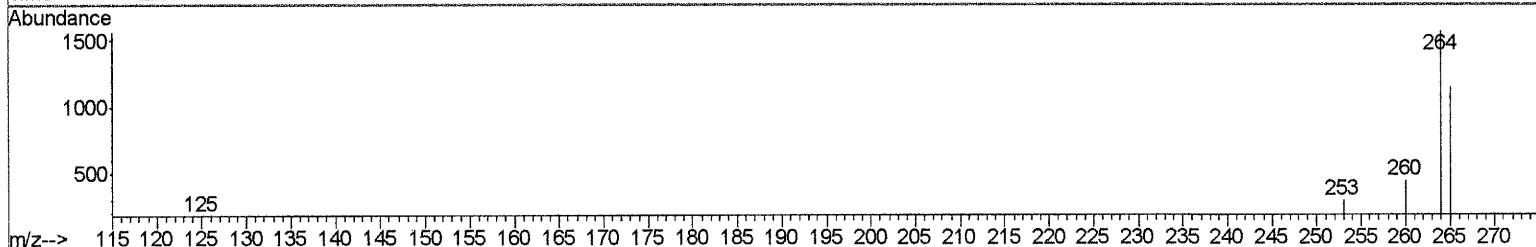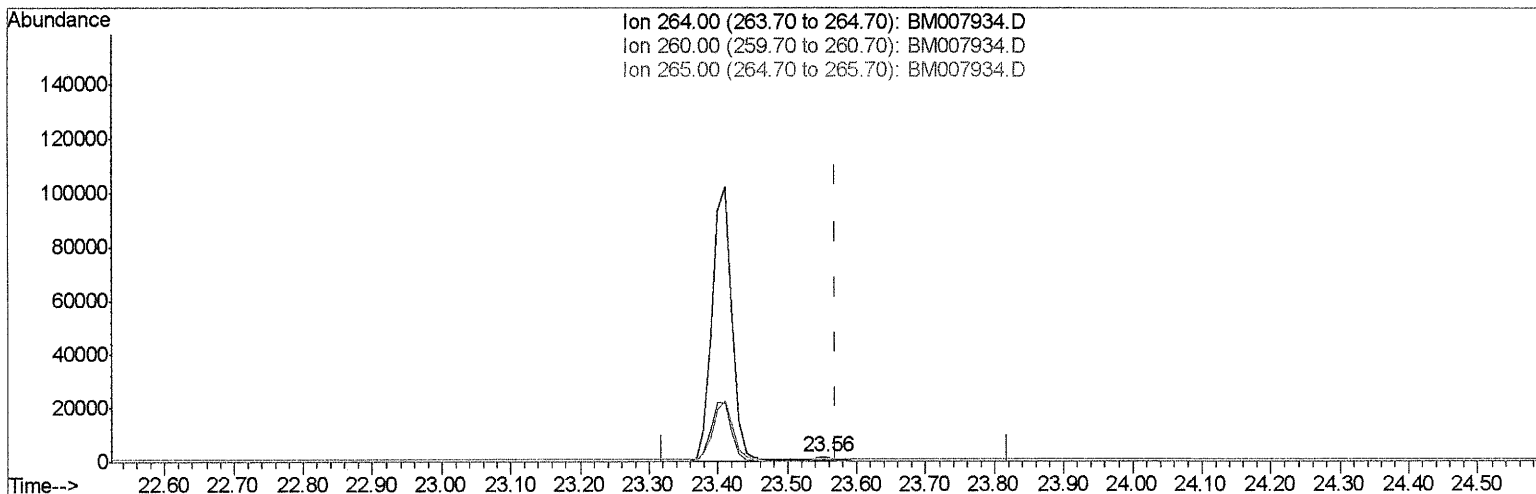

TIC: BM007934.D

(20) Perylene-d12 (I)

23.556min (-0.014) 0.40ng/ul m

response 2747

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	27.92
265.00	103.50	73.35#
0.00	0.00	0.00

um
 11/17/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007934.D
 Acq On : 16 Nov 2016 22:47
 Operator : UM/SJ
 Sample : H5622-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WL3

Manual Integrations
 APPROVED

umangi
 11/17/2016 5:55:59 PM

Quant Time: Nov 17 06:22:39 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 04:42:29 2016
 Response via : Initial Calibration

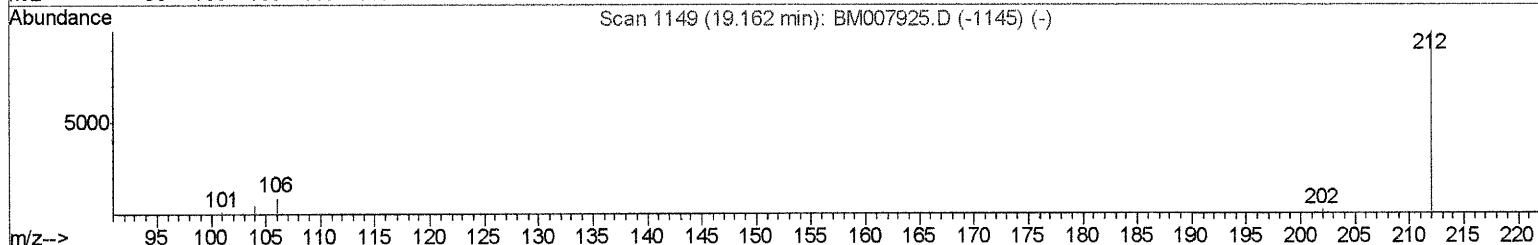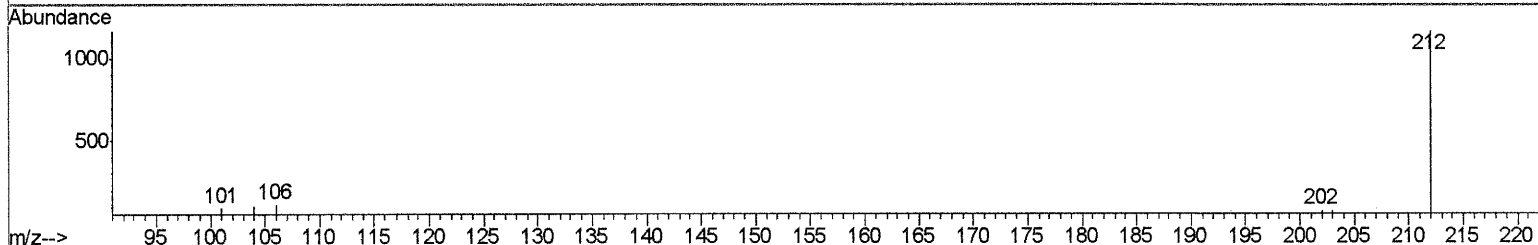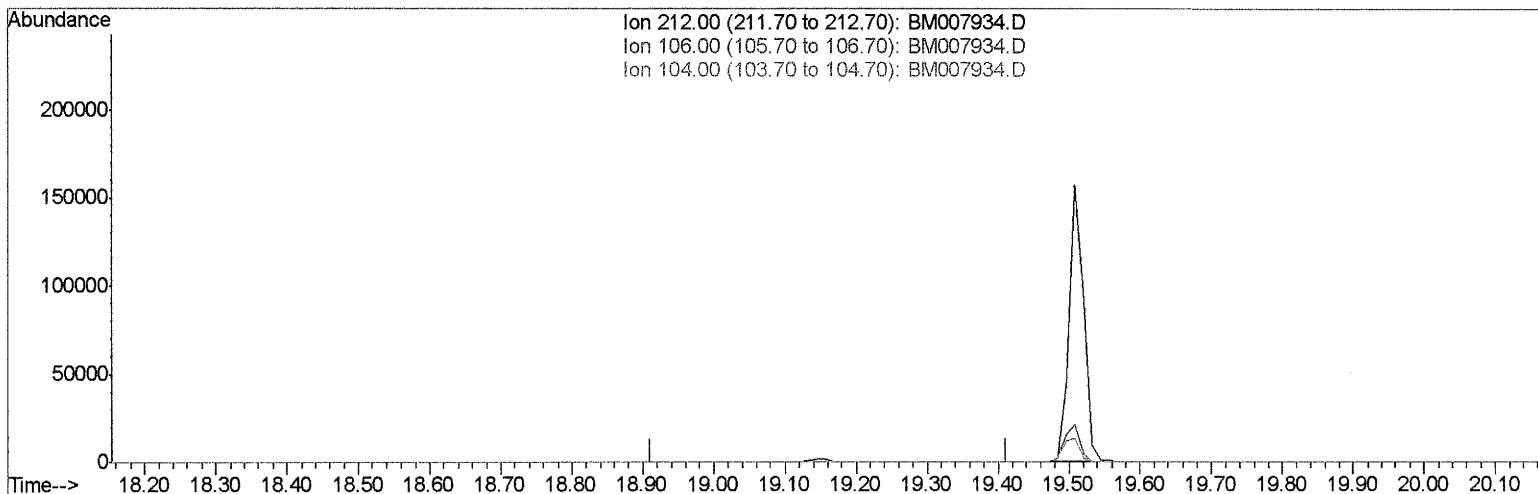

TIC: BM007934.D

(14) Fluoranthene-d10 (SURR)

19.162min (-19.162) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007934.D
Acq On : 16 Nov 2016 22:47
Operator : UM/SJ
Sample : H5622-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A4WL3

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:59 PM

Quant Time: Nov 17 06:22:39 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

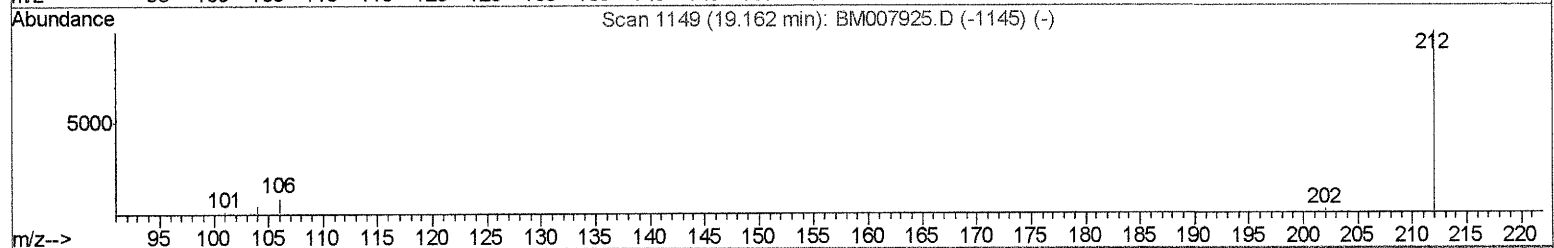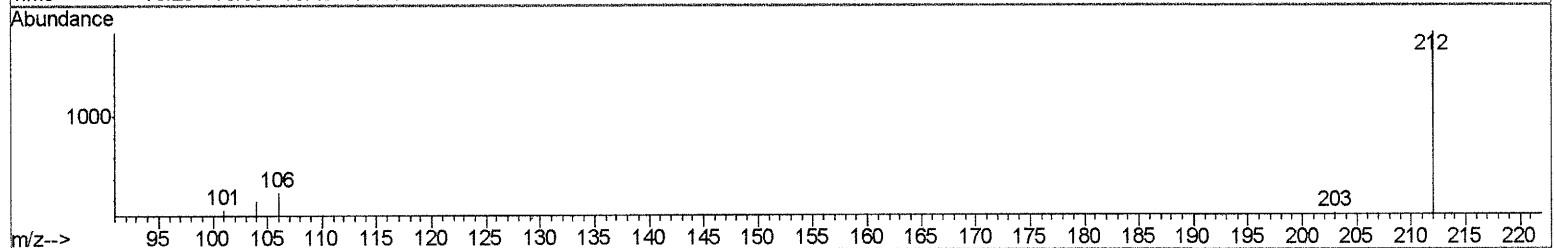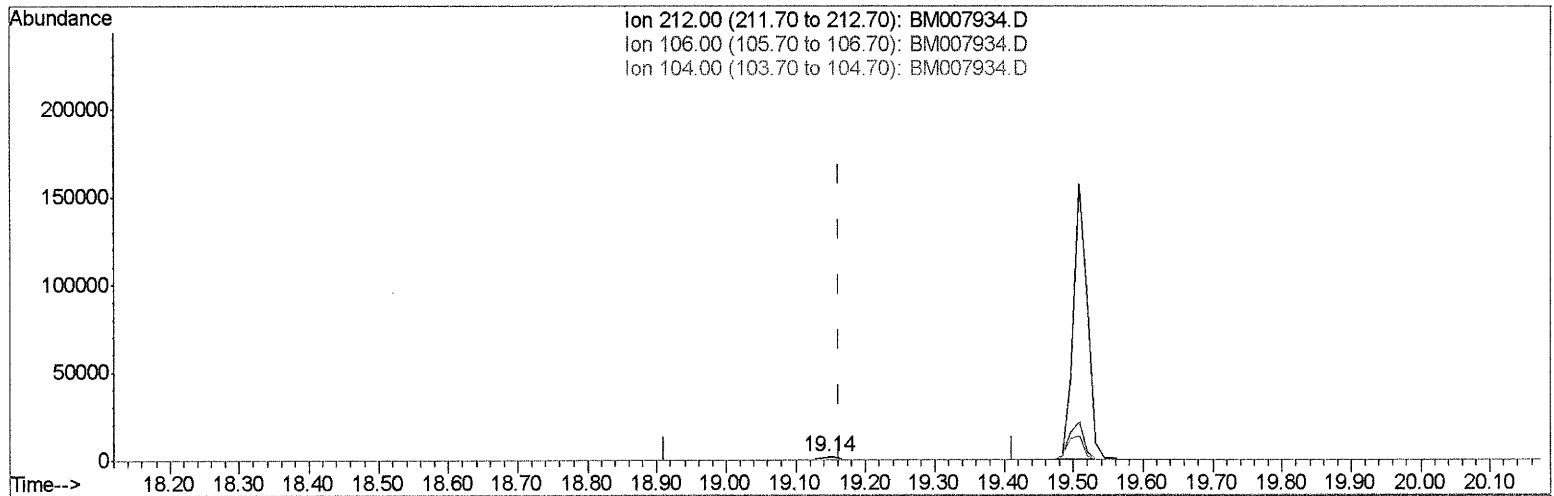

TIC: BM007934.D

(14) Fluoranthene-d10 (SURR)

19.145min (-0.017) 0.38ng/ul m

response 2748

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

um
11/17/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007934.D
Acq On : 16 Nov 2016 22:47
Operator : UM/SJ
Sample : H5622-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WL3

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:59 PM

Quant Time: Nov 17 06:23:18 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 04:42:29 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	865	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.51	136	2765	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.37	164	1644	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	3198m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.30	240	3228	0.40	ng/ul	-0.01
20) Perylene-d12	23.56	264	2747m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	1195	0.36	ng/ul	-0.02
14) Fluoranthene-d10	19.14	212	2748m	0.38	ng/ul	-0.02

} um
11/17/16

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed