

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
 Data File : BM007917.D
 Acq On : 16 Nov 2016 12:45
 Operator : UM/SJ
 Sample : H5622-10MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WK9MS

Manual Integrations
 APPROVED

umangi
 11/17/2016 5:55:14 PM

Quant Time: Nov 17 06:36:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:16:41 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	961	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	3138	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.37	164	1788	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	3577m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.31	240	3380	0.40	ng/ul	0.00
20) Perylene-d12	23.56	264	2875m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1114	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.16	212	2750m	0.34	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.42	153	1682	0.26	ng/ul	91
11) Pentachlorophenol	16.80	266	309	0.37	ng/ul	96
17) Pyrene	19.53	202	4523	0.39	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111616\
Data File : BM007917.D
Acq On : 16 Nov 2016 12:45
Operator : UM/SJ
Sample : H5622-10MS
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4WK9MS

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:14 PM

Quant Time: Nov 17 06:36:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:16:41 2016
Response via : Initial Calibration

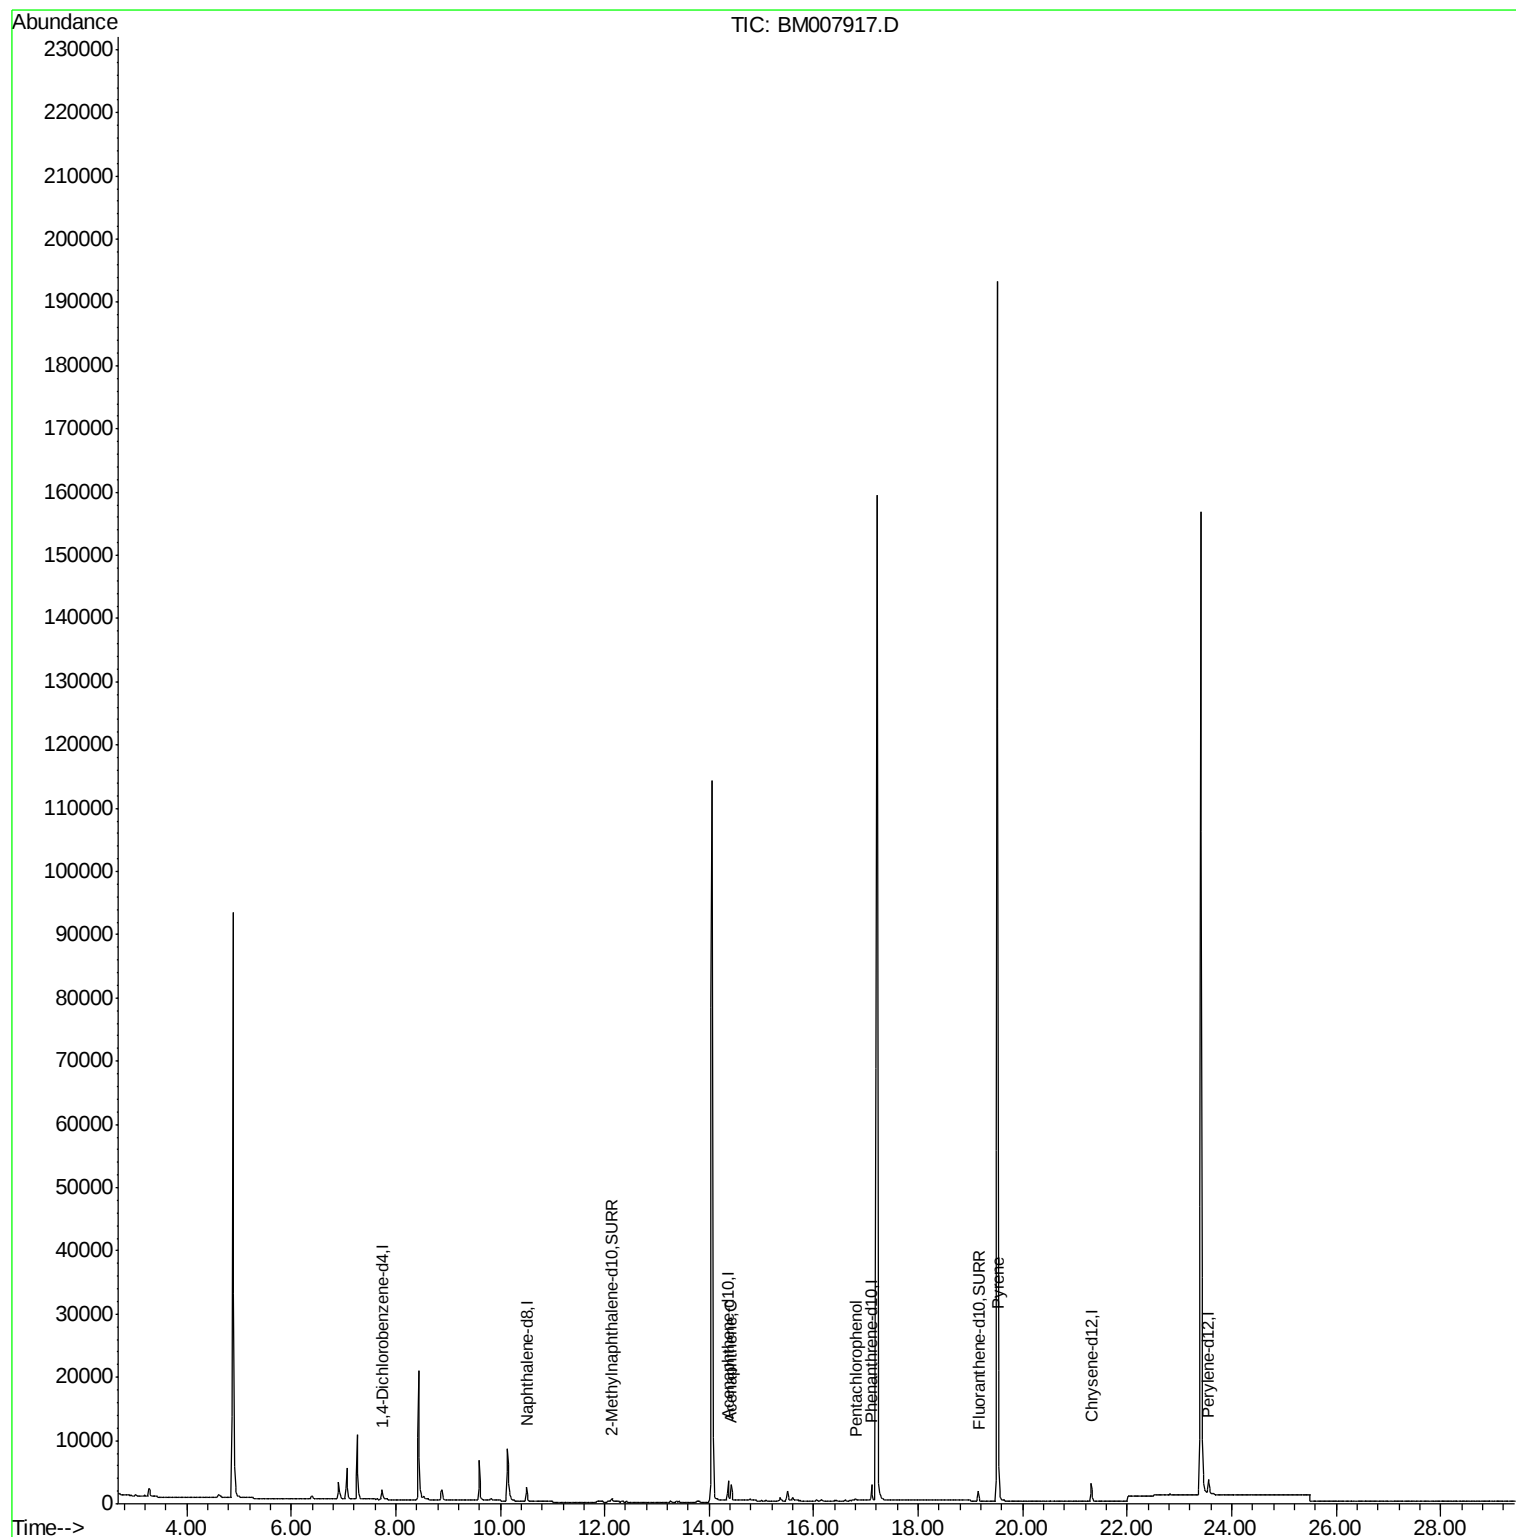

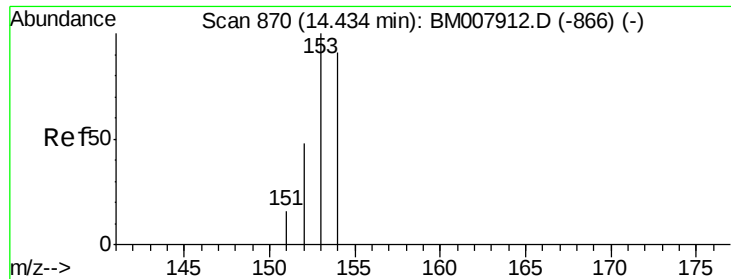

#8

Acenaphthene

Concen: 0.26 ng/ul

RT: 14.42 min Scan# 869

Delta R.T. -0.02 min

Lab File: BM007917.D

Acq: 16 Nov 2016 12:45

Instrument :

BNA_M


ClientSampleId :

A4WK9MS


Tgt Ion:	153	Resp:	1682
Ion Ratio	Lower	Upper	
153	100		
152	54.9	40.3	60.5
154	79.1	71.4	107.2

Manual Integrations
APPROVED



umangi
11/17/2016 5:55:14 PM

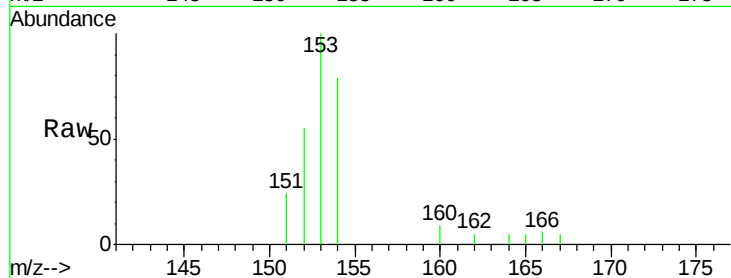

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

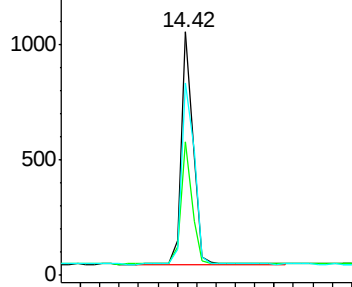

Time-->

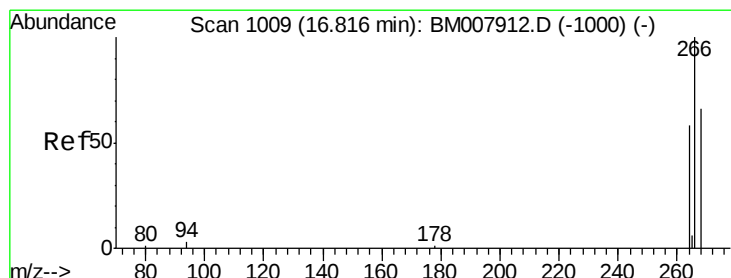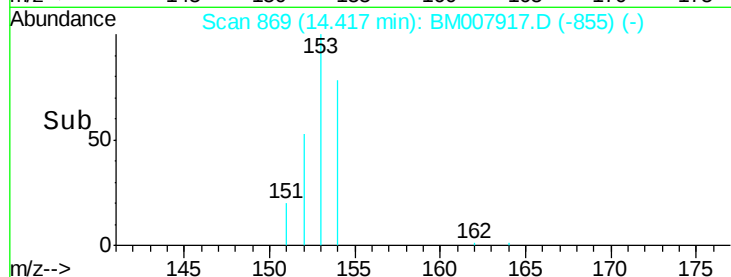

#11

Pentachlorophenol

Concen: 0.37 ng/ul


RT: 16.80 min Scan# 1008

Delta R.T. -0.02 min


Lab File: BM007917.D

Acq: 16 Nov 2016 12:45


Tgt Ion:	266	Resp:	309
Ion Ratio	Lower	Upper	
266	100		
264	63.1	47.9	71.9
268	65.0	49.8	74.8



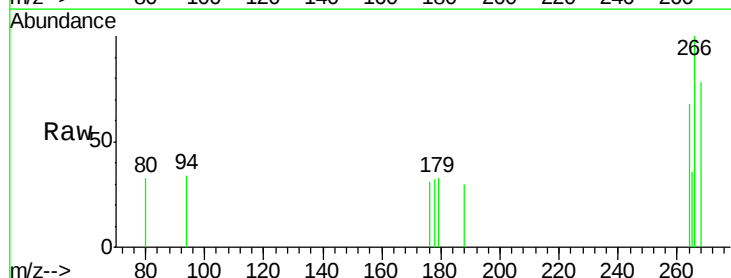


Abundance Ion 266.00 (265.70 to 266.70): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

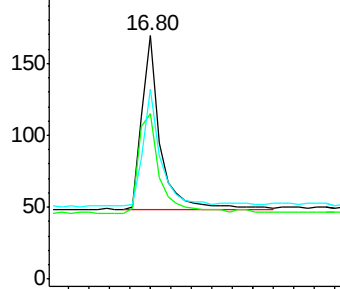

Time-->

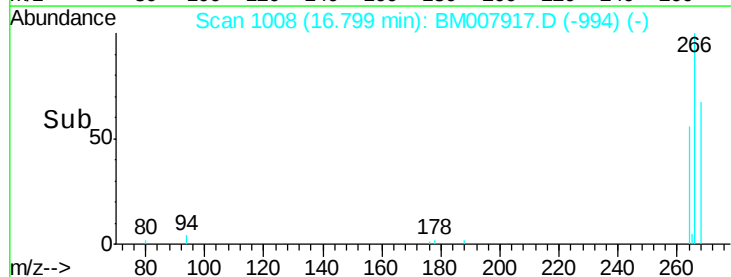

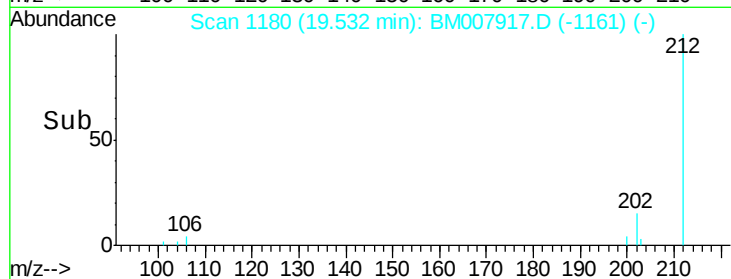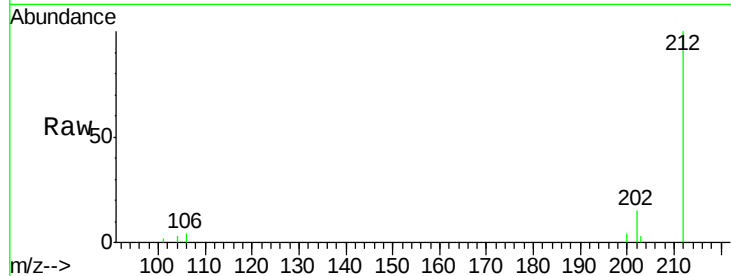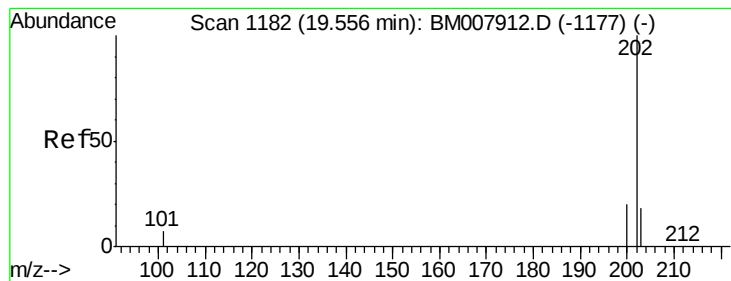

#17

Pyrene

Concen: 0.39 ng/ul

RT: 19.53 min Scan# 1180

Delta R.T. -0.02 min

Lab File: BM007917.D

Acq: 16 Nov 2016 12:45

Tgt Ion:	202	Resp:	4523
Ion Ratio	Lower	Upper	
202	100		
200	25.1	18.2	27.4
203	20.3	15.6	23.4

Instrument :

BNA_M

ClientSampleId :

A4WK9MS

Manual Integrations
APPROVED

umangi
11/17/2016 5:55:14 PM

