

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111617\
 Data File : BM012983.D
 Acq On : 17 Nov 2017 03:36
 Operator : SJ/JU
 Sample : I6361-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE2Q7

Quant Time: Nov 17 05:55:14 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 17 01:17:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	256119	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	984279	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.36	164	562104	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.11	188	1213445	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	1103664	20.00	ng/ul	0.00
83) Perylene-d12	23.53	264	1047677	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	18742	3.39	ng/uL	0.00
5) Phenol-d5	6.89	99	90696	4.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	299598	23.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	341593	19.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	209478	11.53	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	204887	29.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	202039	30.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	405732	23.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	2537	0.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	1379059	27.97	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	1741265	27.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	14805	1.98	ng/ul	0.00
57) Fluorene-d10	15.36	176	1184509	28.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.47	200	143552	27.28	ng/ul	0.00
70) Anthracene-d10	17.21	188	1808217	29.11	ng/ul	0.00
76) Pyrene-d10	19.50	212	1766498	31.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.39	264	1581788	29.77	ng/ul	0.00


Target Compounds					Ovalue
45) 2,6-Dinitrotoluene	13.79	165	8435	1.17	ng/ul# 27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111617\
Data File : BM012983.D
Acq On : 17 Nov 2017 03:36
Operator : SJ/JU
Sample : I6361-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2Q7

Quant Time: Nov 17 05:55:14 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 17 01:17:11 2017
Response via : Initial Calibration

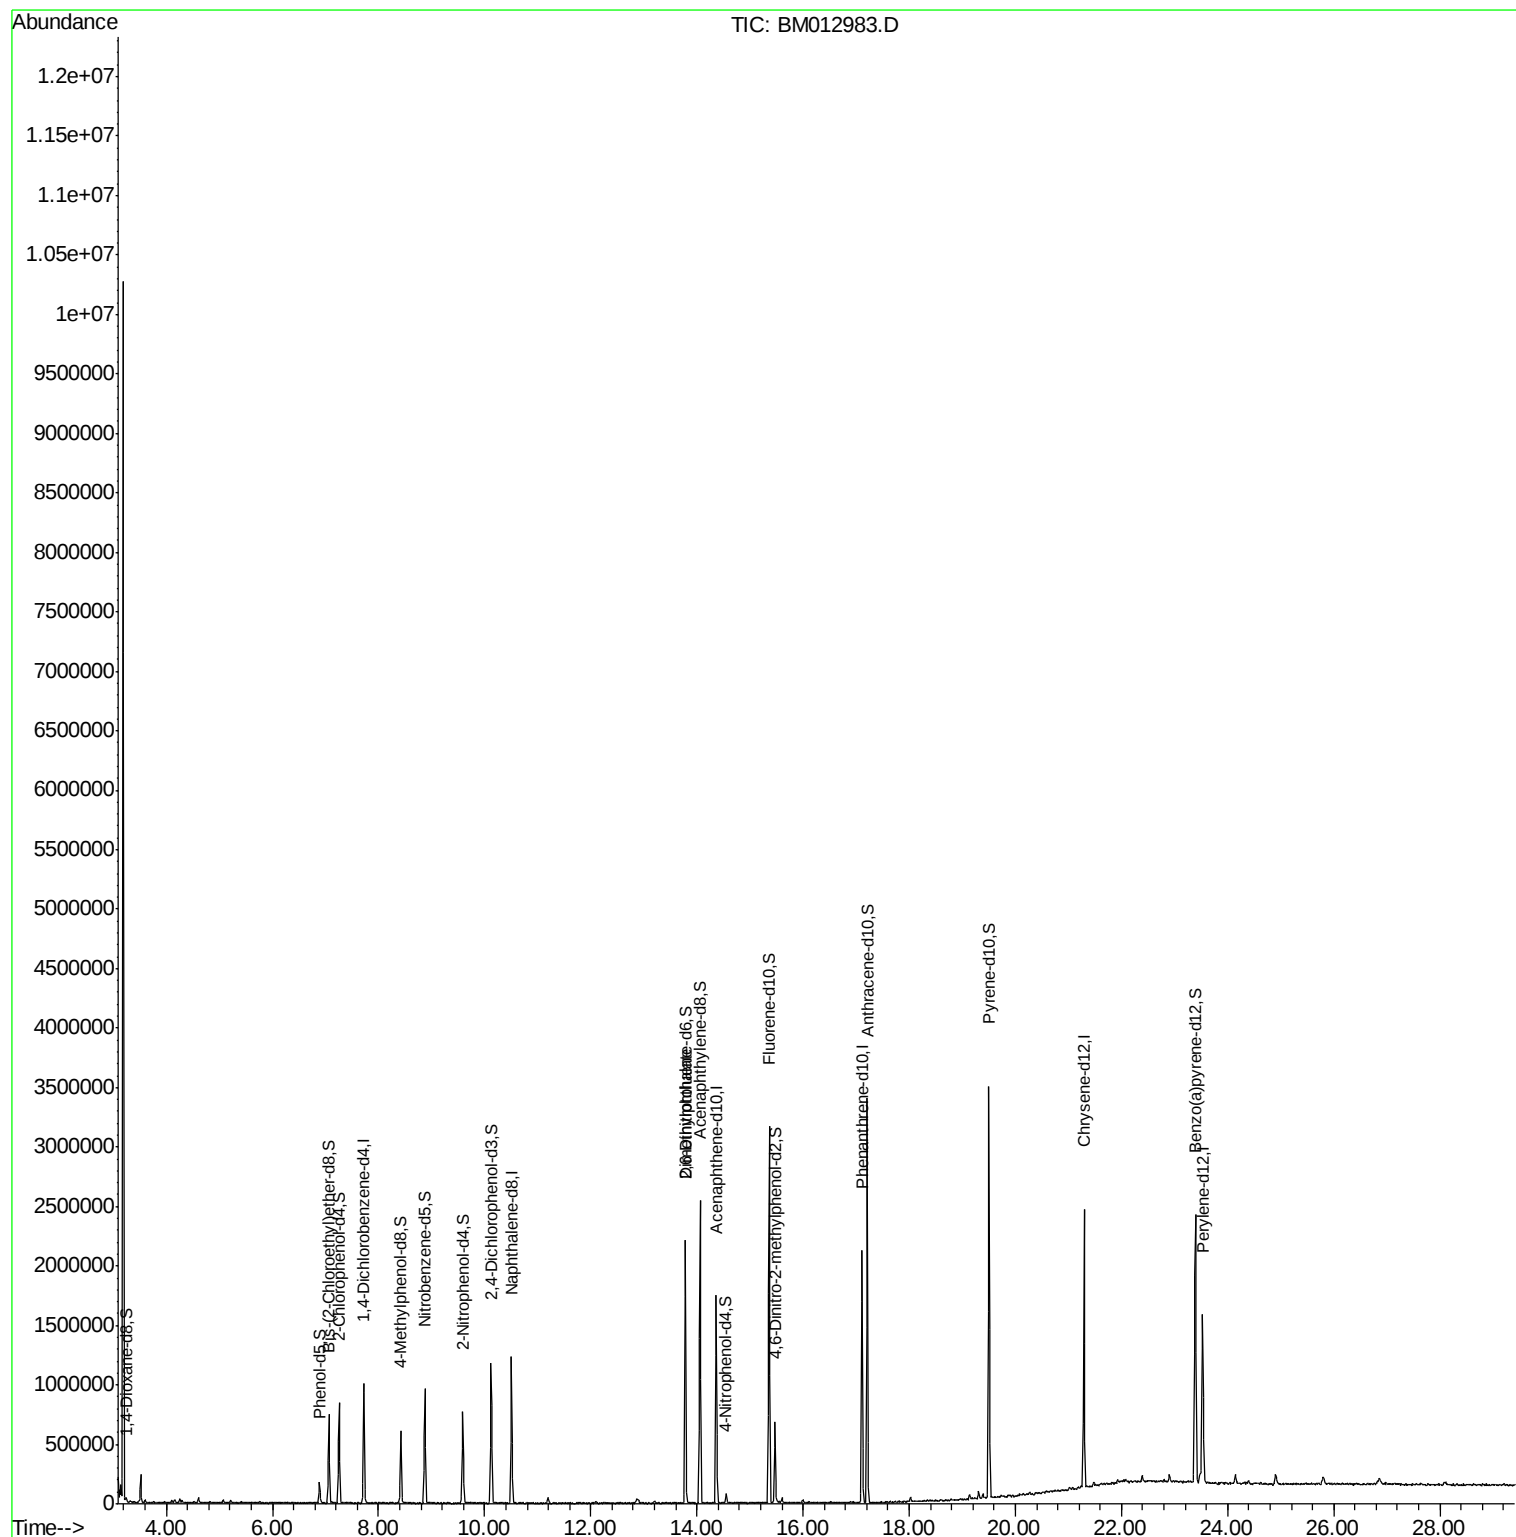

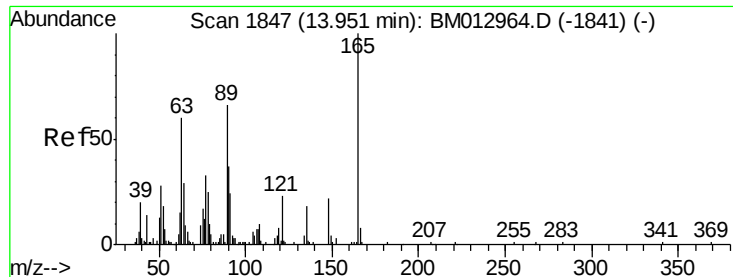

#45

2,6-Dinitrotoluene

Concen: 1.17 ng/ul

RT: 13.79 min Scan# 1819

Delta R.T. -0.16 min

Lab File: BM012983.D

Acq: 17 Nov 2017 03:36

Instrument :

BNA_M

ClientSampleId :

BE2Q7


Tot Ion:165 Resp: 8435

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 35.6 14.6 22.0#

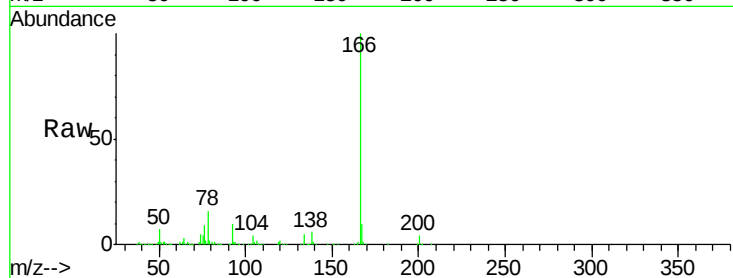

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

