

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111618\
 Data File : BM017675.D
 Acq On : 16 Nov 2018 11:54
 Operator : MJ/SJ
 Sample : PB114851TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB114851TB

Quant Time: Nov 16 13:33:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 12 18:37:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	172173	20.00	ng	0.00
21) Naphthalene-d8	10.39	136	633212	20.00	ng	0.00
39) Acenaphthene-d10	14.26	164	359965	20.00	ng	0.00
64) Phenanthrene-d10	17.01	188	823423	20.00	ng	0.00
76) Chrysene-d12	21.22	240	805424	20.00	ng	0.00
87) Perylene-d12	23.41	264	682794	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	1315793	128.97	ng	0.00
7) Phenol-d6	6.80	99	1705857	119.72	ng	0.00
23) Nitrobenzene-d5	8.76	82	1054299	85.96	ng	-0.01
42) 2,4,6-Tribromophenol	15.76	330	613770	118.67	ng	0.00
45) 2-Fluorobiphenyl	12.87	172	2385482	85.97	ng	0.00
79) Terphenyl-d14	19.66	244	3676137	103.44	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111618\
Data File : BM017675.D
Acq On : 16 Nov 2018 11:54
Operator : MJ/SJ
Sample : PB114851TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114851TB

Quant Time: Nov 16 13:33:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

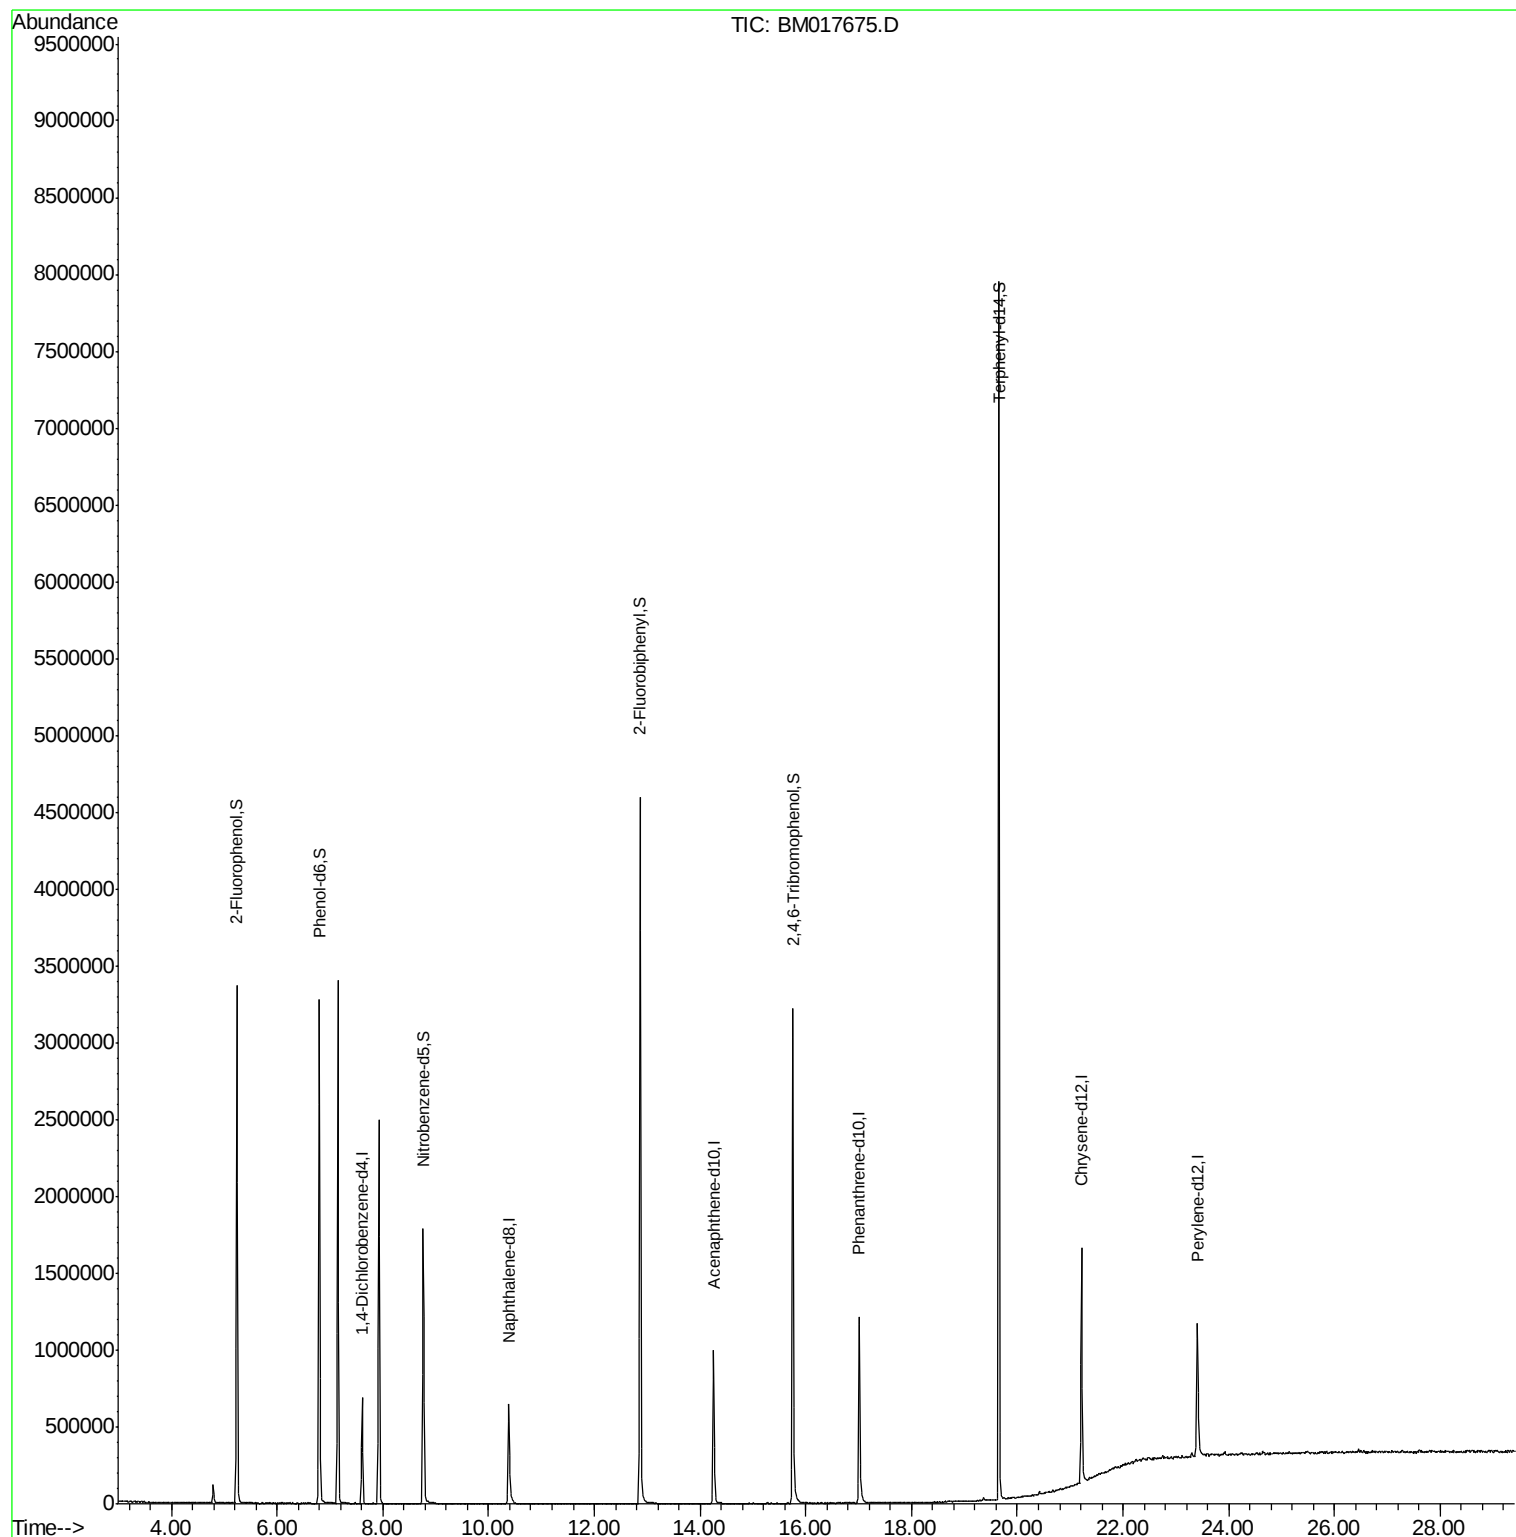

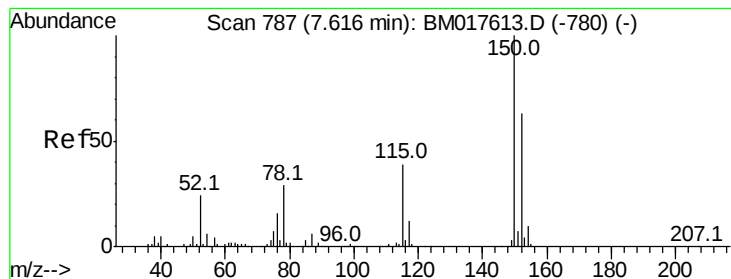


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.61 min Scan# 786
Delta R.T. -0.01 min
Lab File: BM017675.D
Acq: 16 Nov 2018 11:54

Instrument :
BNA_M
ClientSampleId :
PB114851TB

Tot Ion	Ratio	Lower	Upper
152	100		
150	152.6	126.4	189.6
115	62.4	49.4	74.0



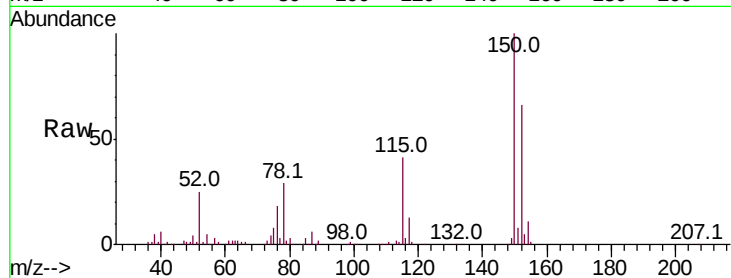


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

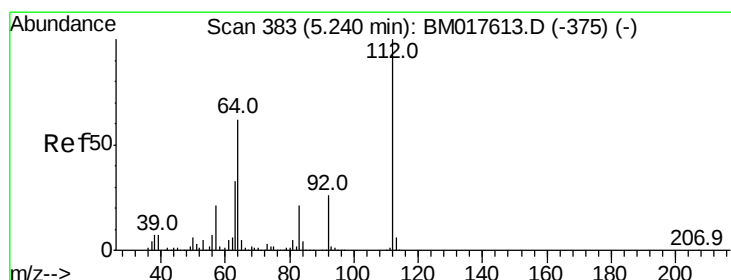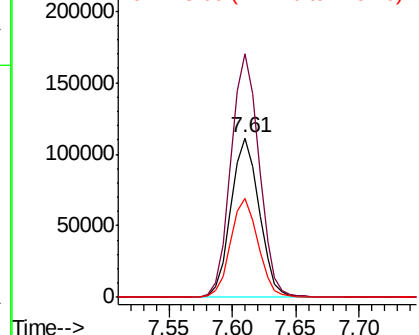

#5

2-Fluorophenol
Concen: 128.975 ng
RT: 5.23 min Scan# 382
Delta R.T. -0.01 min
Lab File: BM017675.D
Acq: 16 Nov 2018 11:54

Tgt Ion	Ratio	Lower	Upper
112	100		
64	62.0	49.3	73.9
63	33.8	26.2	39.4


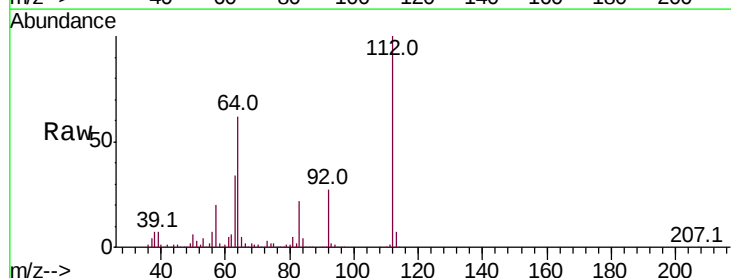



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

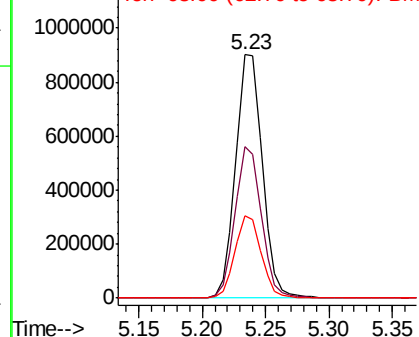



#7

Phenol-d6

Concen: 119.722 ng

RT: 6.80 min Scan# 648

Delta R.T. -0.01 min

Lab File: BM017675.D

Acq: 16 Nov 2018 11:54

Instrument :


BNA_M

ClientSampleId :

PB114851TB

Tot Ion: 99 Resp: 1705857

Ion	Ratio	Lower	Upper
99	100		
42	20.0	16.3	24.5
71	38.8	29.8	44.8



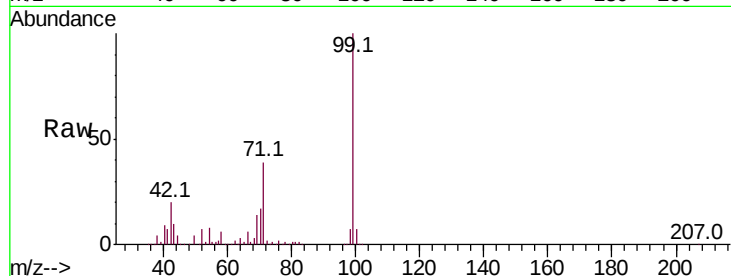


Abundance

Ion 99.00 (98.70 to 99.70): BM017613.D (-641) (-)

Ion 42.00 (41.70 to 42.70): BM017613.D (-641) (-)

Ion 71.00 (70.70 to 71.70): BM017613.D (-641) (-)

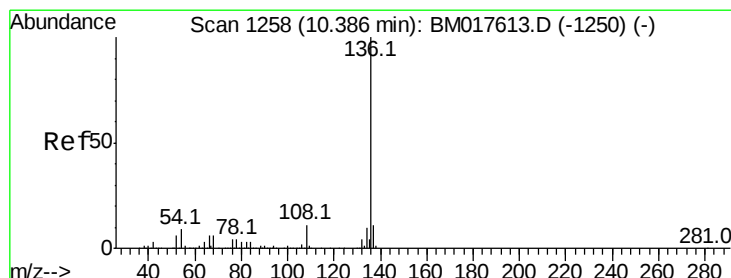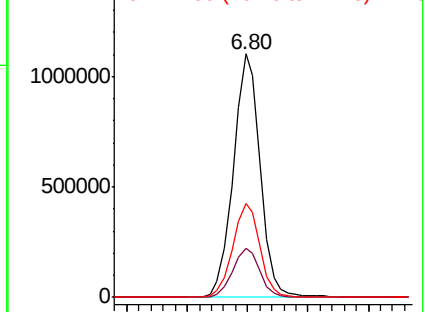

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.39 min Scan# 1258


Delta R.T. -0.00 min

Lab File: BM017675.D

Acq: 16 Nov 2018 11:54

Tgt Ion: 136 Resp: 633212

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.6	12.8
54	8.4	7.0	10.6
68	5.4	4.9	7.3

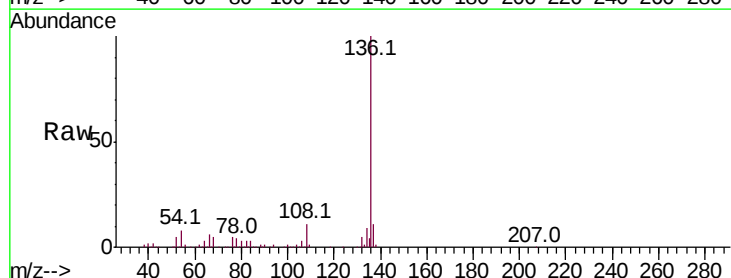



Abundance

Ion 136.00 (135.70 to 136.70): BM017613.D (-1250) (-)

Ion 137.00 (136.70 to 137.70): BM017613.D (-1250) (-)

Ion 54.00 (53.70 to 54.70): BM017613.D (-1250) (-)

Ion 68.00 (67.70 to 68.70): BM017613.D (-1250) (-)


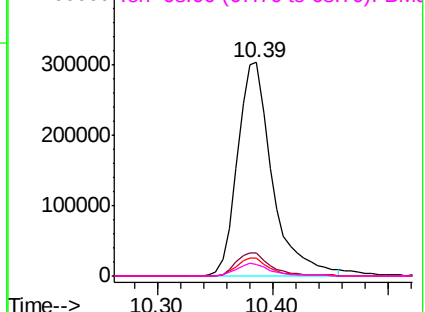





#23
Nitrobenzene-d5
Concen: 85.956 ng
RT: 8.76 min Scan# 982
Delta R.T. -0.01 min
Lab File: BM017675.D
Acq: 16 Nov 2018 11:54




Instrument :
BNA_M
ClientSampleId :
PB114851TB


Tot Ion: 82 Resp: 1054299
Ion Ratio Lower Upper
82 100
128 40.2 33.0 49.4
54 52.2 41.4 62.2

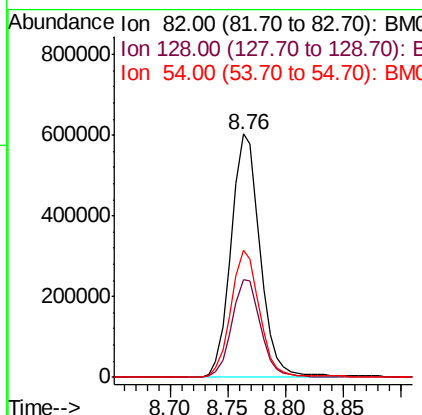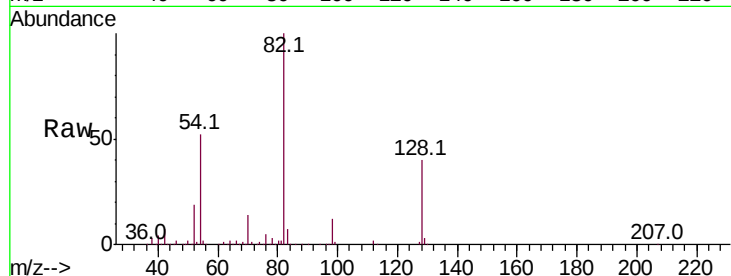

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.26 min Scan# 1916
Delta R.T. -0.01 min
Lab File: BM017675.D
Acq: 16 Nov 2018 11:54

Tgt Ion:164 Resp: 359965
Ion Ratio Lower Upper
164 100
162 100.7 81.4 122.0
160 48.3 35.6 53.4

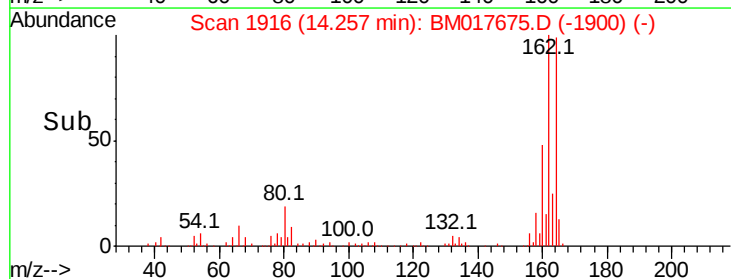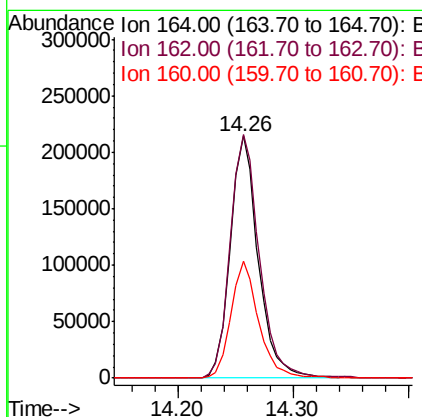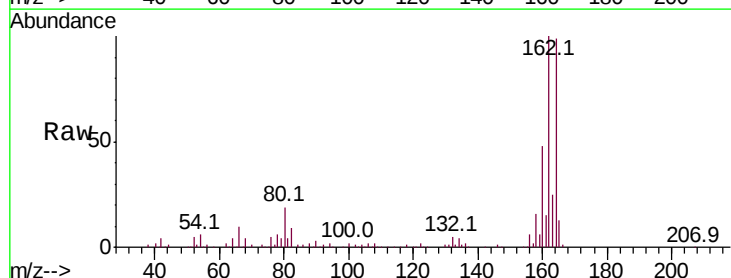


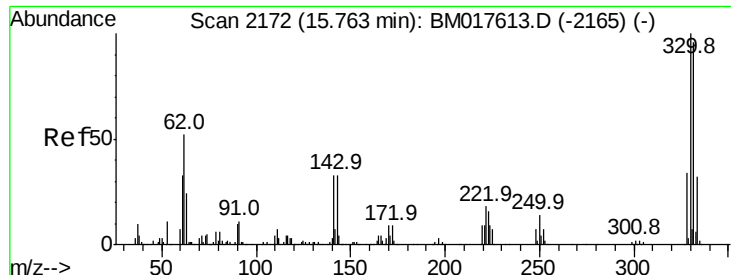




#42
 2,4,6-Tribromophenol
 Concen: 118.667 ng
 RT: 15.76 min Scan# 2171
 Delta R.T. -0.01 min
 Lab File: BM017675.D
 Acq: 16 Nov 2018 11:54

Instrument :
 BNA_M
 ClientSampleId :
 PB114851TB

Tot Ion:330 Resp: 613770
 Ion Ratio Lower Upper
 330 100
 332 97.5 77.9 116.9
 141 37.6 27.5 41.3

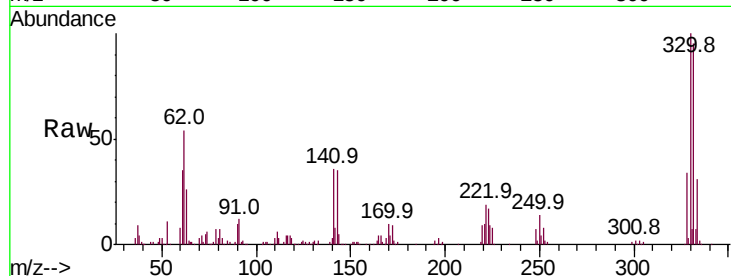


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

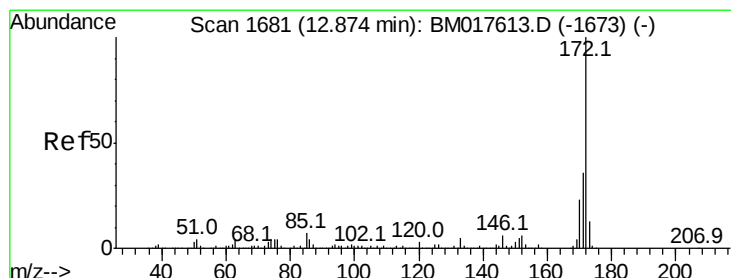
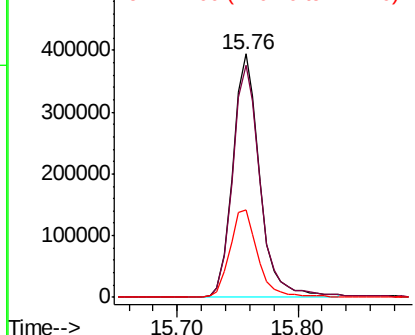



#45
 2-Fluorobiphenyl
 Concen: 85.974 ng
 RT: 12.87 min Scan# 1680
 Delta R.T. -0.01 min
 Lab File: BM017675.D
 Acq: 16 Nov 2018 11:54

Tgt Ion:172 Resp: 2385482
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.7 43.1
 170 23.1 18.3 27.5

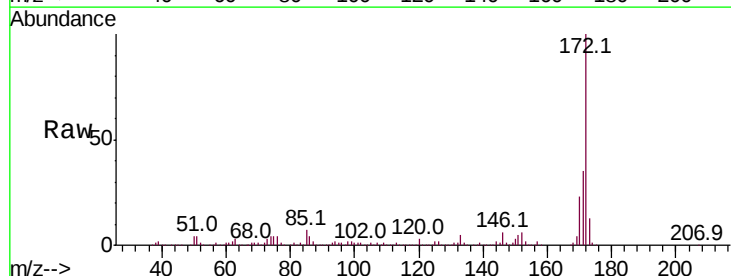

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




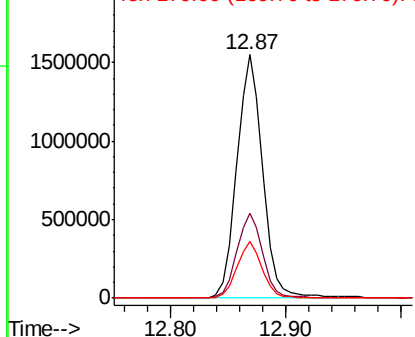


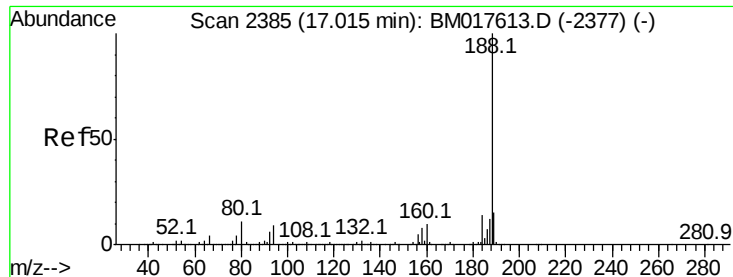

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.01 min Scan# 2384
Delta R.T. -0.01 min
Lab File: BM017675.D
Acq: 16 Nov 2018 11:54




Instrument :
BNA_M
ClientSampleId :
PB114851TB


Tot Ion:188 Resp: 823423
Ion Ratio Lower Upper
188 100
94 8.9 7.5 11.3
80 10.1 8.6 13.0

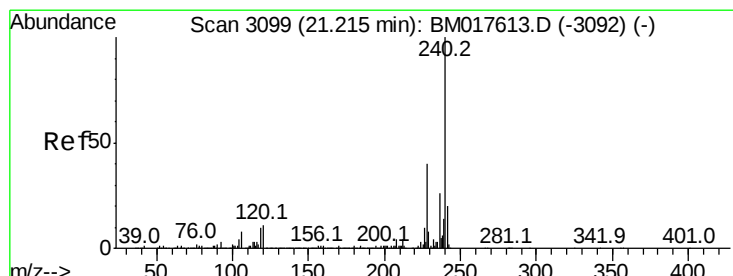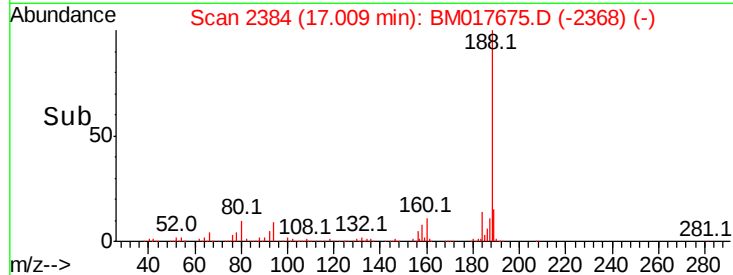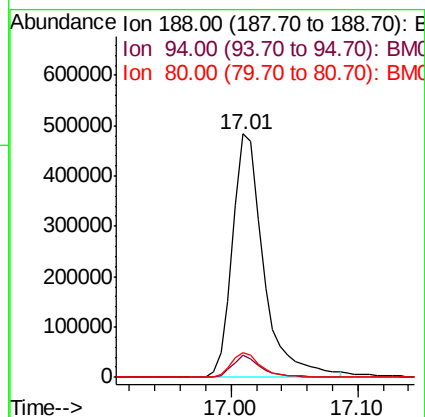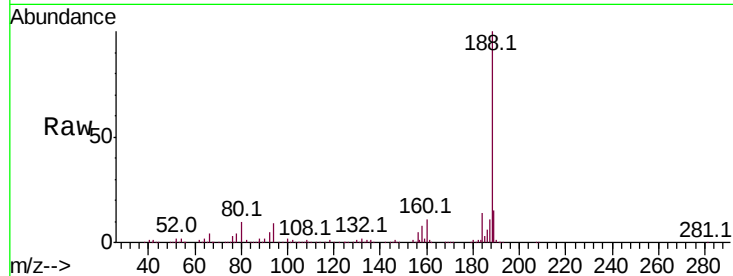

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.22 min Scan# 3099
Delta R.T. -0.00 min
Lab File: BM017675.D
Acq: 16 Nov 2018 11:54

Tgt Ion:240 Resp: 805424
Ion Ratio Lower Upper
240 100
120 9.4 8.5 12.7
236 24.9 20.4 30.6

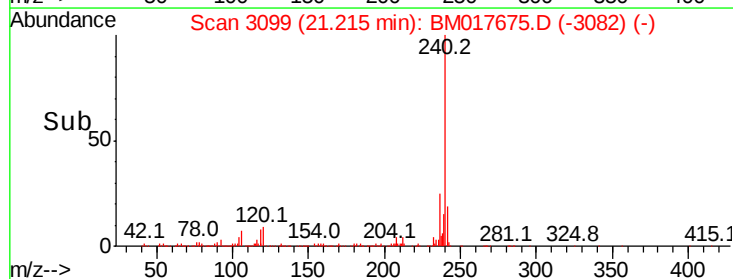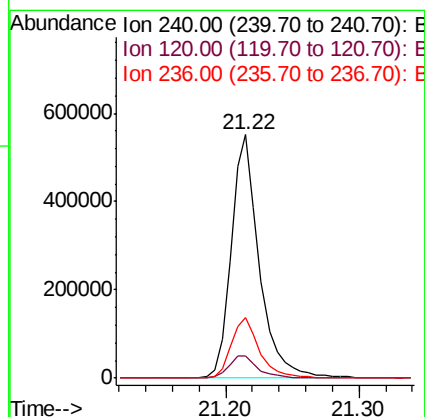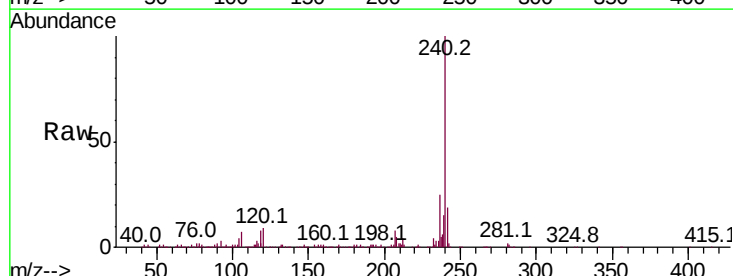



#79

Terphenyl-d14

Concen: 103.445 ng

RT: 19.66 min Scan# 2834

Delta R.T. -0.00 min

Lab File: BM017675.D

Acq: 16 Nov 2018 11:54

Instrument :

BNA_M

ClientSampleId :

PB114851TB


Tot Ion:244 Resp: 3676137

Ion Ratio Lower Upper

244 100

212 7.4 5.8 8.6




122 9.4 9.0 13.6

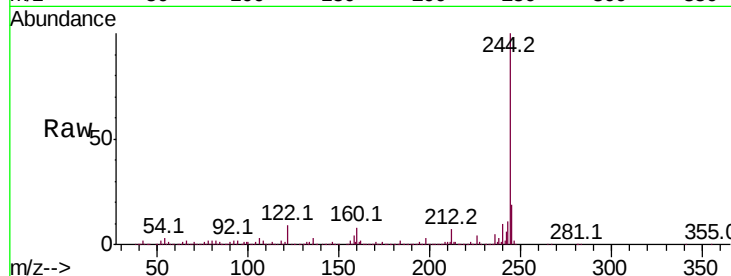

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

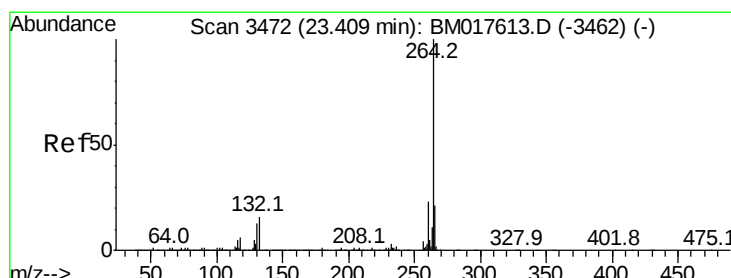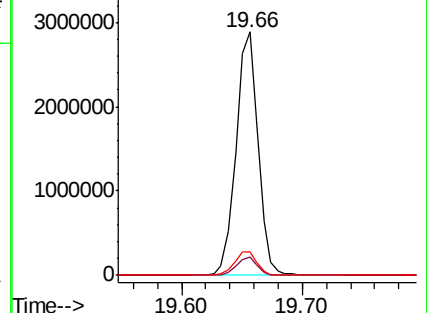

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.41 min Scan# 3472

Delta R.T. -0.00 min

Lab File: BM017675.D

Acq: 16 Nov 2018 11:54


Tgt Ion:264 Resp: 682794

Ion Ratio Lower Upper

264 100

260 22.8 18.2 27.2

265 23.2 17.5 26.3

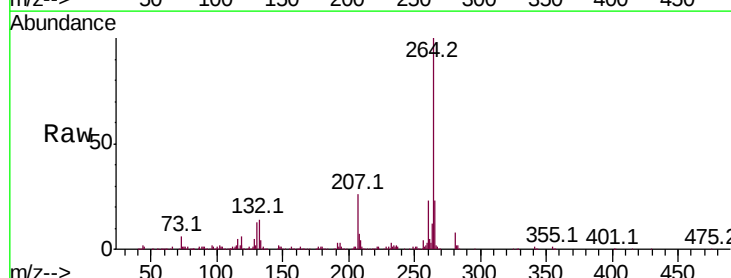

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

