


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111618\
 Data File : BM017671.D
 Acq On : 16 Nov 2018 09:30
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

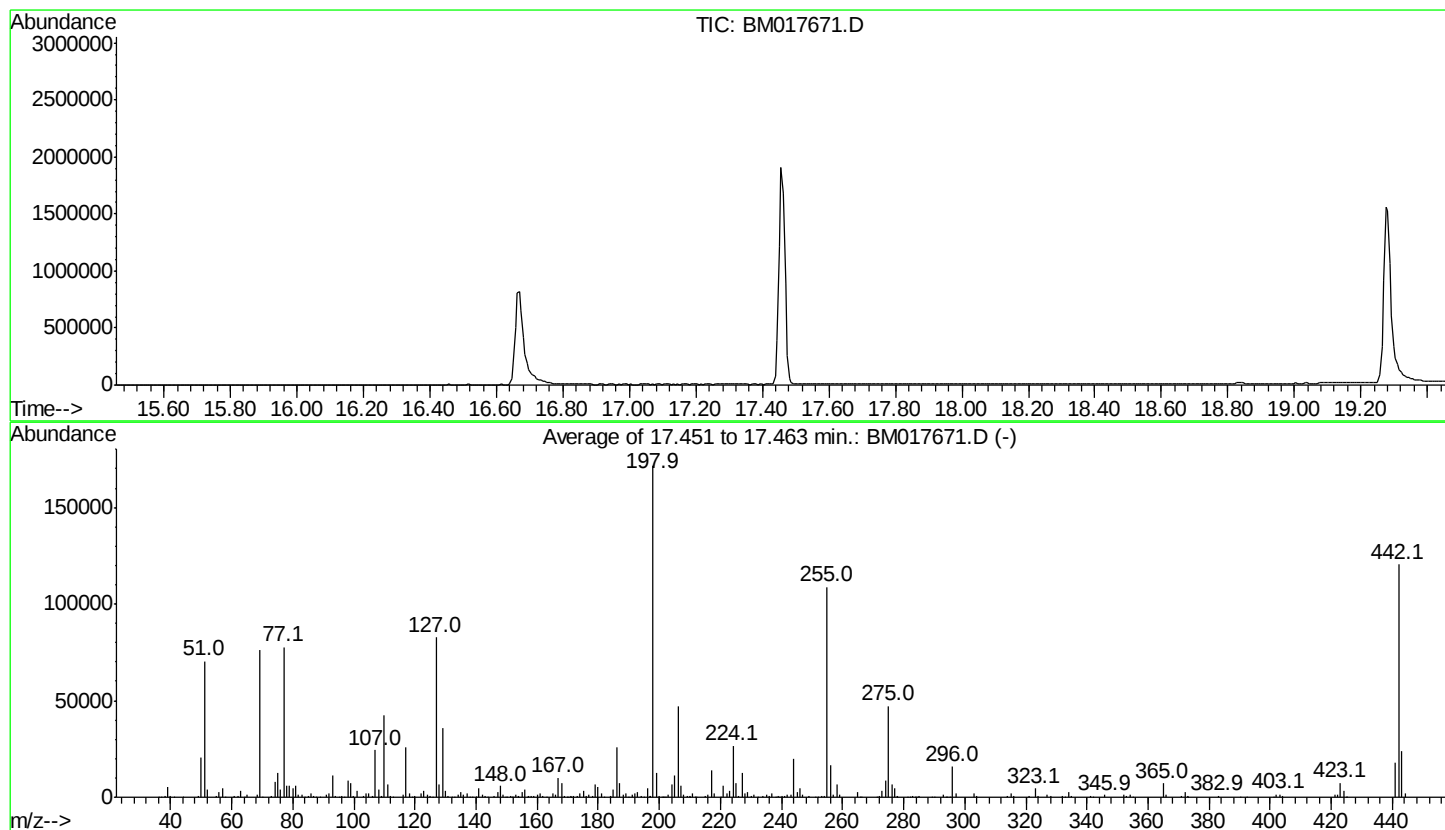

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	70296	PASS
68	69	0.00	2	1.8	1341	PASS
69	198	0.00	100	44.4	76234	PASS
70	69	0.00	2	0.3	251	PASS
127	198	10	80	48.1	82522	PASS
197	198	0.00	2	0.5	783	PASS
198	198	100	100	100.0	171629	PASS
199	198	5	9	7.2	12286	PASS
275	198	10	60	27.4	47106	PASS
365	198	1	100	4.1	7018	PASS
441	198	0.01	100	10.4	17768	PASS
442	198	50	100	70.2	120514	PASS
443	442	15	24	19.7	23699	PASS