
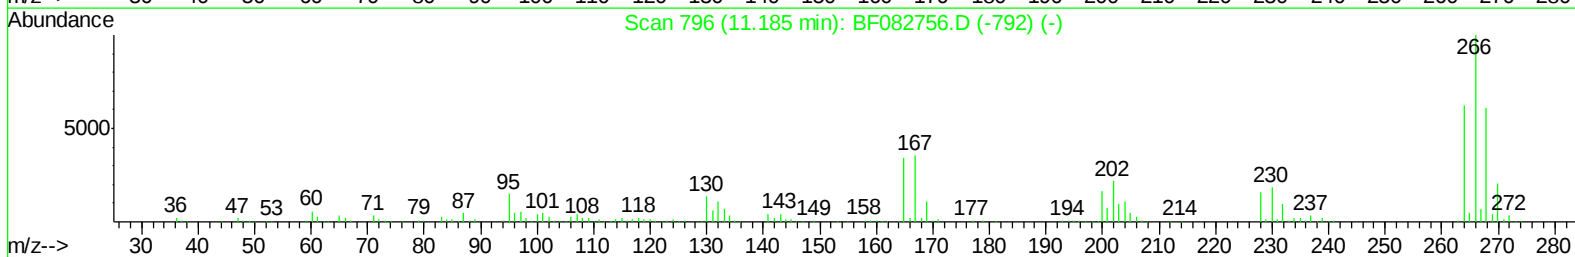
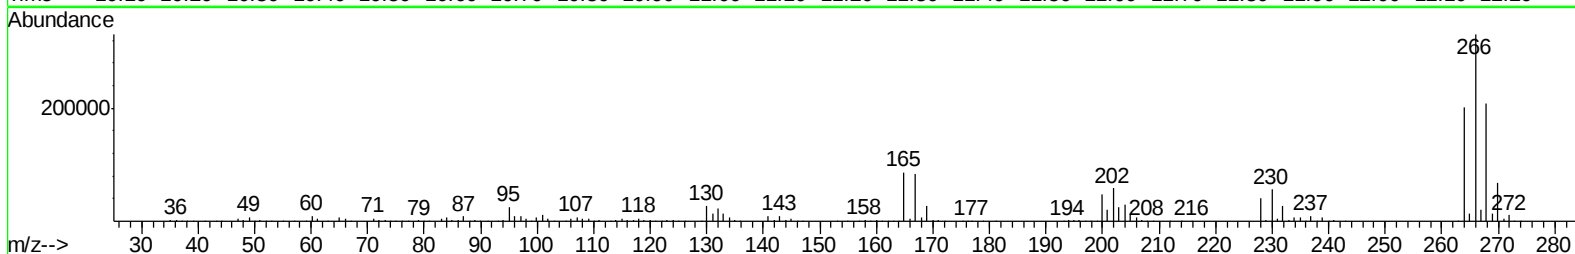


Data Path : Z:\HPCHEM1\BNA F\Data\BF111615\
Data File : BF082940.D
Acq On : 16 Nov 2015 13:22
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 08:10:01 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 17 04:41:30 2015
Response via : Initial Calibration

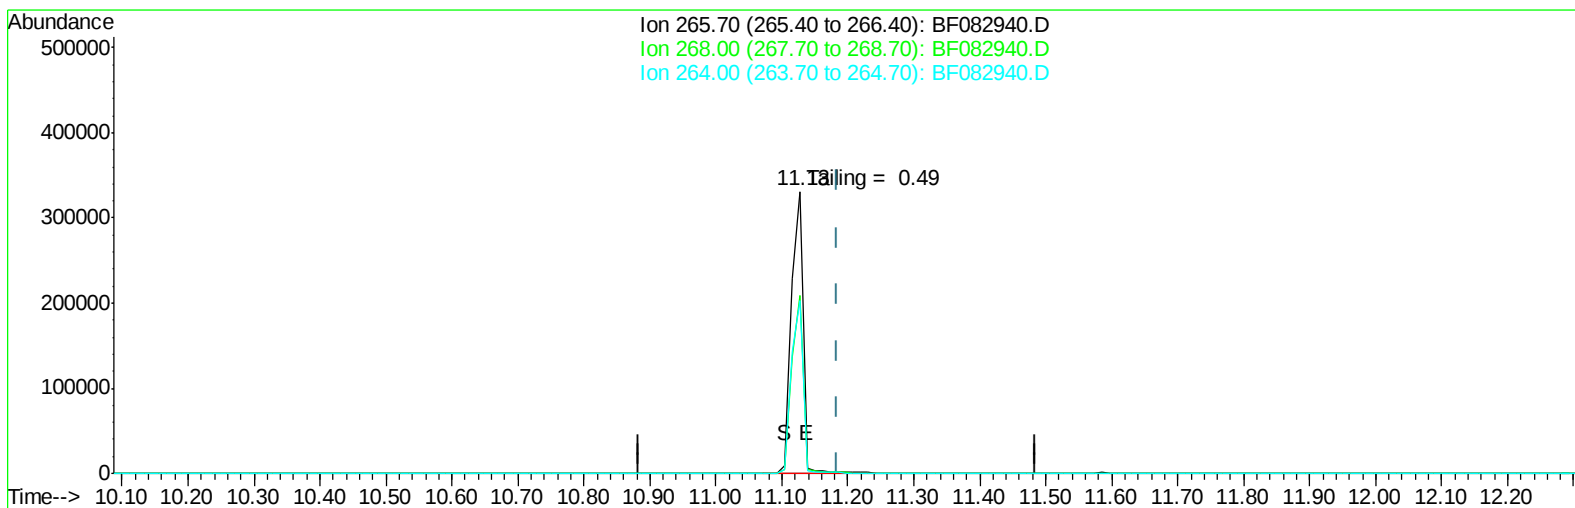

TIC: BF082940.D

(69) Pentachlorophenol (C)

11.128min (-0.057) 10594.52ng

response 405851

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	63.32
264.00	63.20	61.16
0.00	0.00	0.00