
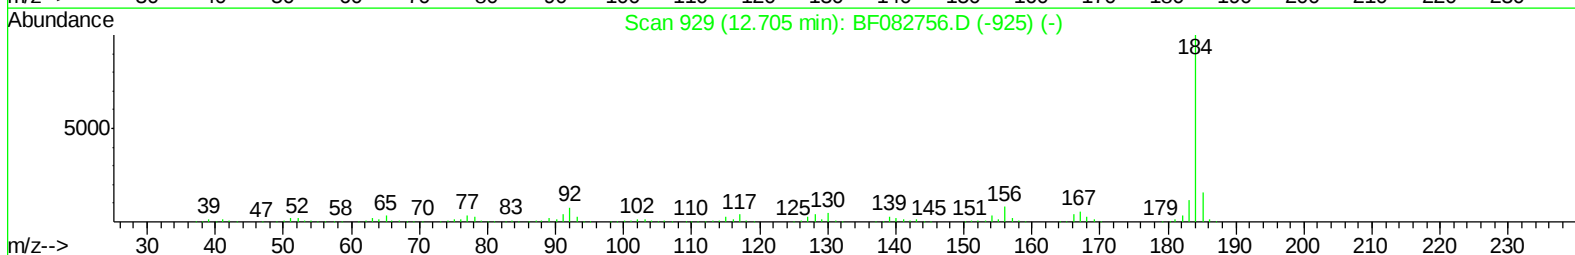
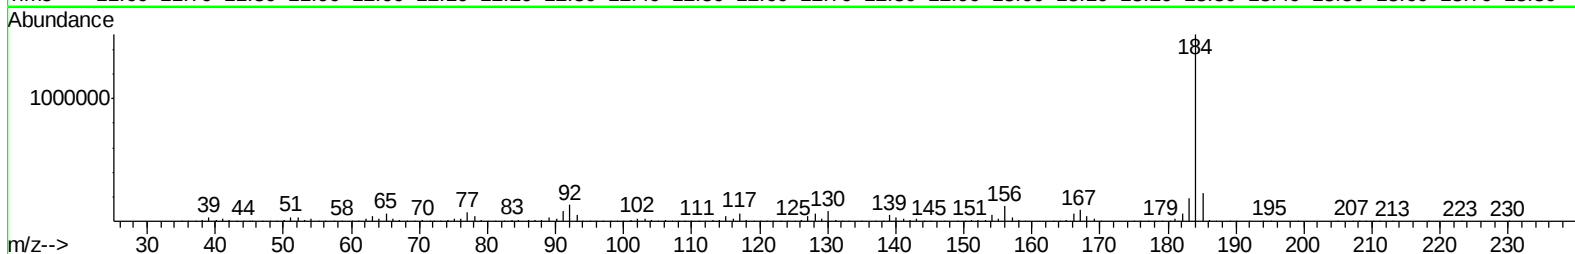


Data Path : Z:\HPCHEM1\BNA F\Data\BF111615\
Data File : BF082940.D
Acq On : 16 Nov 2015 13:22
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 08:10:01 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 17 04:41:30 2015
Response via : Initial Calibration

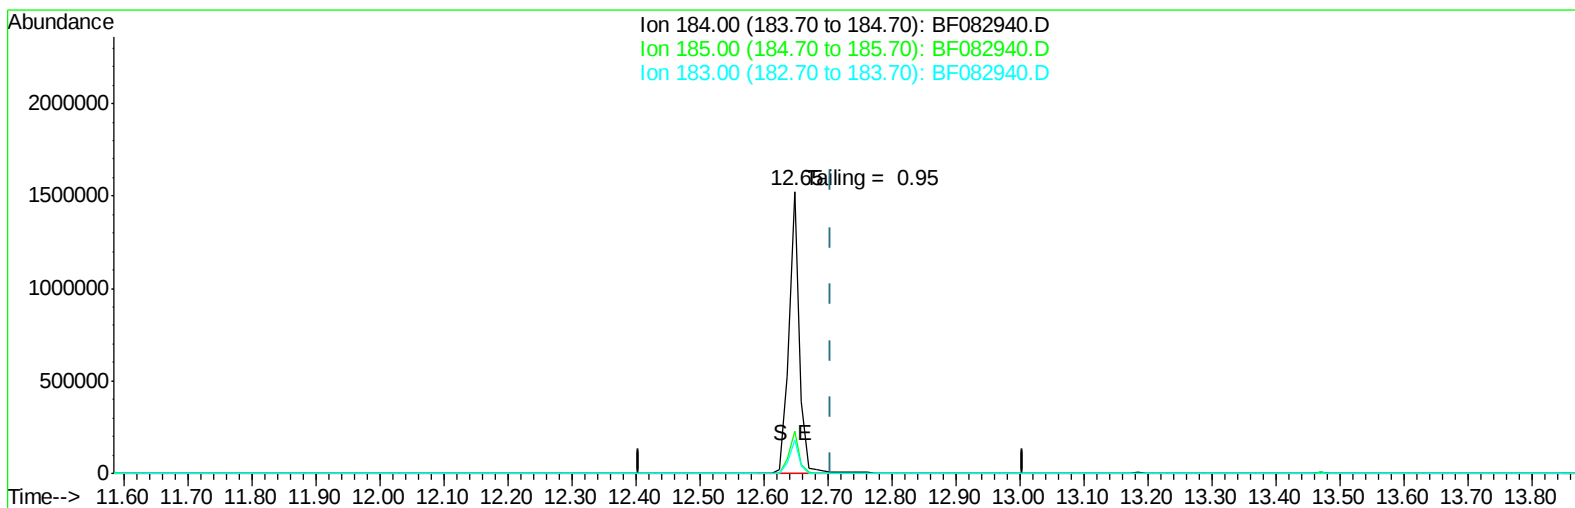

TIC: BF082940.D

(76) Benzidine

12.648min (-0.057) 4692.64ng

response 1766136

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	15.20
183.00	12.00	12.04
0.00	0.00	0.00