
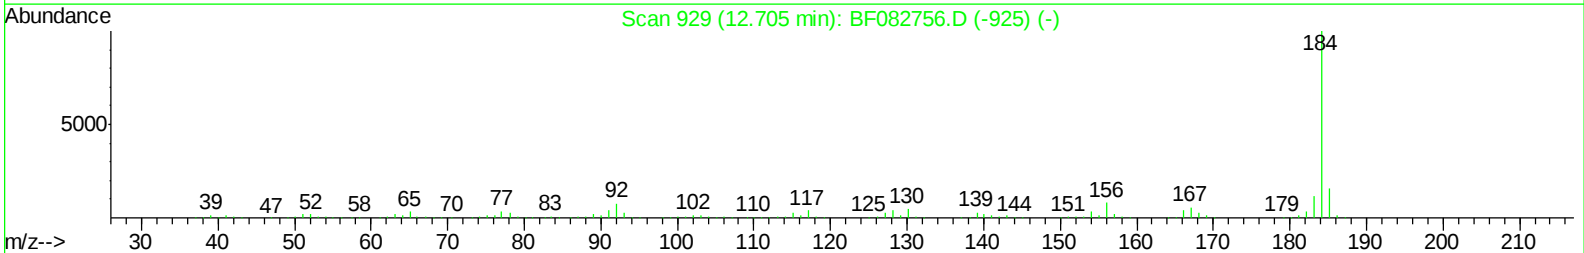
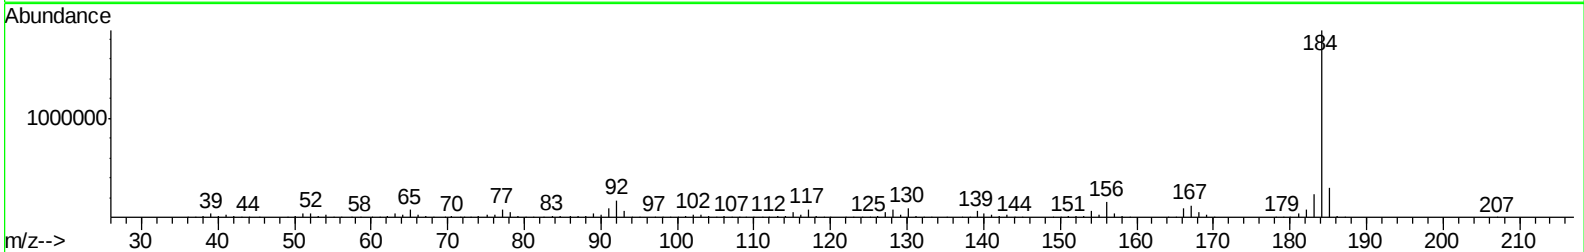


```
Data Path : Z:\HPCHEM1\BNA F\Data\BF111615\  
Data File : BF082958.D  
Acq On    : 17 Nov 2015  00:50  
Operator  : UM/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Nov 17 08:12:35 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 17 04:41:30 2015
Response via : Initial Calibration

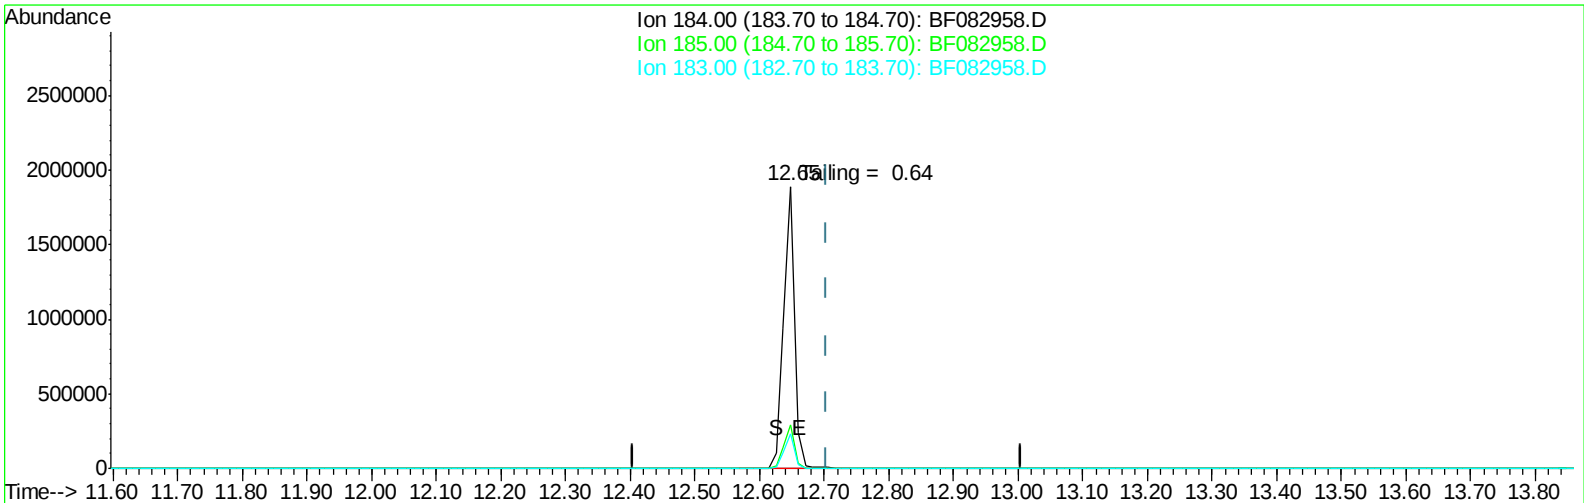

TIC: BF082958.D

(76) Benzidine

12.648min (-0.057) 0.00ng

response 2222859

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	15.53
183.00	12.00	12.36
0.00	0.00	0.00