

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
 Data File : BM003149.D
 Acq On : 16 Nov 2015 19:01
 Operator : UM/IZ
 Sample : G4309-25
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9KN5

Quant Time: Nov 17 00:21:12 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 17 00:18:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	105377	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	452619	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	248459	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.13	188	544199	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	587597	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	606072	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	13142	5.88	ng/uL	0.00
5) Phenol-d5	6.90	99	260608	31.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	151529	31.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	225908	32.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	217625	32.40	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	105429	38.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	112612	40.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	205107	32.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	311450	38.38	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	667262	35.70	ng/ul	0.00
47) Acenaphthylene-d8	14.09	160	807421	34.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	109395	34.72	ng/ul	0.00
58) Fluorene-d10	15.39	176	574039	35.52	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	78808	31.27	ng/ul	0.00
71) Anthracene-d10	17.23	188	868346	35.99	ng/ul	0.00
79) Pyrene-d10	19.53	212	965171	33.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.45	264	1074946	37.32	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.85	163	190873	10.02	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
Data File : BM003149.D
Acq On : 16 Nov 2015 19:01
Operator : UM/IZ
Sample : G4309-25
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9KN5

Quant Time: Nov 17 00:21:12 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 17 00:18:48 2015
Response via : Initial Calibration

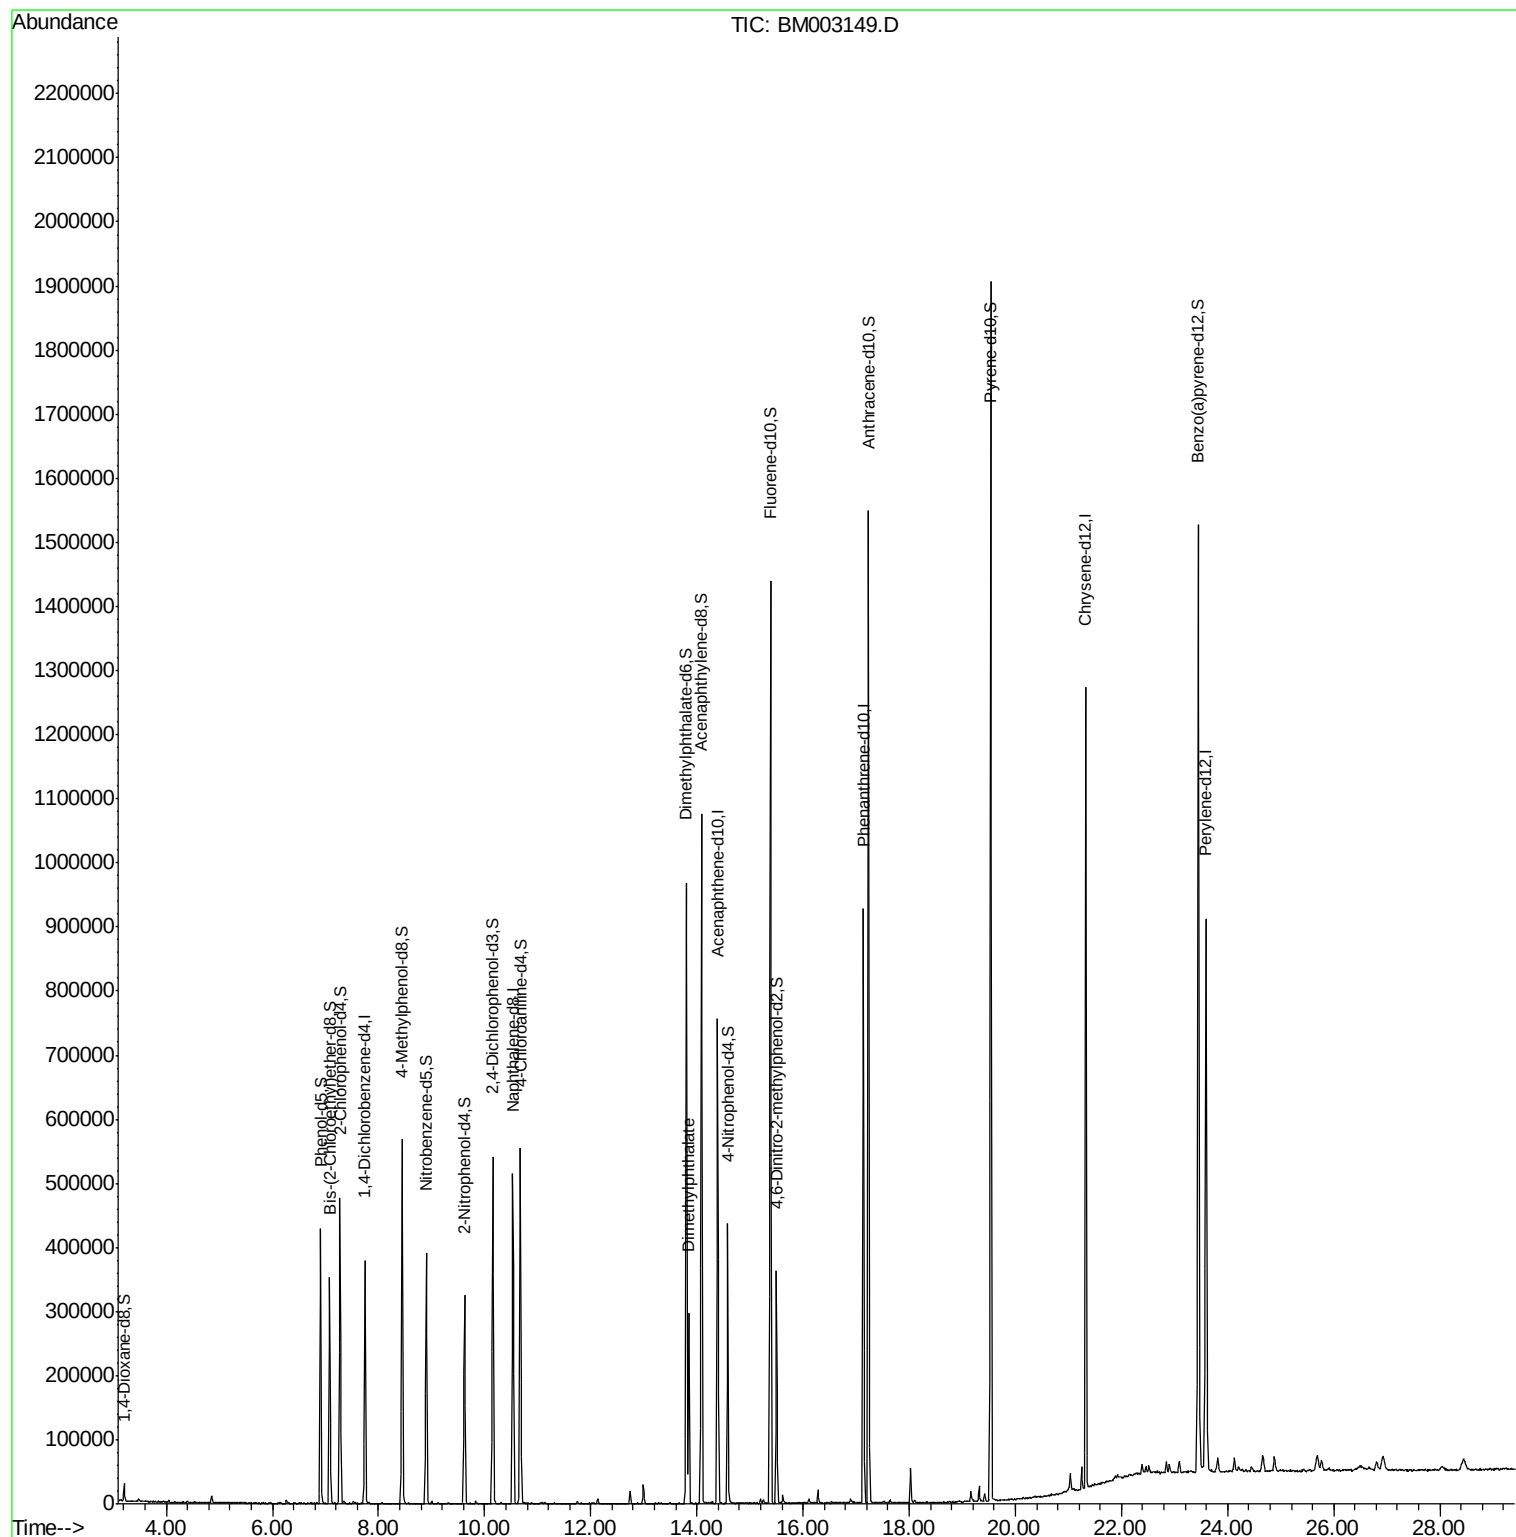

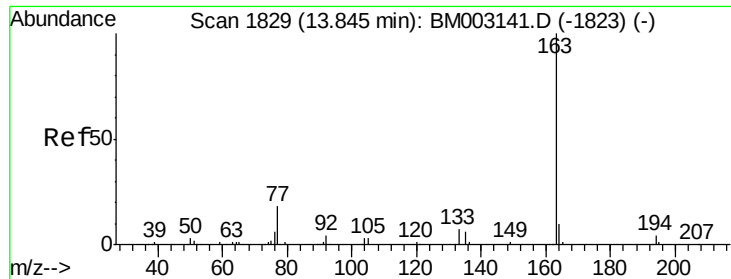

#45

Dimethylphthalate

Concen: 10.02 ng/ul

RT: 13.85 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM003149.D

Acq: 16 Nov 2015 19:01

Instrument :

BNA_M

ClientSampleId :

D9KN5



Tot Ion:163 Resp: 190873

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.3 7.8 11.8

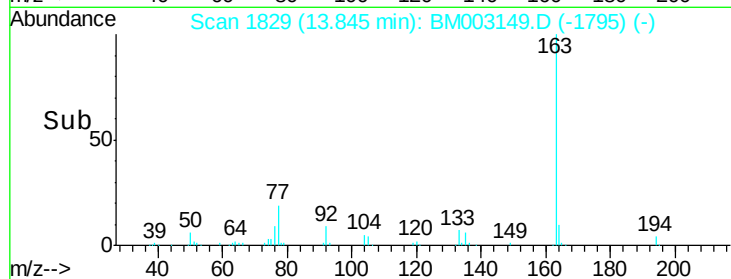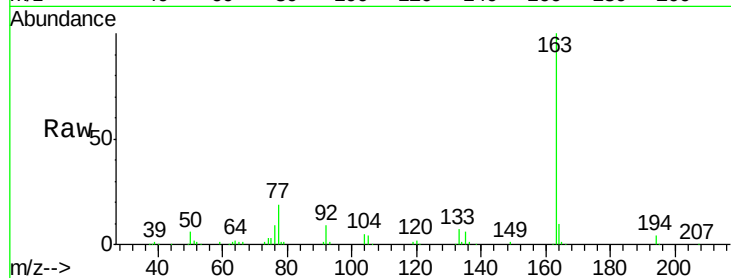

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

