

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\  
 Data File : BM003151.D  
 Acq On : 16 Nov 2015 20:13  
 Operator : UM/IZ  
 Sample : G4323-05  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :

Quant Time: Nov 17 00:21:25 2015  
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Nov 17 00:18:48 2015  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.75  | 152  | 134459   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.53 | 136  | 572170   | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.39 | 164  | 314777   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.13 | 188  | 709791   | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.33 | 240  | 790027   | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.59 | 264  | 783807   | 20.00 | ng/ul | 0.00     |

| System Monitoring Compounds    | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 3) 1,4-Dioxane-d8              | 3.20  | 96   | 11247    | 3.94  | ng/uL | 0.00     |
| 5) Phenol-d5                   | 6.90  | 99   | 206675   | 19.44 | ng/ul | 0.00     |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.07  | 67   | 121764   | 19.59 | ng/ul | 0.00     |
| 9) 2-Chlorophenol-d4           | 7.27  | 132  | 180697   | 20.06 | ng/ul | 0.00     |
| 13) 4-Methylphenol-d8          | 8.45  | 113  | 168958   | 19.71 | ng/ul | 0.00     |
| 19) Nitrobenzene-d5            | 8.90  | 128  | 80537    | 23.08 | ng/ul | 0.00     |
| 22) 2-Nitrophenol-d4           | 9.62  | 143  | 85358    | 24.15 | ng/ul | 0.00     |
| 26) 2,4-Dichlorophenol-d3      | 10.15 | 165  | 158096   | 19.94 | ng/ul | 0.00     |
| 29) 4-Chloroaniline-d4         | 10.67 | 131  | 205830   | 20.06 | ng/ul | 0.00     |
| 44) Dimethylphthalate-d6       | 13.80 | 166  | 508307   | 21.46 | ng/ul | 0.00     |
| 47) Acenaphthylene-d8          | 14.08 | 160  | 597424   | 19.91 | ng/ul | 0.00     |
| 52) 4-Nitrophenol-d4           | 14.58 | 143  | 78432    | 19.65 | ng/ul | 0.00     |
| 58) Fluorene-d10               | 15.39 | 176  | 424644   | 20.74 | ng/ul | 0.00     |
| 63) 4,6-Dinitro-2-methylphenol | 15.50 | 200  | 55144    | 16.78 | ng/ul | 0.00     |
| 71) Anthracene-d10             | 17.23 | 188  | 651876   | 20.72 | ng/ul | 0.00     |
| 79) Pyrene-d10                 | 19.53 | 212  | 725381   | 18.65 | ng/ul | 0.00     |
| 90) Benzo(a)pyrene-d12         | 23.44 | 264  | 751336   | 20.17 | ng/ul | 0.00     |


| Target Compounds      | R.T.  | QIon | Response | Conc  | Units | Ovalue |
|-----------------------|-------|------|----------|-------|-------|--------|
| 45) Dimethylphthalate | 13.85 | 163  | 267872   | 11.10 | ng/ul | 99     |




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\  
Data File : BM003151.D  
Acq On : 16 Nov 2015 20:13  
Operator : UM/IZ  
Sample : G4323-05  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :

Quant Time: Nov 17 00:21:25 2015  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Nov 17 00:18:48 2015  
Response via : Initial Calibration

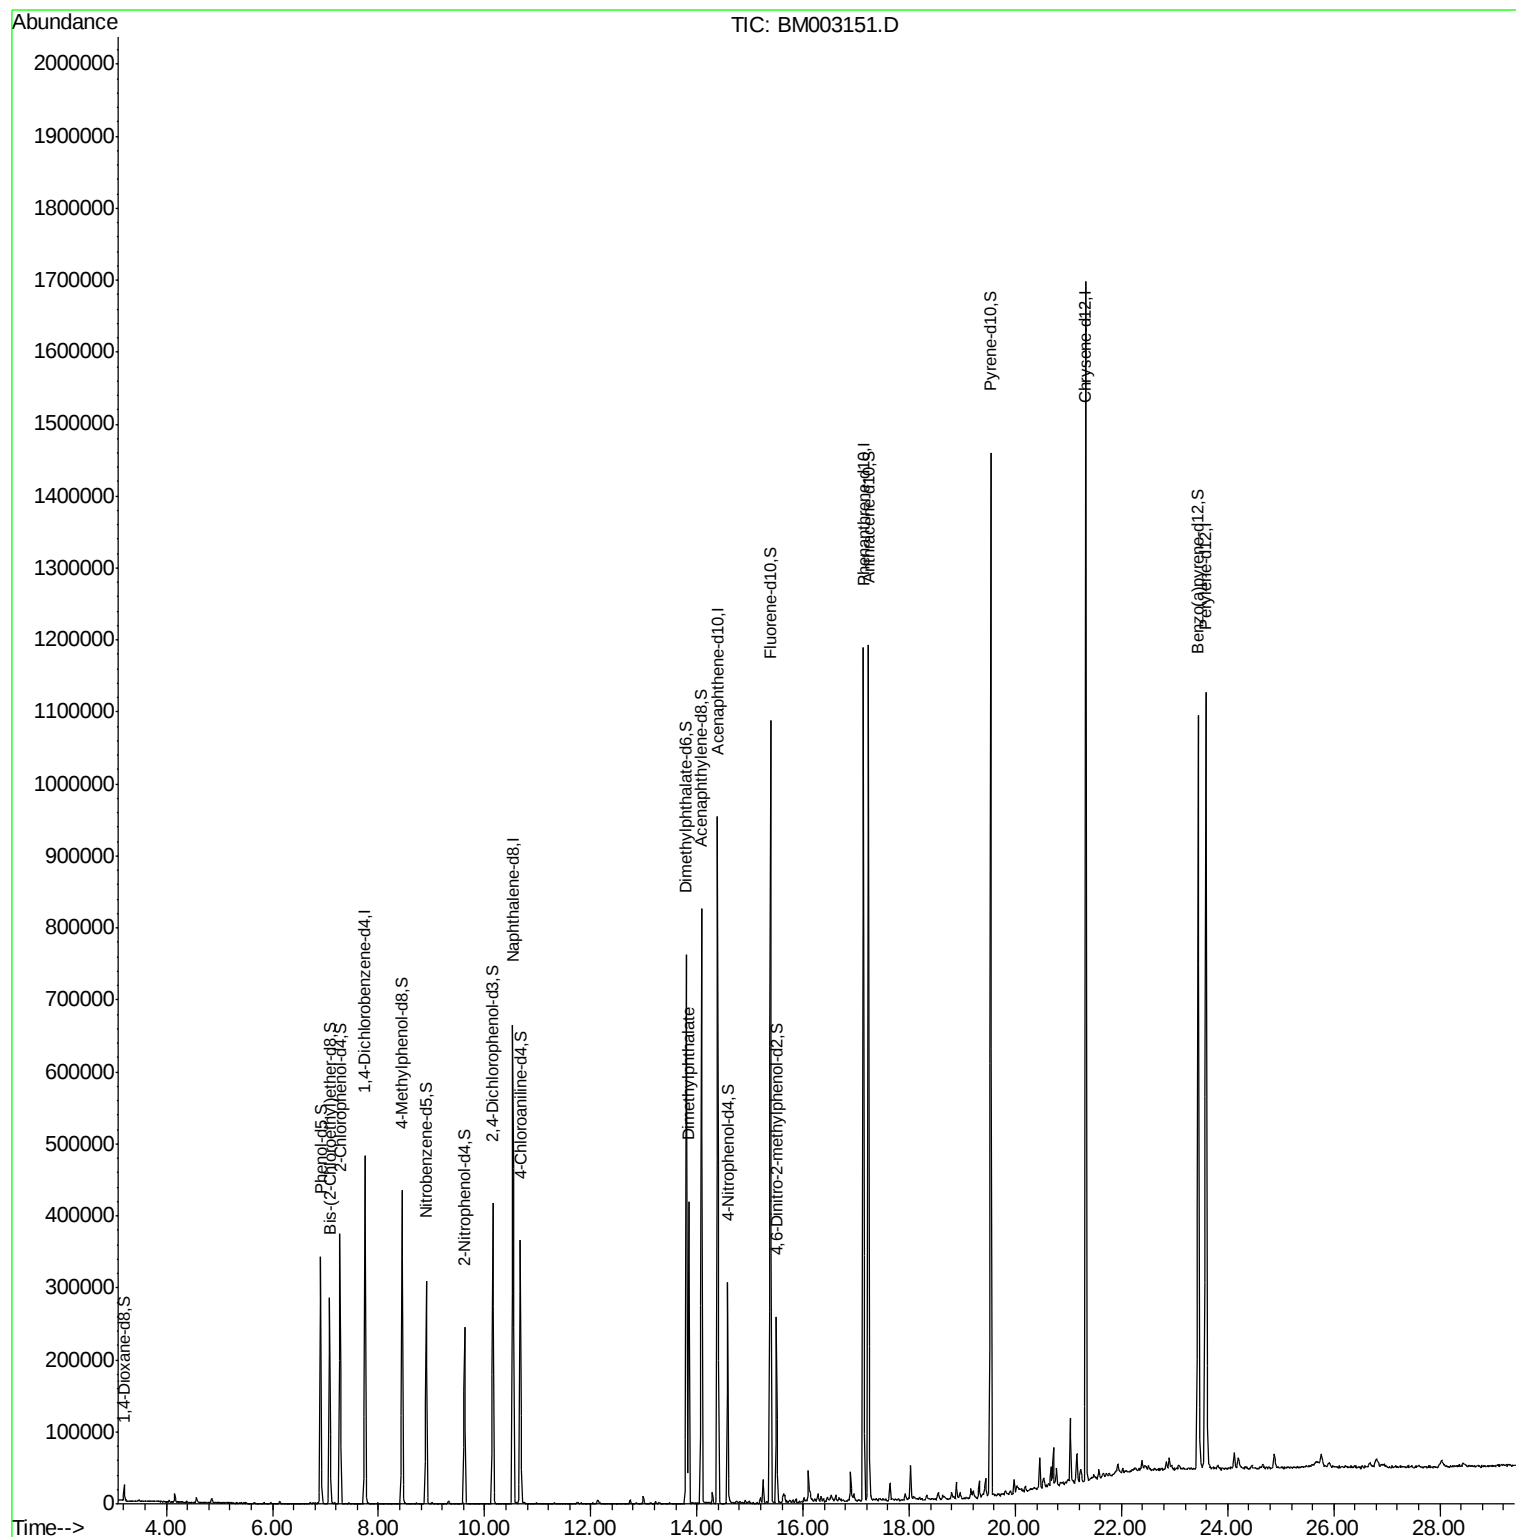

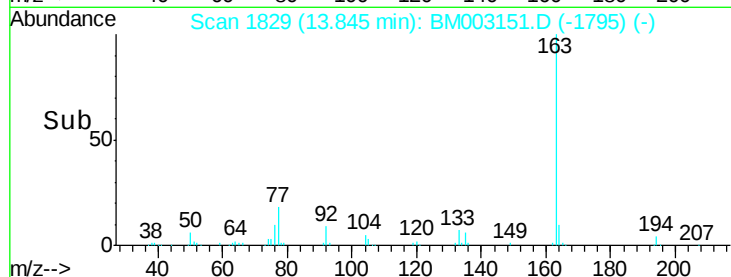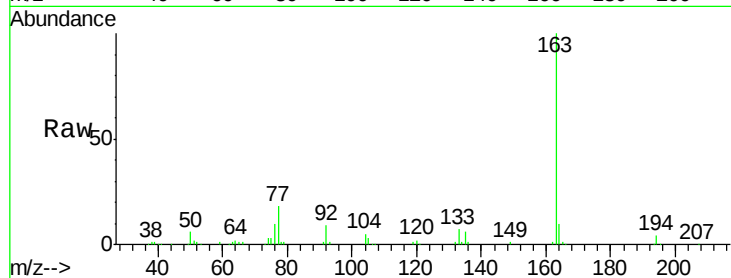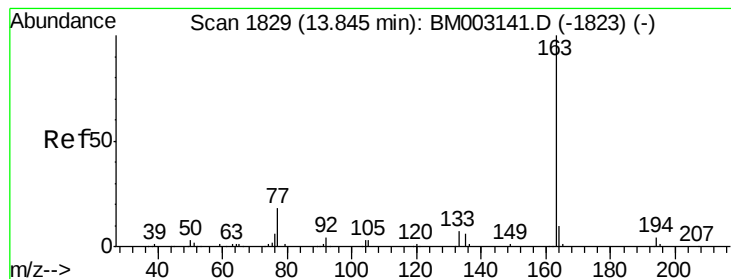

#45

Dimethylphthalate

Concen: 11.10 ng/ul

RT: 13.85 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM003151.D

Acq: 16 Nov 2015 20:13

Instrument :

BNA\_M

ClientSampleId :

Tot Ion:163 Resp: 267872

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.2 7.8 11.8

